


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY120623\
Data File : VY016606.D
Acq On : 06 Dec 2023 08:46
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y120423S.M
Title : SW846 8260
Last Update : Tue Dec 05 01:24:25 2023

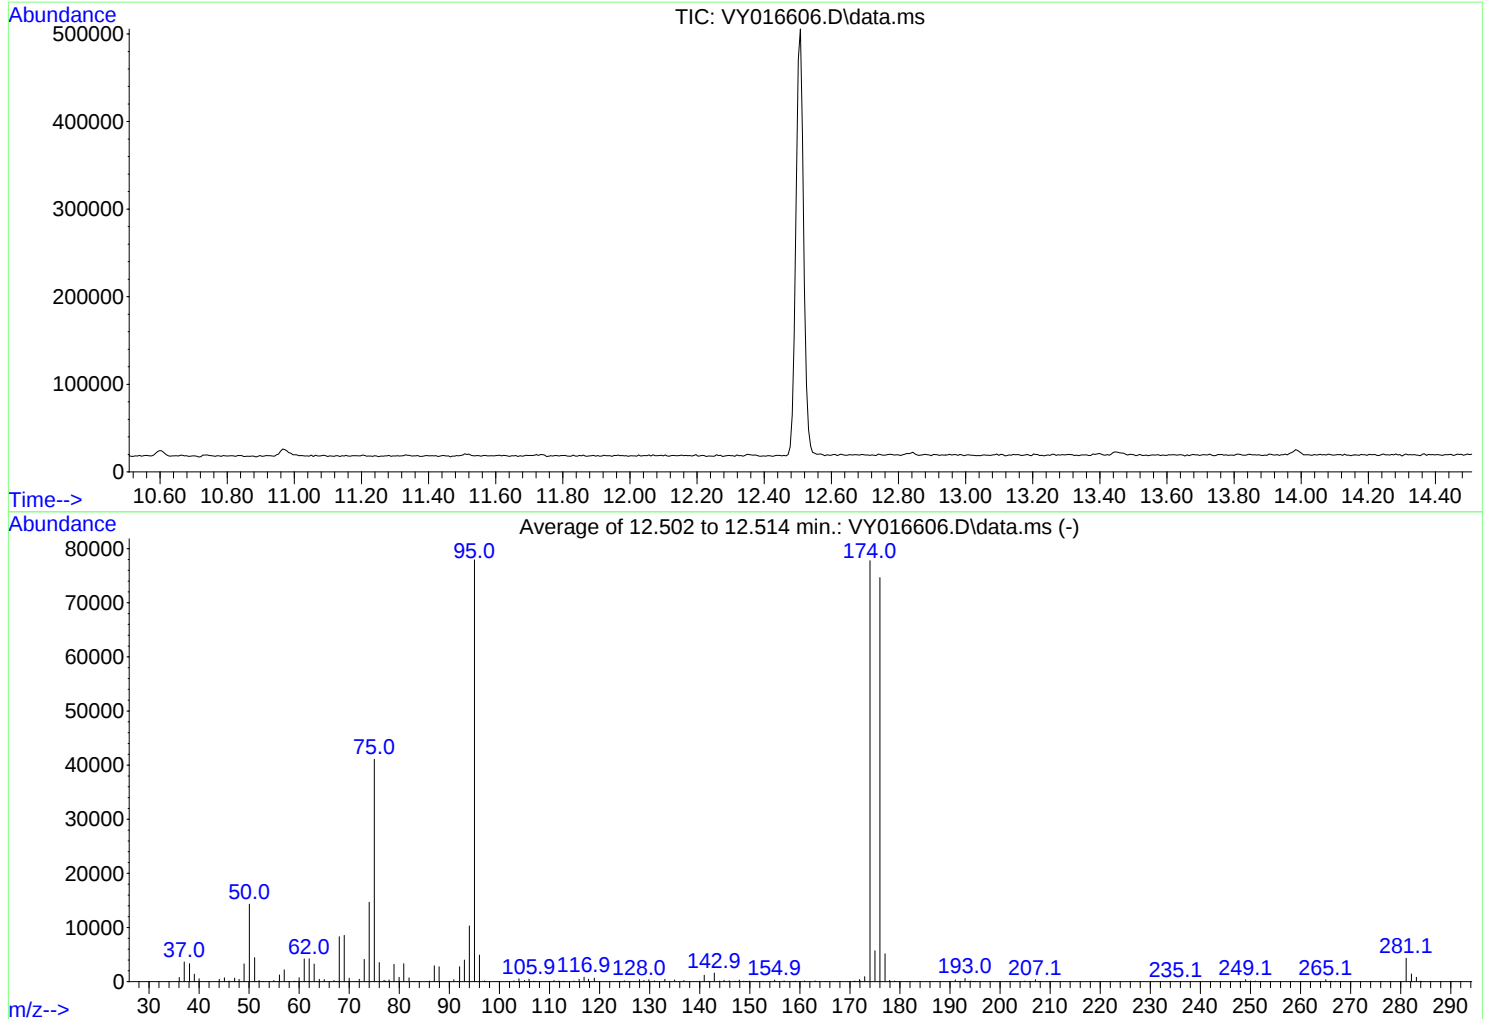

AutoFind: Scans 1752, 1753, 1754; Background Corrected with Scan 1744

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.4	14313	PASS
75	95	30	60	52.7	41083	PASS
95	95	100	100	100.0	77931	PASS
96	95	5	9	6.3	4906	PASS
173	174	0.00	2	1.2	929	PASS
174	95	50	100	99.8	77773	PASS
175	174	5	9	7.3	5705	PASS
176	174	95	101	96.0	74661	PASS
177	176	5	9	6.9	5134	PASS