
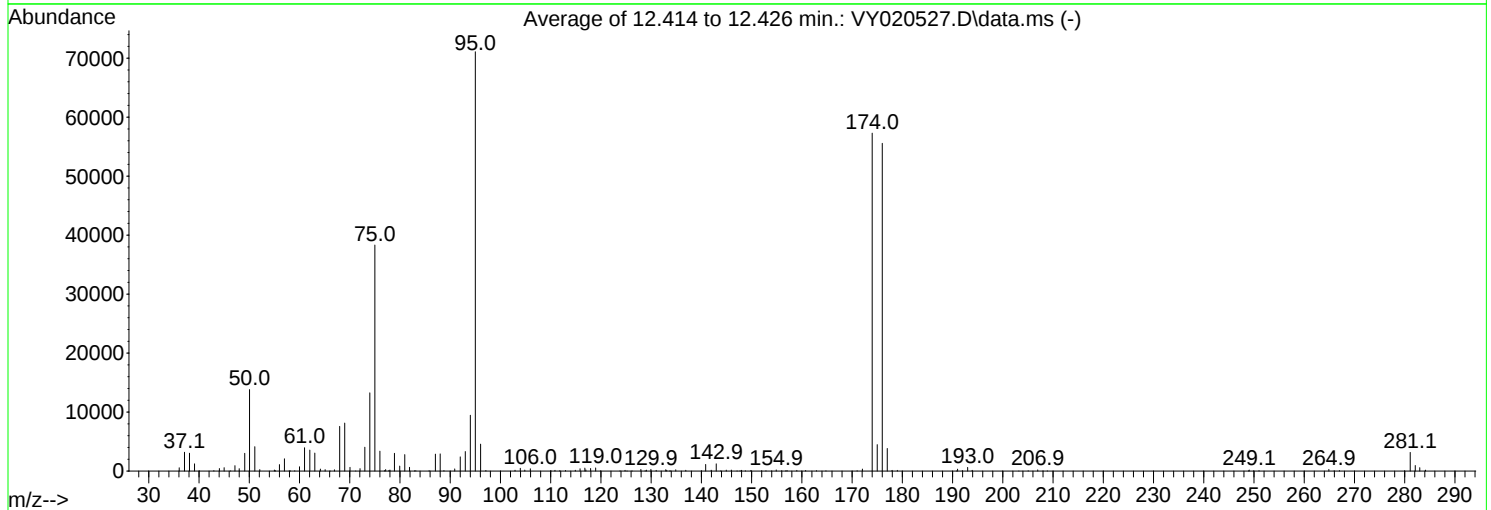


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY120624\
Data File : VY020527.D
Acq On : 06 Dec 2024 09:07
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y120224S.M
Title : SW846 8260
Last Update : Tue Dec 03 01:39:23 2024

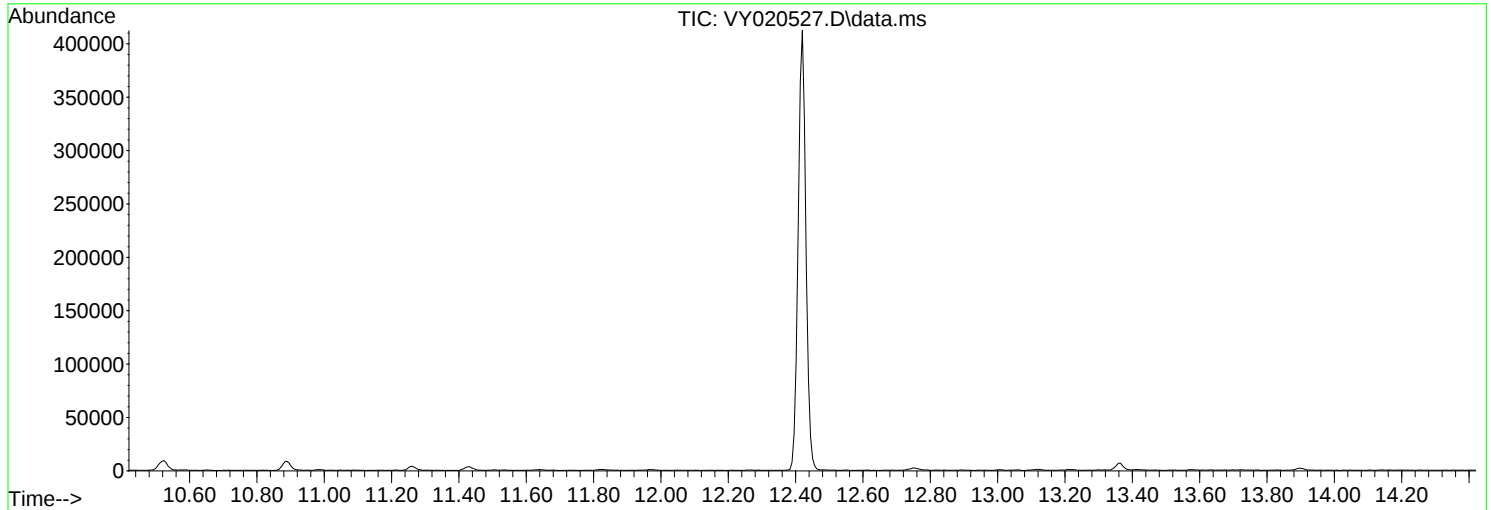

AutoFind: Scans 1754, 1755, 1756; Background Corrected with Scan 1746

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.4	13822	PASS
75	95	30	60	53.9	38320	PASS
95	95	100	100	100.0	71093	PASS
96	95	5	9	6.4	4566	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	80.6	57293	PASS
175	174	5	9	7.8	4489	PASS
176	174	95	101	97.0	55568	PASS
177	176	5	9	6.9	3839	PASS