

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY120721\
 Data File : VY007001.D
 Acq On : 07 Dec 2021 17:05
 Operator : SY/MD
 Sample : M4887-01
 Misc : 5.08g/10.0mL/MSVOA_Y/SOIL
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :

Quant Time: Dec 08 02:57:23 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\SFAMYLEM120721SMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Dec 08 02:54:31 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.691	114	150825	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.490	117	159035	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.428	152	73390	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.253	65	48286	14.241	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	56.960%
7) Chloroethane-d5	2.766	69	39033	15.056	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	60.240%
11) 1,1-Dichloroethene-d2	3.851	63	56789	10.854	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	43.400%#
21) 2-Butanone-d5	6.887	46	41938	42.700	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	85.400%
24) Chloroform-d	7.478	84	83216	17.401	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	69.600%
26) 1,2-Dichloroethane-d4	8.143	65	52321	18.277	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	73.120%
32) Benzene-d6	8.112	84	152299	14.650	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	58.600%
36) 1,2-Dichloropropane-d6	9.124	67	56641	16.159	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	64.640%#
41) Toluene-d8	10.185	98	154170	16.066	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	64.280%
43) trans-1,3-Dichloroprop...	10.441	79	29728	18.324	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	73.280%
47) 2-Hexanone-d5	10.788	63	33101	41.090	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	82.180%
56) 1,1,2,2-Tetrachloroeth...	12.563	84	56680	18.891	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	75.560%
66) 1,2-Dichlorobenzene-d4	13.727	152	52524	18.616	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	74.480%#
Target Compounds						
					Qvalue	
13) Acetone	3.948	43	2657	3.132	ug/L	97
27) 1,2-Dichloroethane	8.246	62	2356	0.697	ug/L	96
34) Trichloroethene	8.947	95	3576	1.255	ug/L	87
46) Tetrachloroethene	10.727	164	1745	0.797	ug/L	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY120721\
Data File : VY007001.D
Acq On : 07 Dec 2021 17:05
Operator : SY/MD
Sample : M4887-01
Misc : 5.08g/10.0mL/MSVOA_Y/SOIL
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :

Quant Time: Dec 08 02:57:23 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\SFAMYL120721SMA.M
Quant Title : VOC Analysis
QLast Update : Wed Dec 08 02:54:31 2021
Response via : Initial Calibration




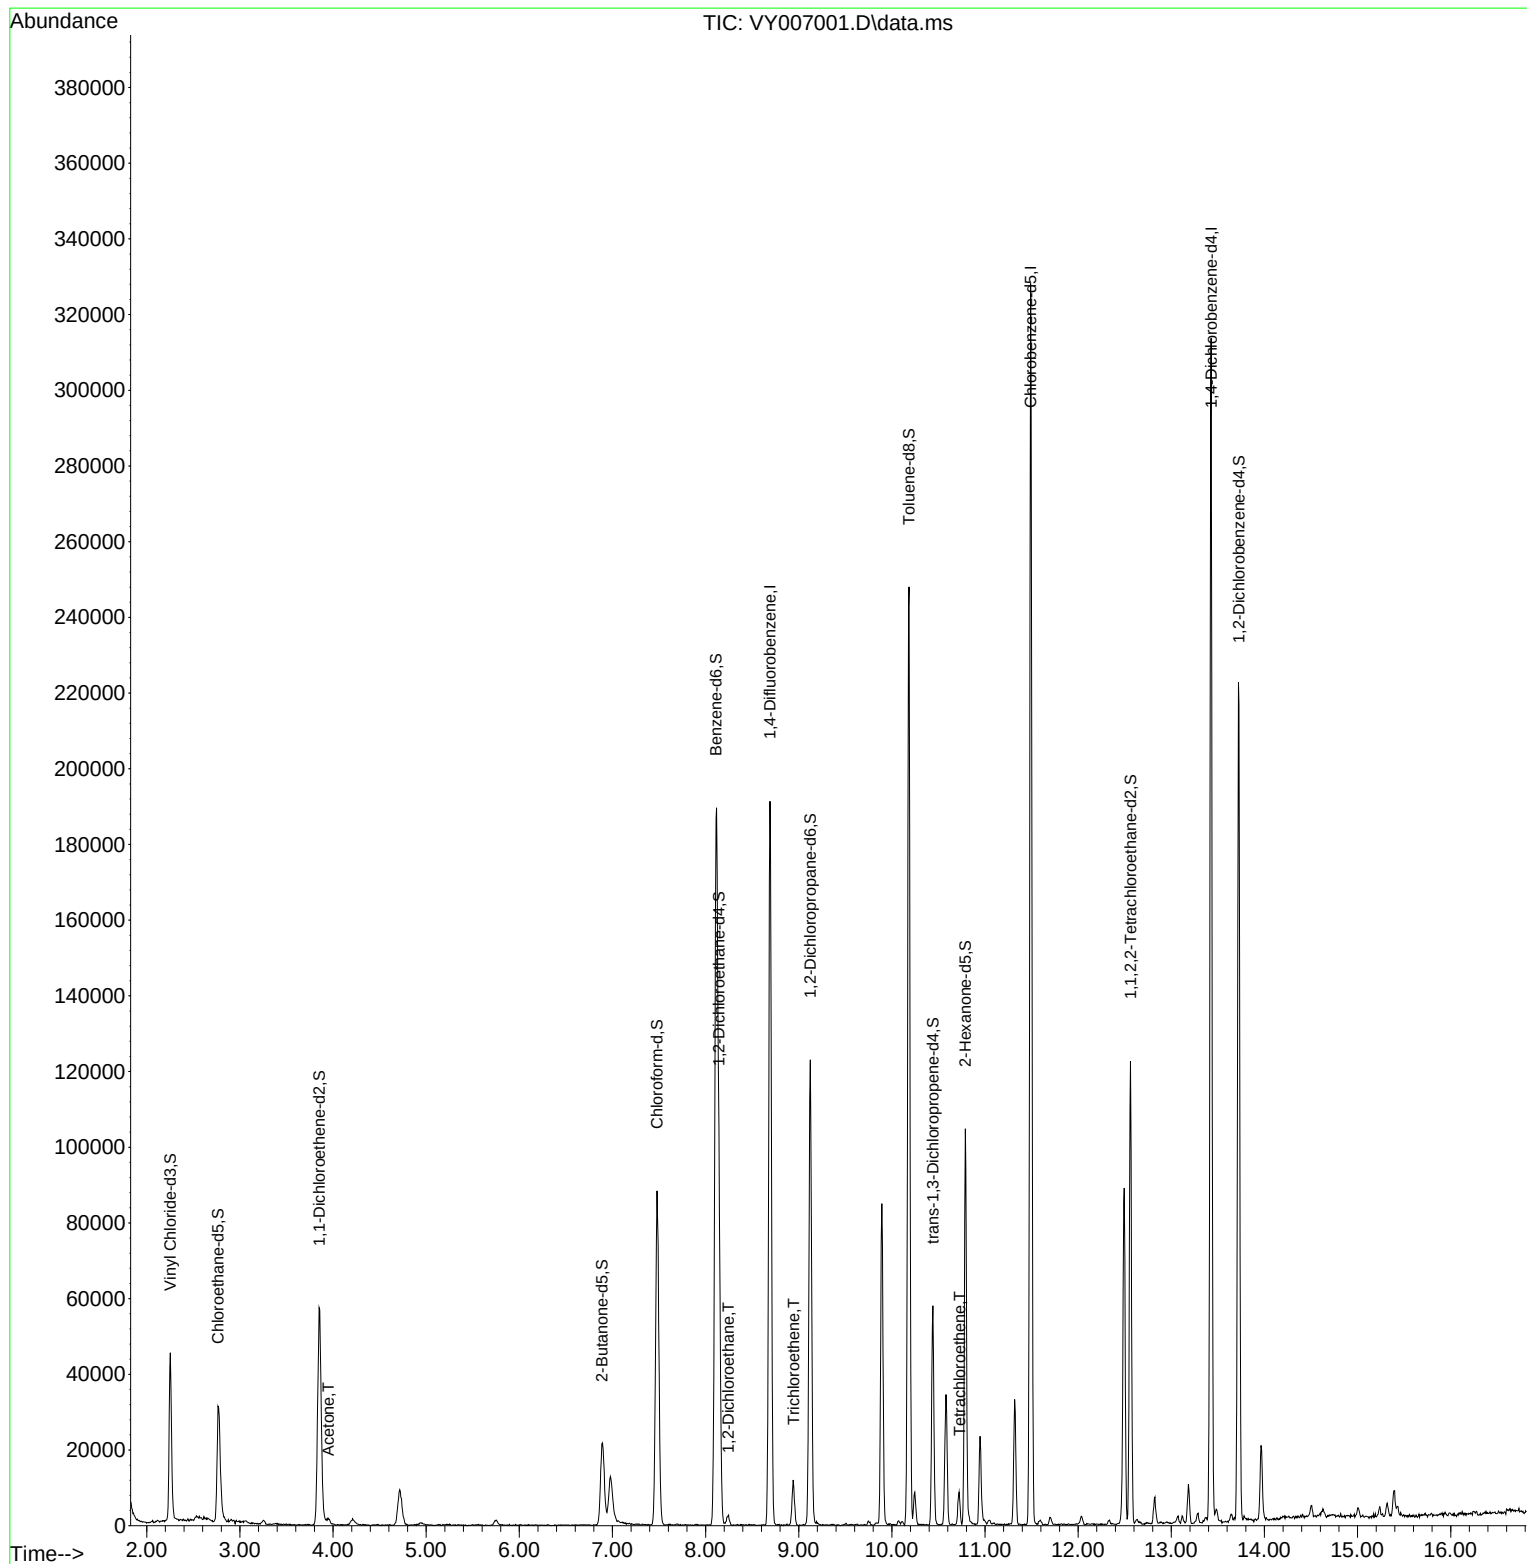


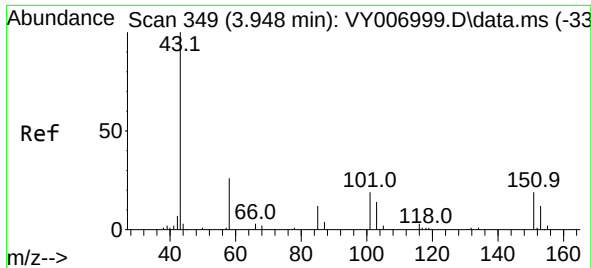

#13
Acetone
Concen: 3.132 ug/L
RT: 3.948 min Scan# 349
Delta R.T. 0.000 min
Lab File: VY007001.D
Acq: 07 Dec 2021 17:05




Instrument :
MSVOA_Y
ClientSampleId :


Tgt Ion: 43 Resp: 2657
Ion Ratio Lower Upper
43 100
58 29.7 0.0 56.4

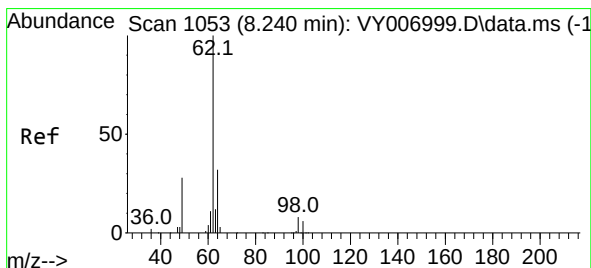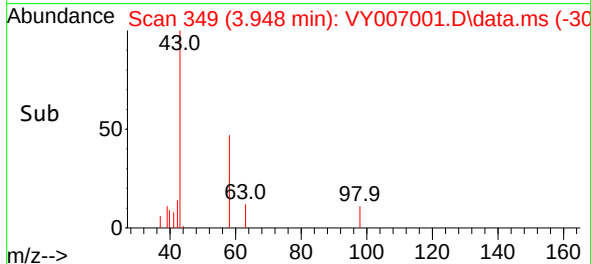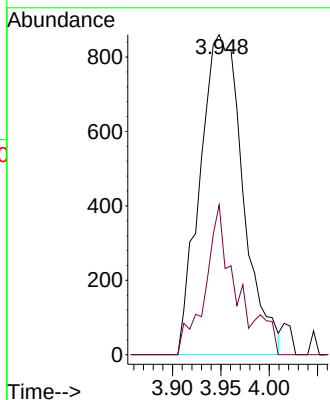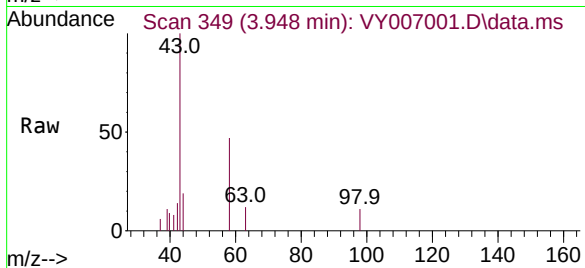

#27
1,2-Dichloroethane
Concen: 0.697 ug/L
RT: 8.246 min Scan# 1054
Delta R.T. 0.006 min
Lab File: VY007001.D
Acq: 07 Dec 2021 17:05

Tgt Ion: 62 Resp: 2356
Ion Ratio Lower Upper
62 100
98 9.6 6.6 9.8


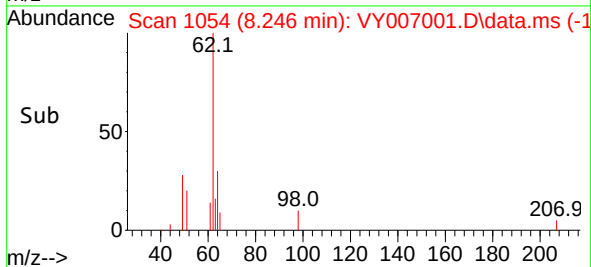
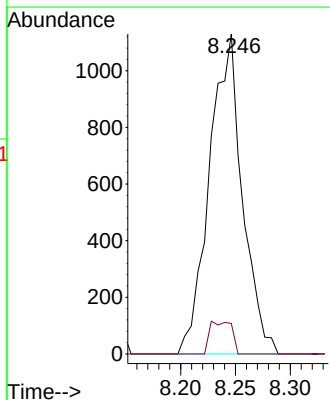
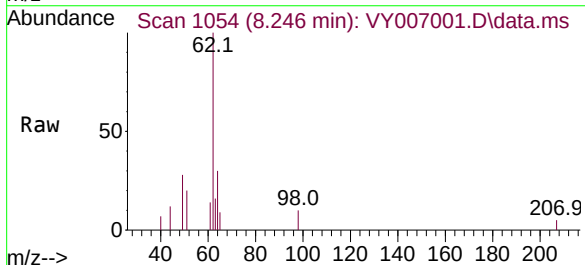


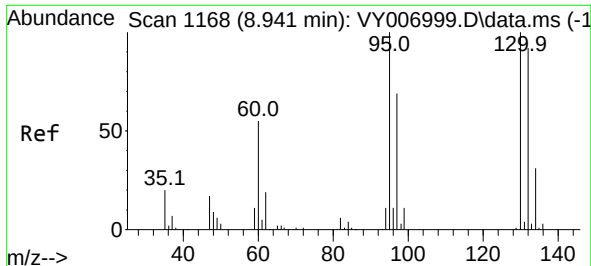

#34
Trichloroethene
Concen: 1.255 ug/L
RT: 8.947 min Scan# 1168
Delta R.T. 0.006 min
Lab File: VY007001.D
Acq: 07 Dec 2021 17:05

Instrument :
MSVOA_Y
ClientSampleId :

Tgt Ion: 95 Resp: 3576
Ion Ratio Lower Upper
95 100
97 63.7 46.4 86.2
132 82.3 63.0 117.0
130 72.0 66.7 123.9

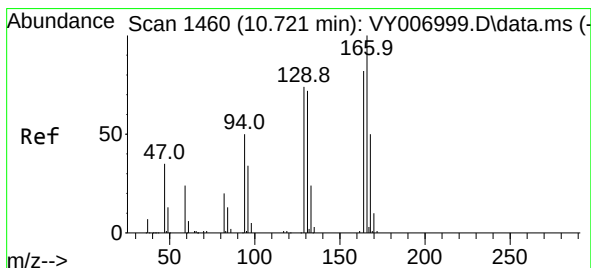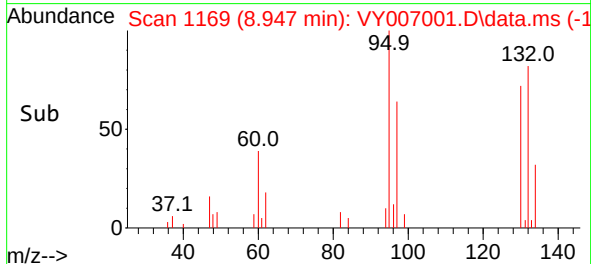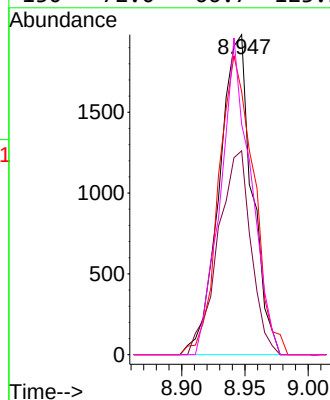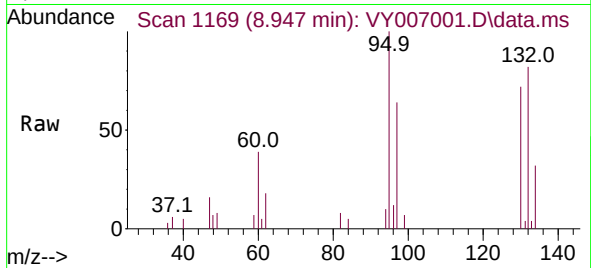

#46
Tetrachloroethene
Concen: 0.797 ug/L
RT: 10.727 min Scan# 1461
Delta R.T. 0.006 min
Lab File: VY007001.D
Acq: 07 Dec 2021 17:05

Tgt Ion:164 Resp: 1745
Ion Ratio Lower Upper
164 100
129 79.3 64.0 118.8
131 82.3 60.5 112.5
166 100.7 89.2 165.8

