
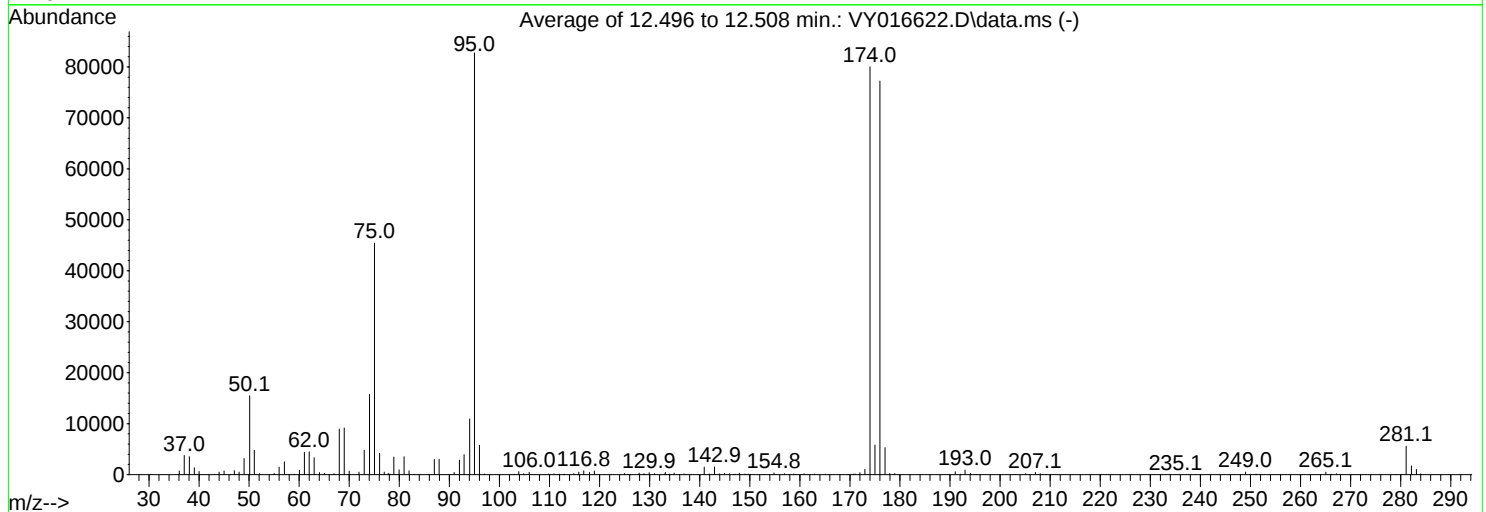


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY120723\
Data File : VY016622.D
Acq On : 07 Dec 2023 11:19
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y120423S.M
Title : SW846 8260
Last Update : Fri Dec 08 15:03:57 2023

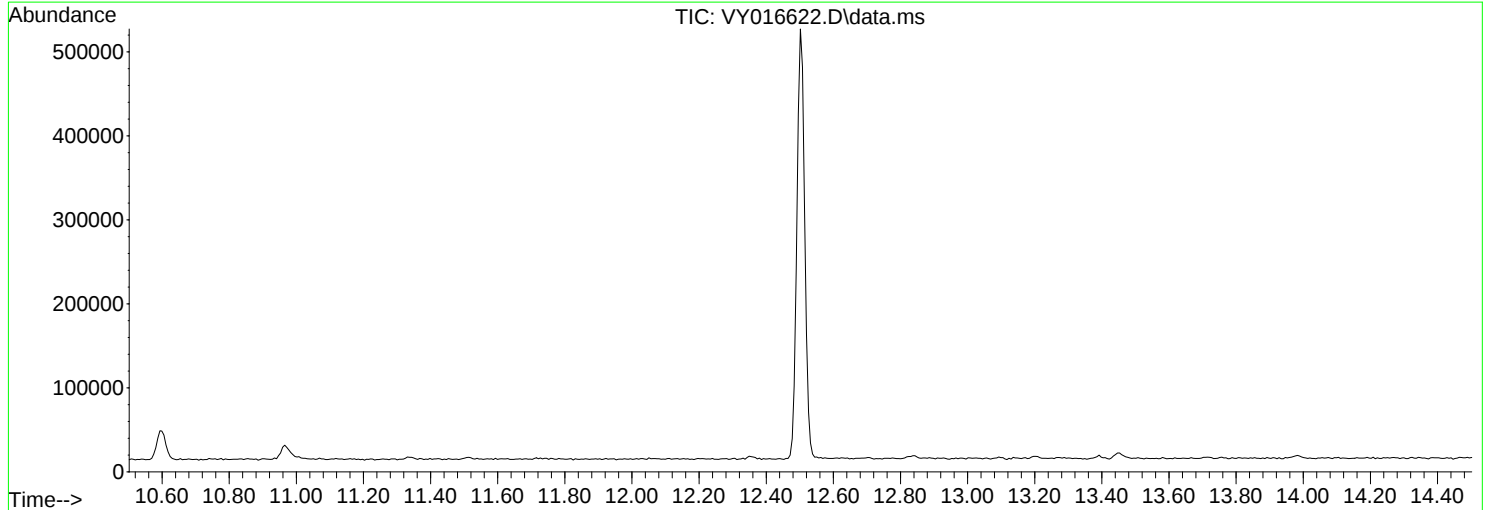

AutoFind: Scans 1751, 1752, 1753; Background Corrected with Scan 1743

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.7	15478	PASS
75	95	30	60	54.9	45432	PASS
95	95	100	100	100.0	82763	PASS
96	95	5	9	6.9	5741	PASS
173	174	0.00	2	1.3	1040	PASS
174	95	50	100	96.7	80013	PASS
175	174	5	9	7.3	5818	PASS
176	174	95	101	96.5	77227	PASS
177	176	5	9	6.9	5304	PASS