

Quantitation Report (Qedit)


Data Path : Z:\VOASRV\HPCHEM1\MSVOA Y\DATA\VY120820\
 Data File : VY003681.D
 Acq On : 08 Dec 2020 17:29
 Operator : SY/MD
 Sample : L4979-06
 Misc : 5.00G/10ML/MSVOA Y/SOIL
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 GB1F8

Manual Integrations
 APPROVED

MMDadoda
 12/10/2020 9:59:29 AM

Quant Time: Dec 09 02:00:31 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\SOM2YLM120420S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Dec 09 01:58:23 2020
 Response via : Initial Calibration

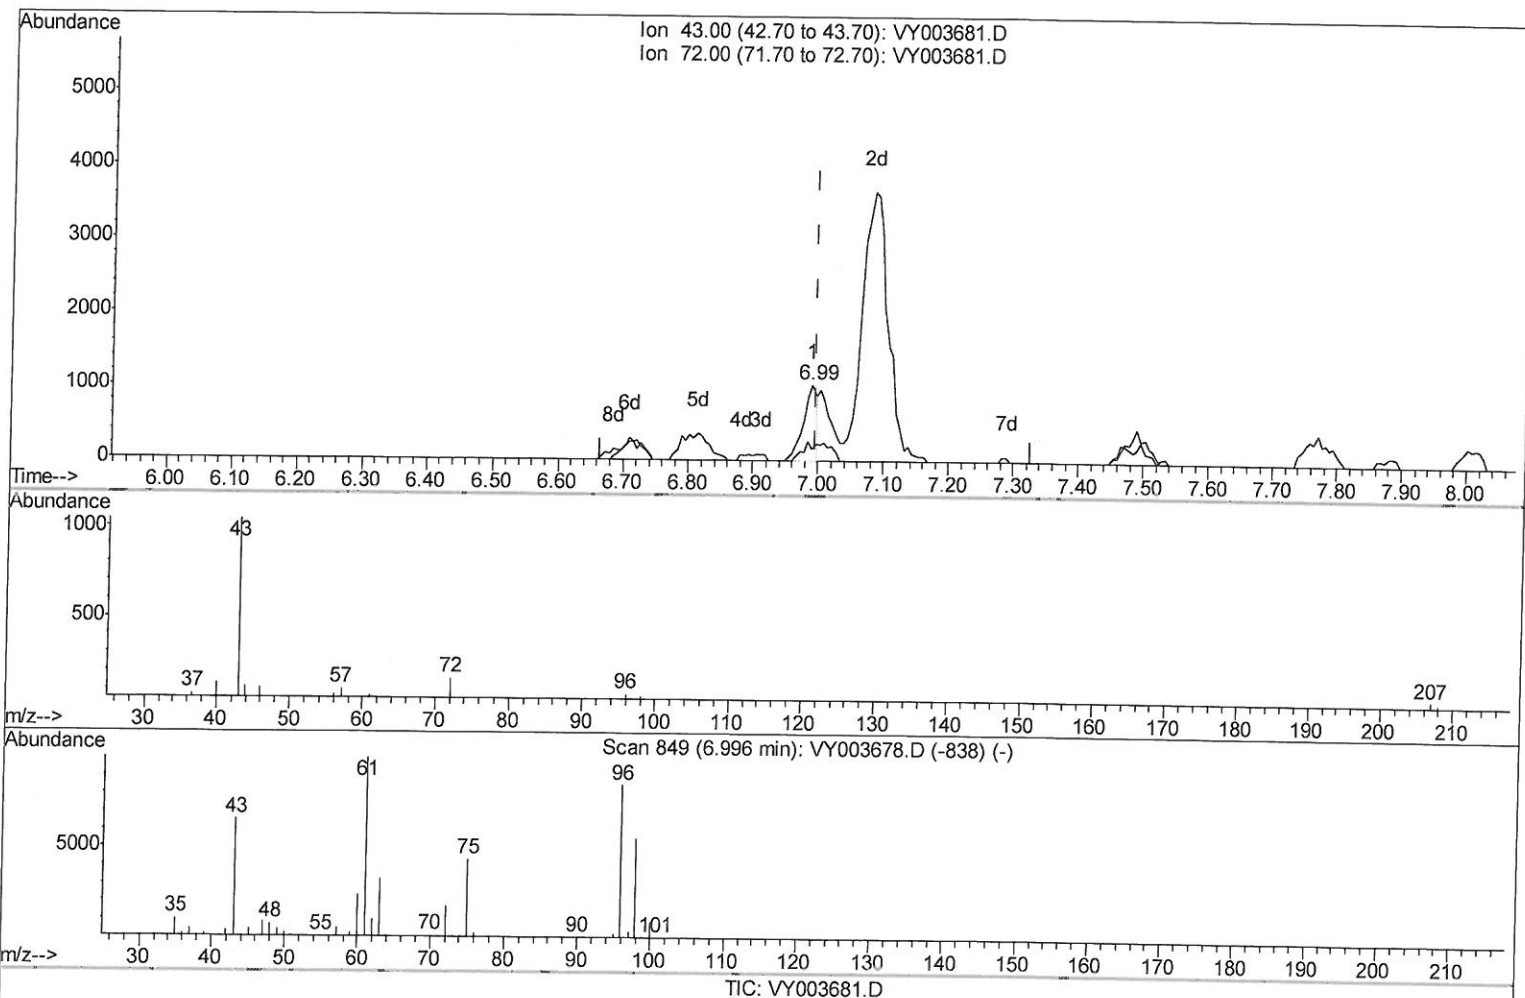

(21) 2-Butanone

6.990min (-0.006) 0.96ug/L

response 1494

Ion	Exp%	Act%
43.00	100	100
72.00	26.60	17.87
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\VOASRV\HPCHEM1\MSVOA Y\DATA\VY120820\
Data File : VY003681.D
Acq On : 08 Dec 2020 17:29
Operator : SY/MD
Sample : L4979-06
Misc : 5.00G/10ML/MSVOA Y/SOIL
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
GB1F8

Manual Integrations
APPROVED

MMDadoda
12/10/2020 9:59:29 AM

Quant Time: Dec 09 02:00:31 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\SOM2YLM120420S.M
Quant Title : VOC Analysis
QLast Update : Wed Dec 09 01:58:23 2020
Response via : Initial Calibration

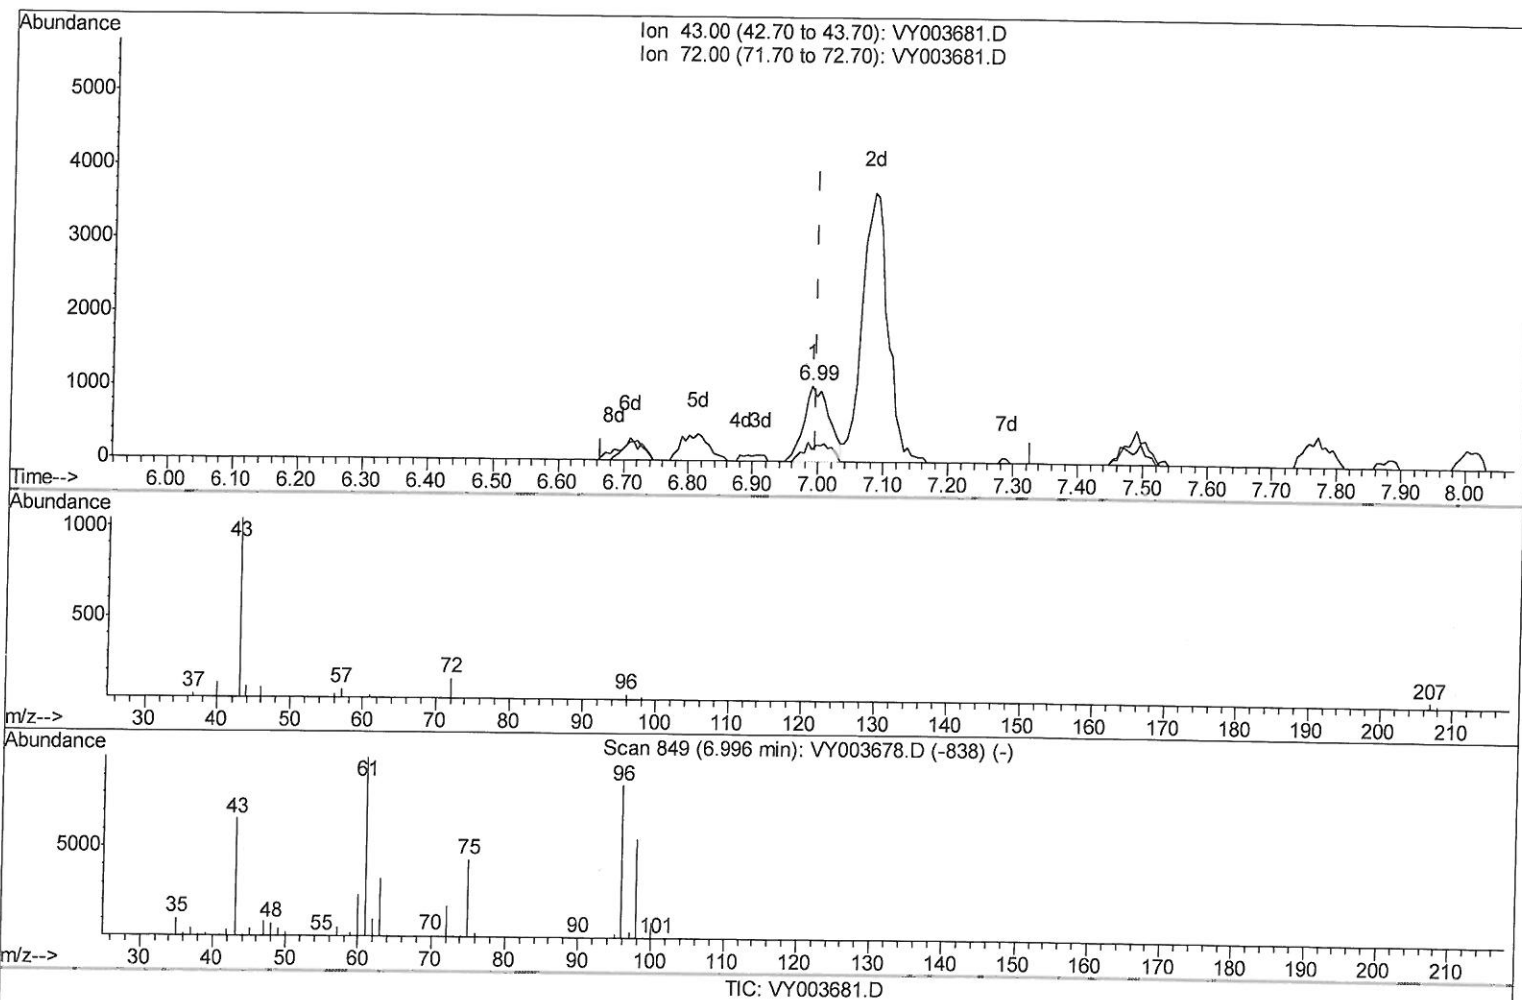

(21) 2-Butanone

6.990min (-0.006) 1.79ug/L m

response 2795

Ion	Exp%	Act%
43.00	100	100
72.00	26.60	9.55#
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\VOASRV\HPCHEM1\MSVOA Y\DATA\VY120820\
Data File : VY003681.D
Acq On : 08 Dec 2020 17:29
Operator : SY/MD
Sample : L4979-06
Misc : 5.00G/10ML/MSVOA Y/SOIL
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
GB1F8

Manual Integrations
APPROVED

MMDadoda
12/10/2020 9:59:29 AM

Quant Time: Dec 09 02:40:10 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\SOM2YLM120420S.M
Quant Title : VOC Analysis
QLast Update : Wed Dec 09 01:58:23 2020
Response via : Initial Calibration

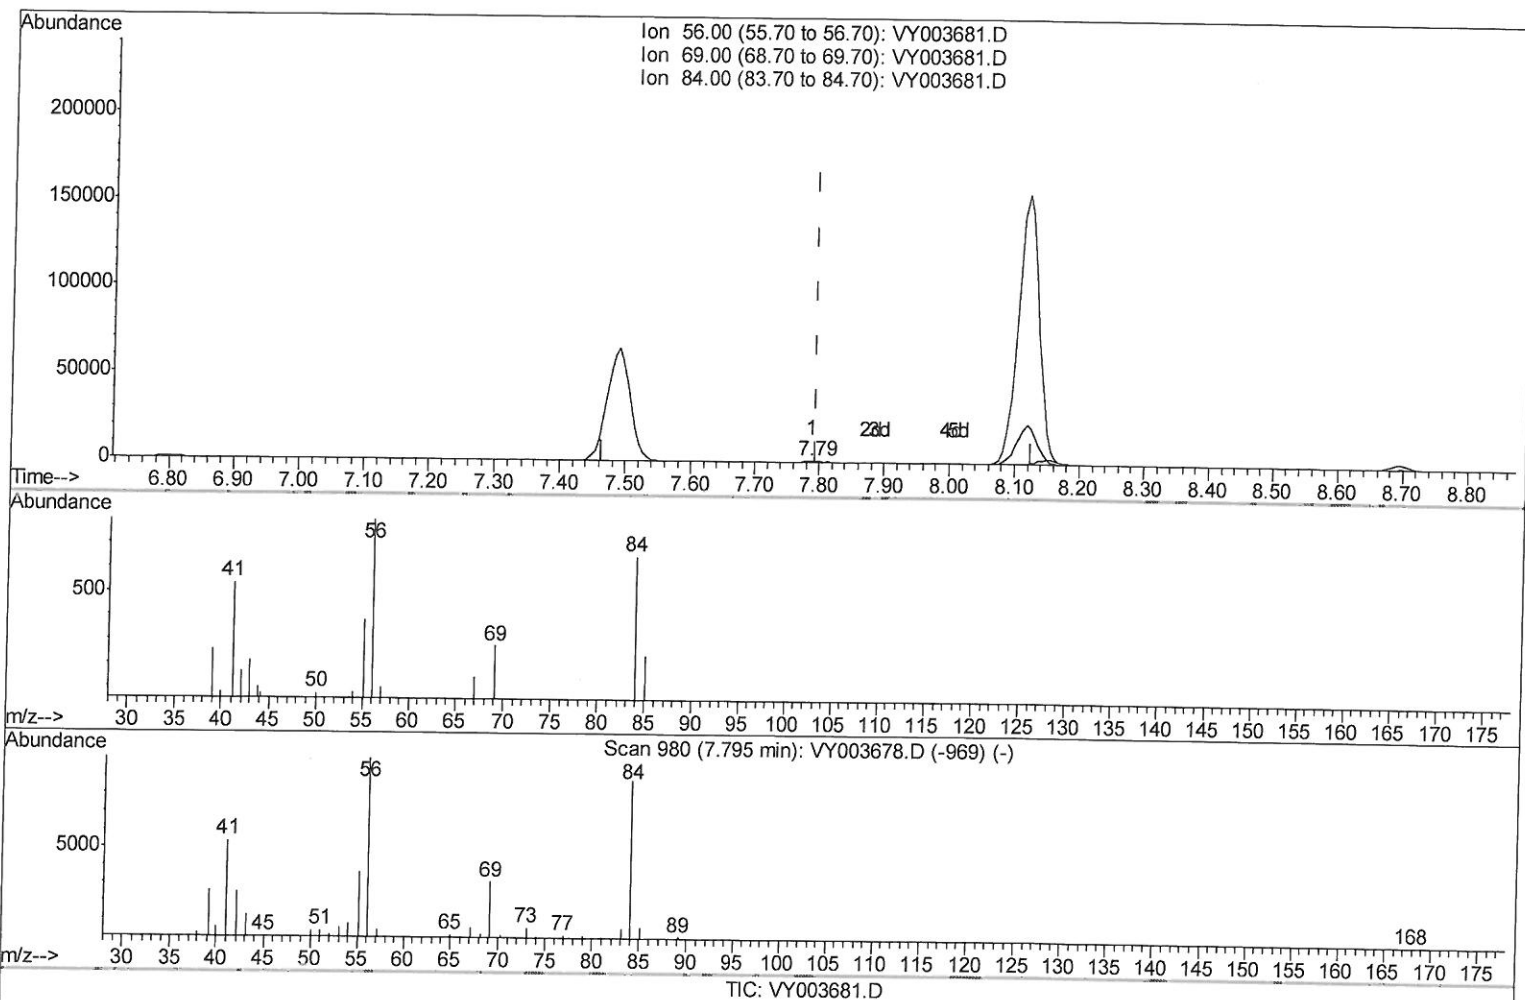

(30) Cyclohexane (T)

7.789min (-0.006) 0.43ug/L

response 1517

Ion	Exp%	Act%
56.00	100	100
69.00	29.80	15.82#
84.00	91.50	107.32
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA Y\DATA\VY120820\
Data File : VY003681.D
Acq On : 08 Dec 2020 17:29
Operator : SY/MD
Sample : L4979-06
Misc : 5.00G/10ML/MSVOA Y/SOIL
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
GB1F8

Manual Integrations
APPROVED

MMDadoda
12/10/2020 9:59:29 AM

Quant Time: Dec 09 02:40:10 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\SOM2YLM120420S.M
Quant Title : VOC Analysis
QLast Update : Wed Dec 09 01:58:23 2020
Response via : Initial Calibration

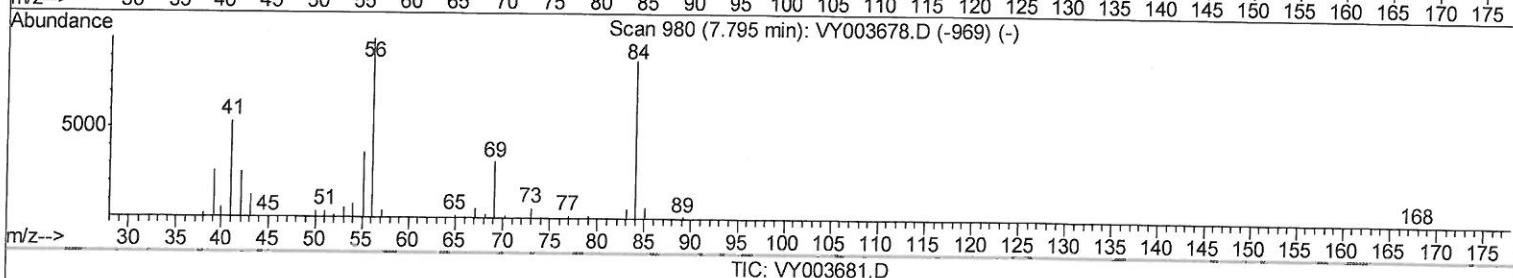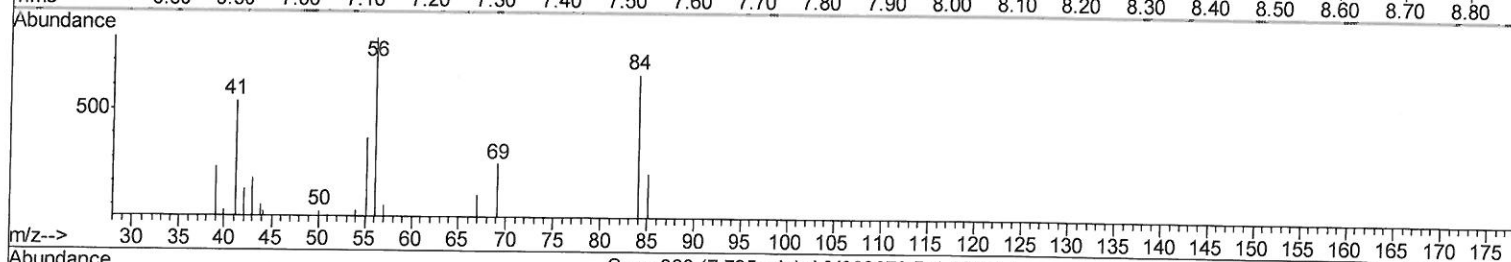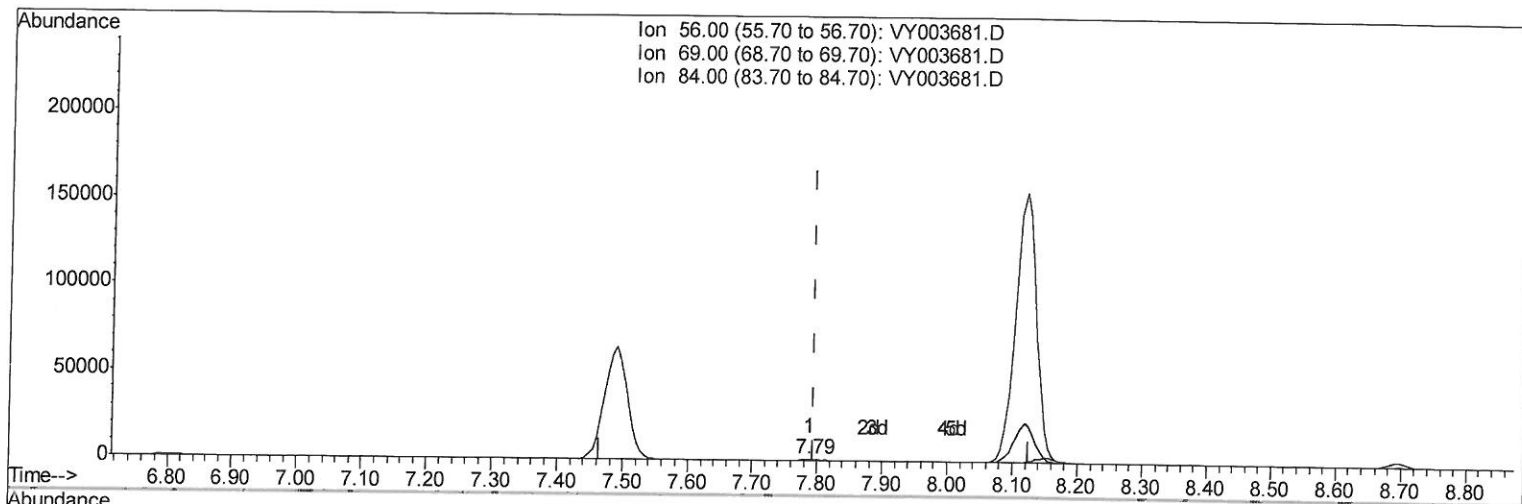

TIC: VY003681.D

(30) Cyclohexane (T)

7.789min (-0.006) 0.51ug/L m

response 1775

Ion	Exp%	Act%
56.00	100	100
69.00	29.80	13.52#
84.00	91.50	91.72
0.00	0.00	0.00

12/20/2020

Data Path : Z:\VOASRV\HPCHEM1\MSVOA Y\DATA\VY120820\
 Data File : VY003681.D
 Acq On : 08 Dec 2020 17:29
 Operator : SY/MD
 Sample : L4979-06
 Misc : 5.00G/10ML/MSVOA Y/SOIL
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 GB1F8

Manual Integrations
 APPROVED

MMDadoda
 12/10/2020 9:59:29 AM

Quant Time: Dec 09 02:45:14 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\SOM2YLM120420S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Dec 09 01:58:23 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.70	114	238802	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.50	117	162361	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.43	152	33509	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.25	65	87975	26.05	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	104.20%		
7) Chloroethane-d5	2.77	69	67091	26.33	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	105.32%		
10) 1,1-Dichloroethene-d2	3.86	63	132043	20.78	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	83.12%		
20) 2-Butanone-d5	6.89	46	36090	29.98	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	59.96%		
24) Chloroform-d	7.49	84	158593	25.81	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	103.24%		
26) 1,2-Dichloroethane-d4	8.15	65	79289	22.93	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	91.72%		
29) Benzene-d6	8.12	84	344241	36.62	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	146.48%#		
33) 1,2-Dichloropropane-d6	9.12	67	98041	35.25	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	141.00%#		
37) Toluene-d8	10.18	98	283675	33.67	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	134.68%#		
38) trans-1,3-Dichloropropene-	10.44	79	37122	27.92	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	111.68%		
39) 2-Hexanone-d5	10.79	63	26435	37.93	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	75.86%		
48) 1,1,2,2-Tetrachloroethane-	12.56	84	45446	18.34	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	73.36%		
61) 1,2-Dichlorobenzene-d4	13.73	152	29376	24.13	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	96.52%		

Target Compounds

					Ovalue	
13) Acetone	3.95	43	14582	16.523	ug/L	97
16) Methylene chloride	4.73	84	11588	2.764	ug/L	88
21) 2-Butanone	6.99	43	2795m	1.794	ug/L	
30) Cyclohexane	7.79	56	1775m	0.507	ug/L	
34) Benzene	8.17	78	5931	0.639	ug/L	100
36) Methylcyclohexane	9.18	83	2350	0.601	ug/L #	88
44) Toluene	10.25	91	28364	2.895	ug/L	95
53) Ethylbenzene	11.59	91	20216	1.891	ug/L	95
54) m,p-Xylene	11.70	106	2350	0.570	ug/L	72
55) o-xylene	12.03	106	1071	0.271	ug/L	92

(#) = qualifier out of range (m) = manual integration (+) = signals summed

12/23/20 SY

Data Path : Z:\VOASRV\HPCHEM1\MSVOA Y\DATA\VY120820\
Data File : VY003681.D
Acq On : 08 Dec 2020 17:29
Operator : SY/MD
Sample : L4979-06
Misc : 5.00G/10ML/MSVOA Y/SOIL
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
GB1F8

Manual Integrations
APPROVED

MMDadoda
12/10/2020 9:59:29 AM

Quant Time: Dec 09 02:45:14 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\SOM2YLM120420S.M
Quant Title : VOC Analysis
QLast Update : Wed Dec 09 01:58:23 2020
Response via : Initial Calibration

