


Data Path : Z:\voasrv\HPCHEM1\MSVOA Y\Data\vv120919\
Data File : VY000905.D
Acq On : 09 Dec 2019 09:52
Operator : SY/MD
Sample : BFB
Misc : 5.00G/5ML/MSVOA Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y112719S.M
Title : SW846 8260
Last Update : Wed Nov 27 12:40:47 2019

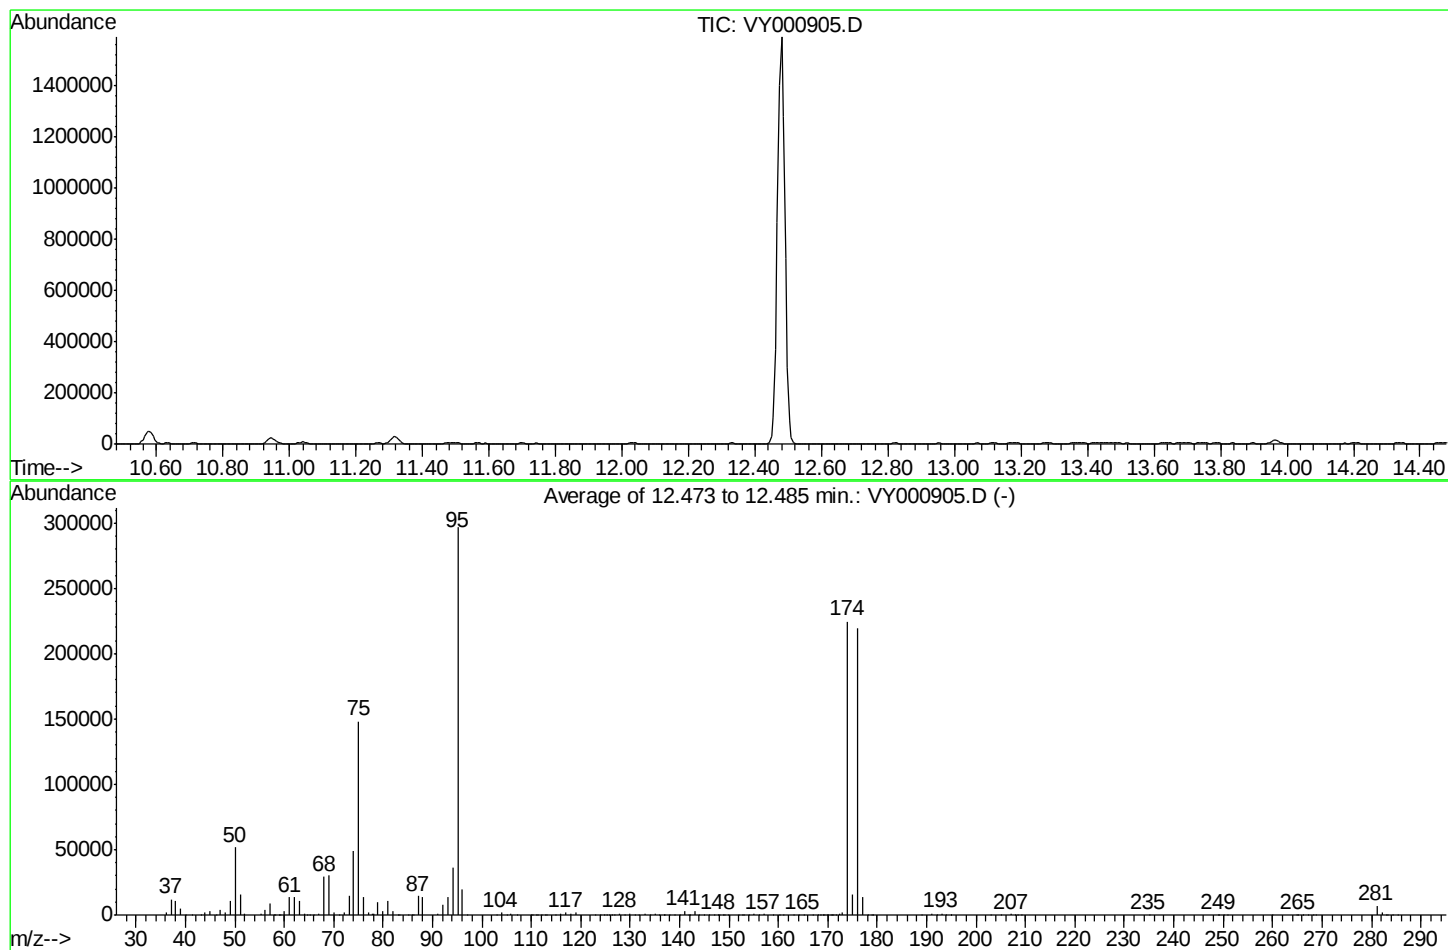

AutoFind: Scans 1761, 1762, 1763; Background Corrected with Scan 1753

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.4	51714	PASS
75	95	30	60	50.0	148208	PASS
95	95	100	100	100.0	296618	PASS
96	95	5	9	6.5	19199	PASS
173	174	0.00	2	0.8	1841	PASS
174	95	50	100	75.7	224426	PASS
175	174	5	9	7.2	16157	PASS
176	174	95	101	98.0	219861	PASS
177	176	5	9	6.5	14222	PASS