

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_Y\DATA\VY120920\NOT REVIEWED DATA\
 Data File : VY003708.D
 Acq On : 09 Dec 2020 18:05
 Operator : SY/MD
 Sample : L4979-11RE
 Misc : 5.59G/10ML/MSVOA_Y/SOIL
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 GB1G1

Quant Time: Dec 10 12:06:04 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\SOM2YLM120420S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Dec 10 11:26:10 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.70	114	193896	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.49	117	183326	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.43	152	85254	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.25	65	54010	19.70	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	78.80%
7) Chloroethane-d5	2.77	69	45144	21.82	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	87.28%
10) 1,1-Dichloroethene-d2	3.86	63	83086	16.10	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	64.40%
20) 2-Butanone-d5	6.90	46	39525	40.43	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	80.86%
24) Chloroform-d	7.49	84	115887	23.23	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	92.92%
26) 1,2-Dichloroethane-d4	8.15	65	64394	22.94	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	91.76%
29) Benzene-d6	8.12	84	249766	23.53	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	94.12%
33) 1,2-Dichloropropane-d6	9.13	67	75405	24.01	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	96.04%
37) Toluene-d8	10.18	98	229867	24.16	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	96.64%
38) trans-1,3-Dichloropropene-	10.44	79	35207	23.45	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	93.80%
39) 2-Hexanone-d5	10.79	63	34817	44.25	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	88.50%
48) 1,1,2,2-Tetrachloroethane-	12.56	84	65319	23.34	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	93.36%
61) 1,2-Dichlorobenzene-d4	13.72	152	82367	26.59	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	106.36%

Target Compounds


					Qvalue
3) Chloromethane	2.11	50	893	0.378 ug/L	83
13) Acetone	3.96	43	5458	7.617 ug/L	100
16) Methylene chloride	4.73	84	4904	1.440 ug/L	76
25) Chloroform	7.51	83	1244	0.280 ug/L #	22
34) Benzene	8.17	78	2785	0.266 ug/L	100
35) Trichloroethene	8.70	95	5246	1.822 ug/L #	2
40) 1,2-Dichloropropane	9.12	63	8247	3.135 ug/L #	86
44) Toluene	10.25	91	9207	0.832 ug/L	95
53) Ethylbenzene	11.59	91	7527	0.623 ug/L	96
58) 1,1,2,2-Tetrachloroethane	12.56	83	441	0.181 ug/L #	1
59) 1,2,3-Trichloropropane	13.42	75	10186	4.686 ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_Y\DATA\VY120920\NOT REVIEWED DATA\
Data File : VY003708.D
Acq On : 09 Dec 2020 18:05
Operator : SY/MD
Sample : L4979-11RE
Misc : 5.59G/10ML/MSVOA_Y/SOIL
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
GB1G1

Quant Time: Dec 10 12:06:04 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_Y\METHODS\SOM2YLM120420S.M
Quant Title : VOC Analysis
QLast Update : Thu Dec 10 11:26:10 2020
Response via : Initial Calibration

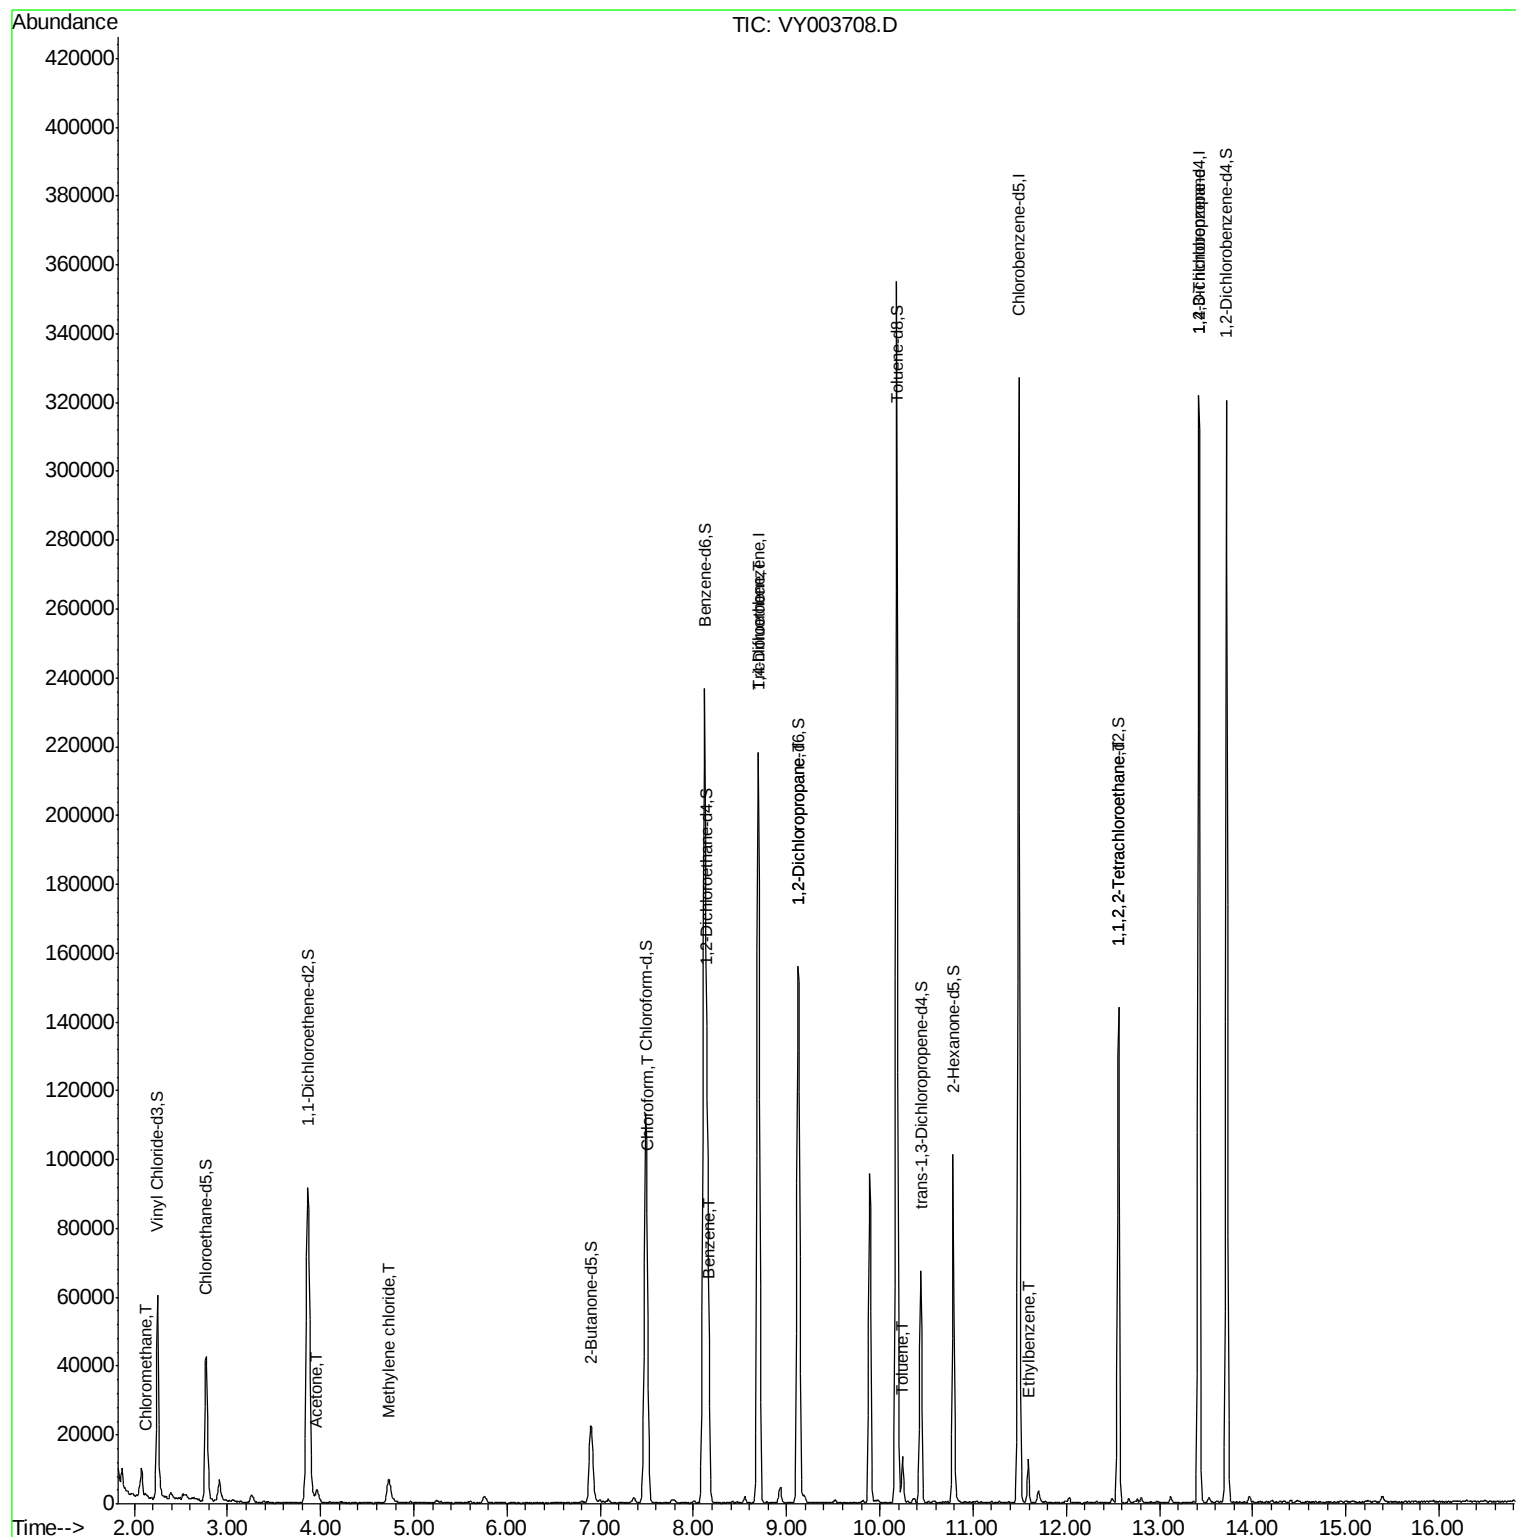

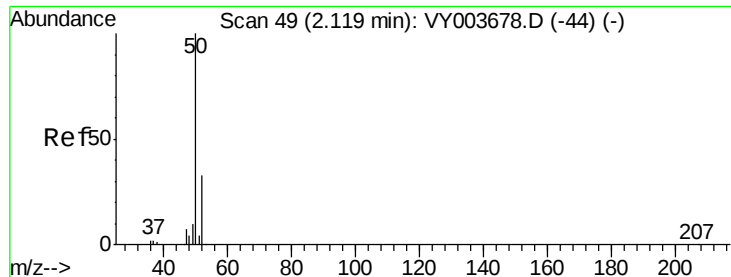

#3

Chloromethane

Concen: 0.378 ug/L

RT: 2.11 min Scan# 48

Delta R.T. -0.01 min

Lab File: VY003708.D

Acq: 09 Dec 2020 18:05

Instrument :

MSVOA_Y

ClientSampleId :





GB1G1

Tgt Ion: 50 Resp: 893

Ion Ratio Lower Upper

50 100

52 23.4 23.1 42.9

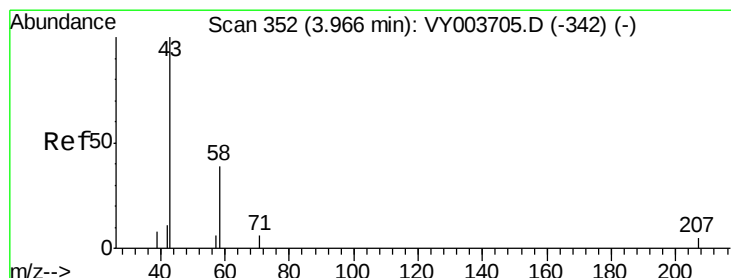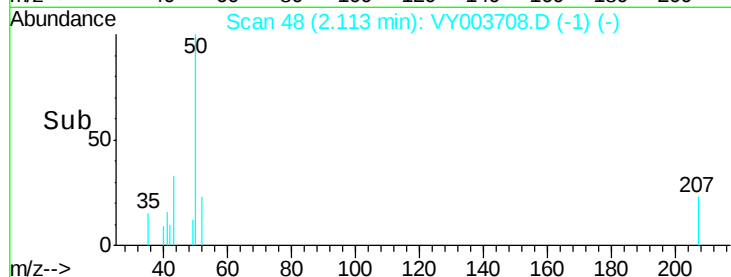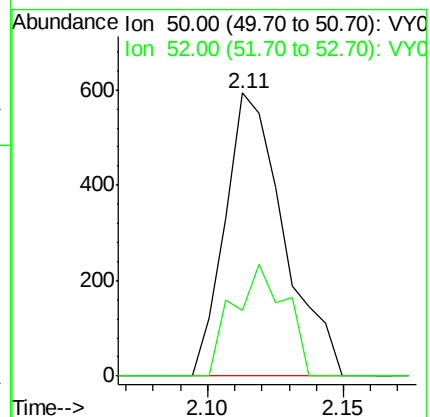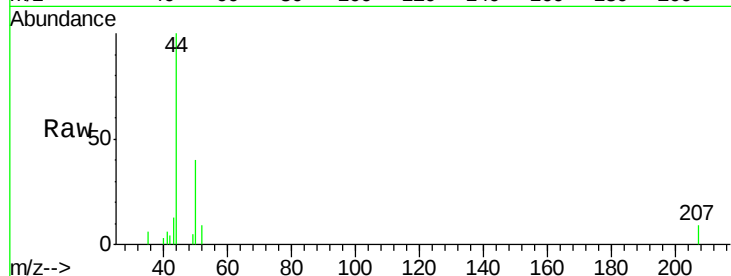

#13

Acetone

Concen: 7.617 ug/L

RT: 3.96 min Scan# 351

Delta R.T. -0.01 min

Lab File: VY003708.D




Acq: 09 Dec 2020 18:05


Tgt Ion: 43 Resp: 5458

Ion Ratio Lower Upper

43 100

58 34.5 0.0 68.8


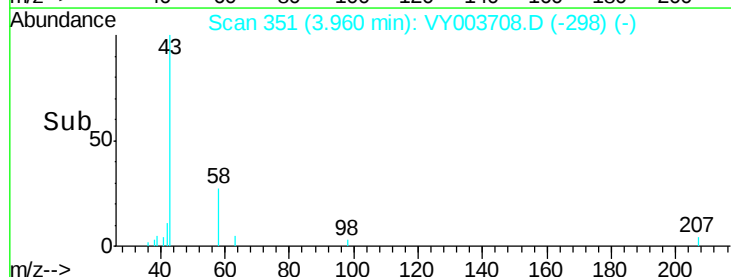
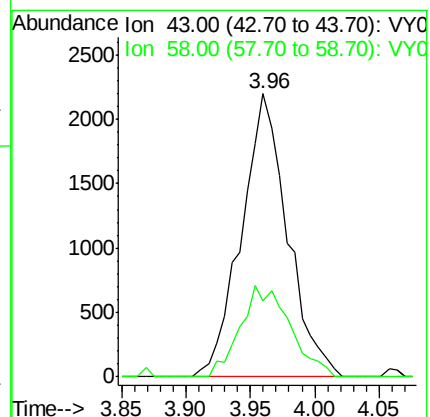
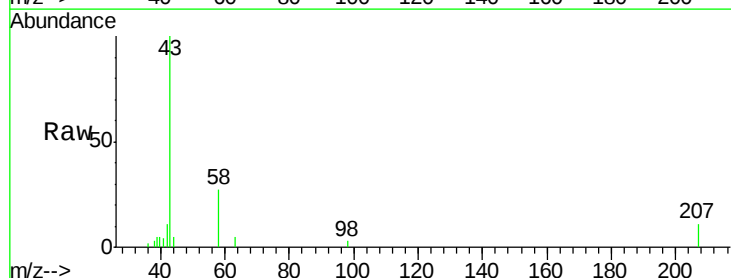


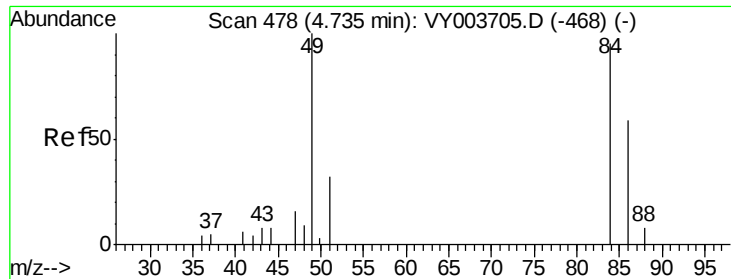

#16
Methylene chloride
Concen: 1.440 ug/L
RT: 4.73 min Scan# 477
Delta R.T. 0.00 min
Lab File: VY003708.D
Acq: 09 Dec 2020 18:05




Instrument :
MSVOA_Y
ClientSampled :
GB1G1


Tgt Ion: 84 Resp: 4904
Ion Ratio Lower Upper
84 100
49 84.9 83.7 155.4
86 56.9 45.0 83.6

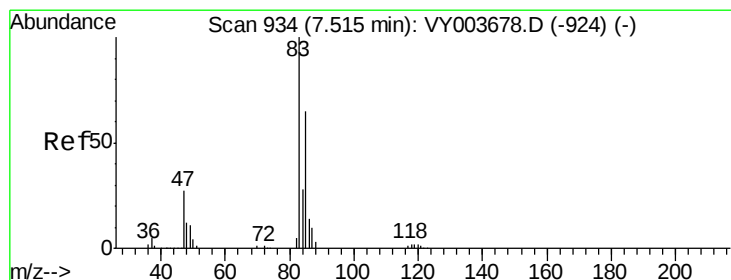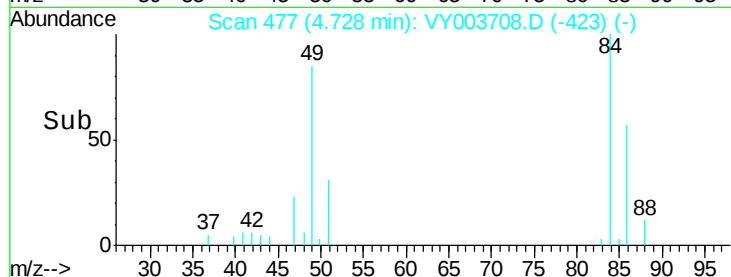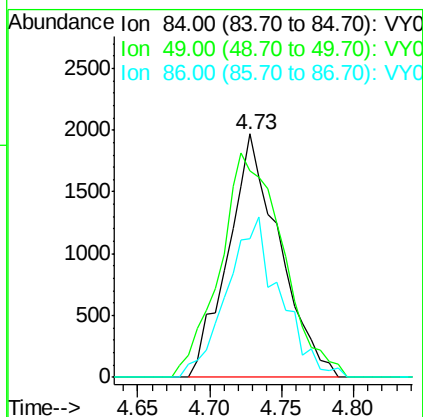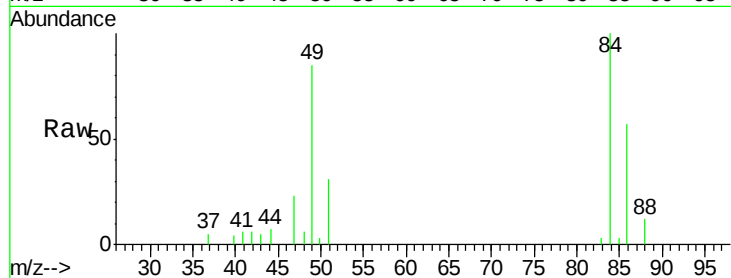

#25
Chloroform
Concen: 0.280 ug/L
RT: 7.51 min Scan# 933
Delta R.T. -0.01 min
Lab File: VY003708.D
Acq: 09 Dec 2020 18:05

Tgt Ion: 83 Resp: 1244
Ion Ratio Lower Upper
83 100
85 128.5 46.5 86.5#

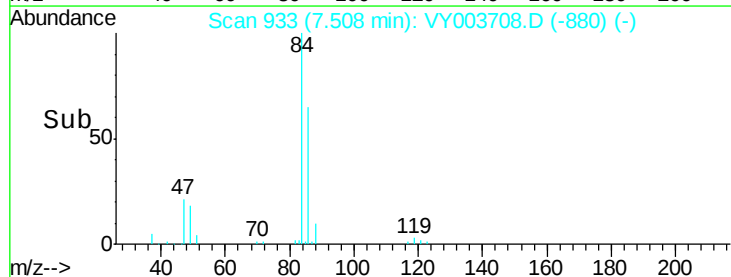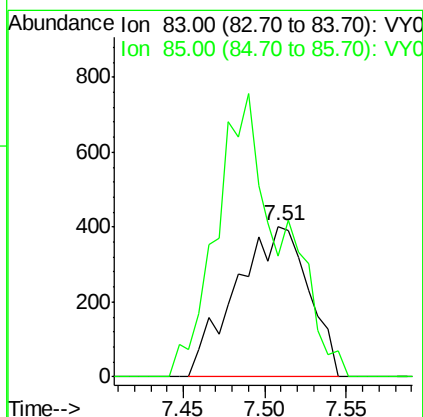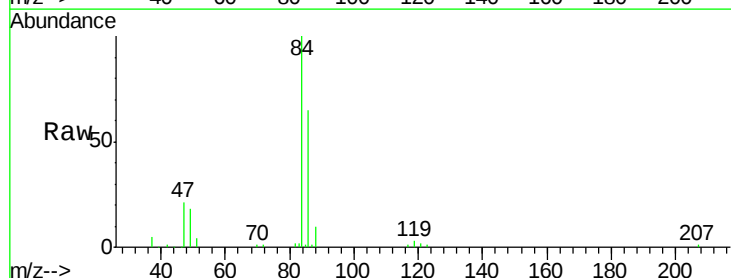

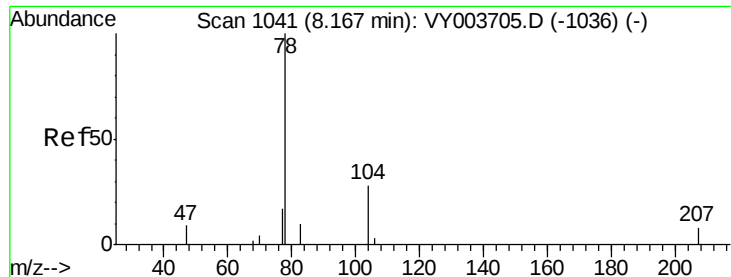

#34

Benzene

Concen: 0.266 ug/L

RT: 8.17 min Scan# 1042

Delta R.T. 0.00 min

Lab File: VY003708.D

Acq: 09 Dec 2020 18:05


Instrument :

MSVOA_Y




ClientSampleId :

GB1G1

Tgt Ion: 78 Resp: 2785

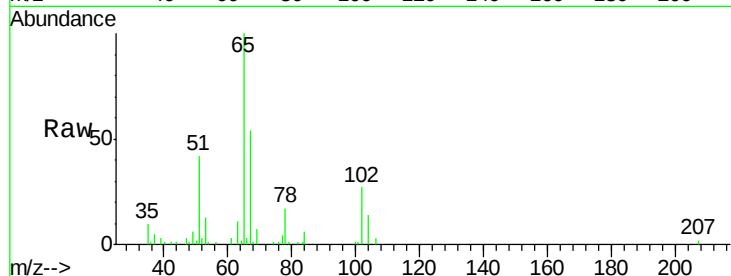

Abundance Ion 78.00 (77.70 to 78.70): VY0

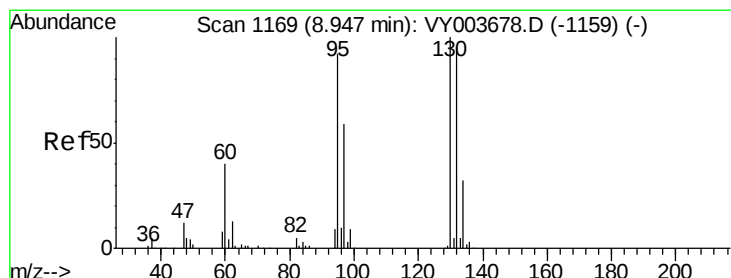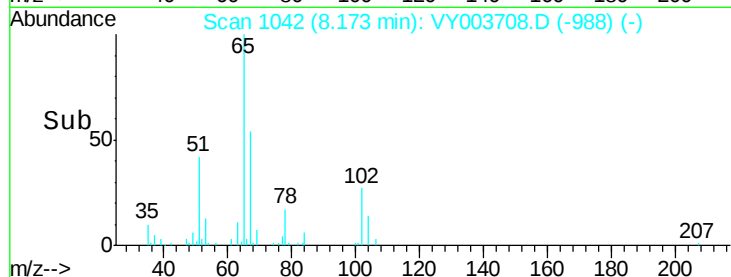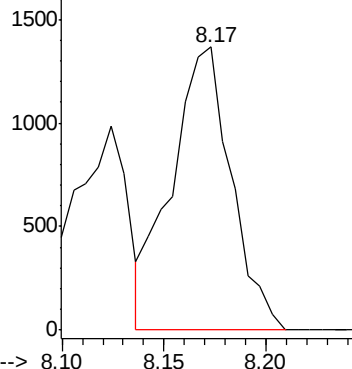

#35

Trichloroethene

Concen: 1.822 ug/L

RT: 8.70 min Scan# 1128

Delta R.T. -0.25 min

Lab File: VY003708.D

Acq: 09 Dec 2020 18:05

Tgt Ion: 95 Resp: 5246


Ion Ratio Lower Upper

95 100

97 0.0 45.8 85.0#

132 0.9 74.2 137.8#

130 1.1 76.2 141.6#


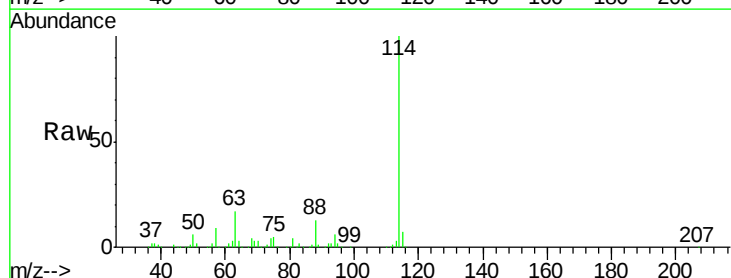



Abundance Ion 95.00 (94.70 to 95.70): VY0

Ion 97.00 (96.70 to 97.70): VY0

Ion 132.00 (131.70 to 132.70): VY0

Ion 130.00 (129.70 to 130.70): VY0



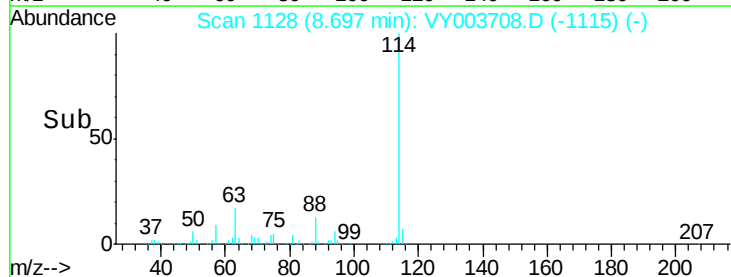
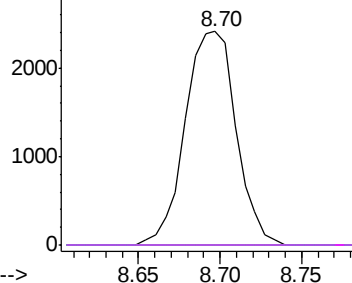


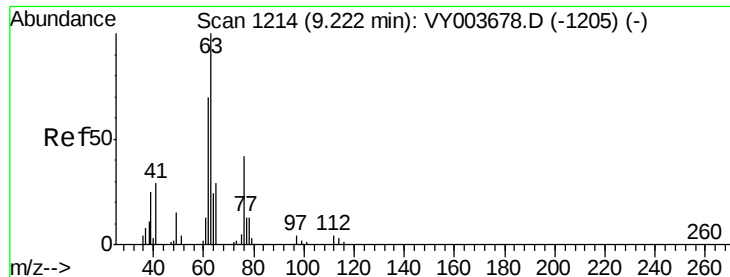

#40
 1,2-Dichloropropane
 Concen: 3.135 ug/L
 RT: 9.12 min Scan# 1198
 Delta R.T. -0.10 min
 Lab File: VY003708.D
 Acq: 09 Dec 2020 18:05




Instrument :
 MSVOA_Y
 ClientSampleId :
 GB1G1


Tgt Ion: 63 Resp: 8247
 Ion Ratio Lower Upper
 63 100
 112 0.0 3.7 5.5#

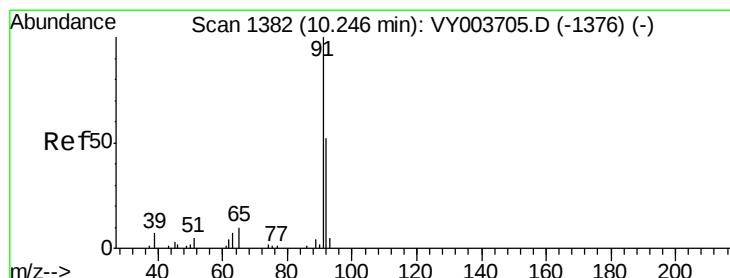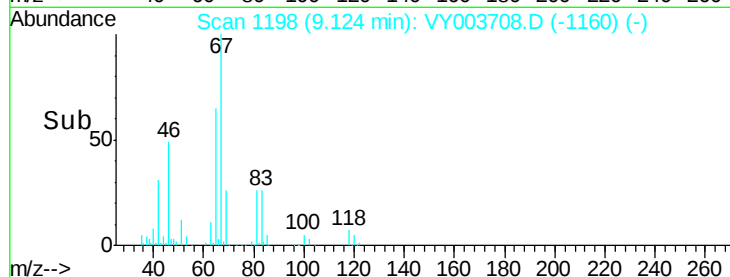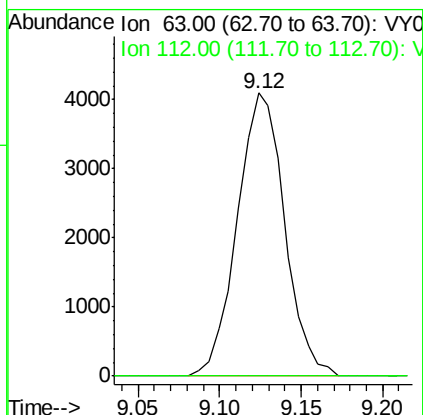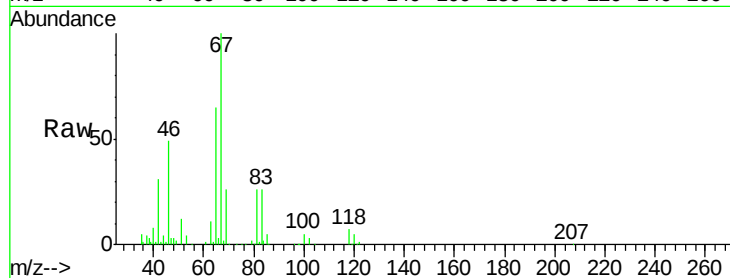

#44
 Toluene
 Concen: 0.832 ug/L
 RT: 10.25 min Scan# 1382
 Delta R.T. 0.00 min
 Lab File: VY003708.D
 Acq: 09 Dec 2020 18:05

Tgt Ion: 91 Resp: 9207
 Ion Ratio Lower Upper
 91 100
 92 53.3 39.8 73.8

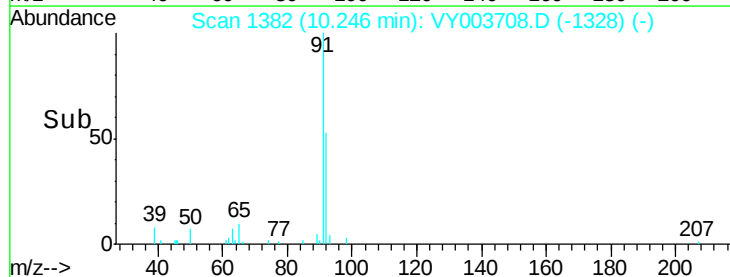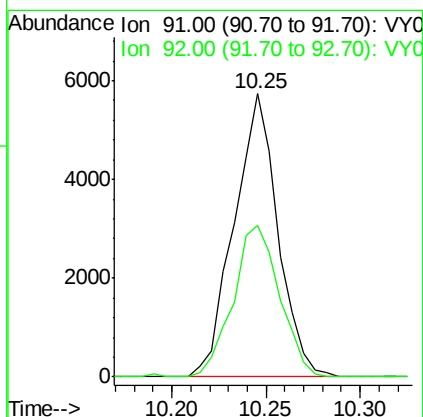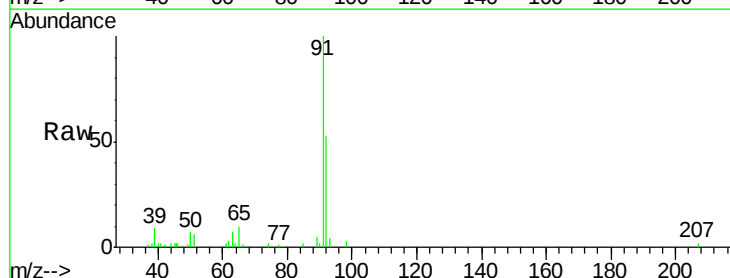

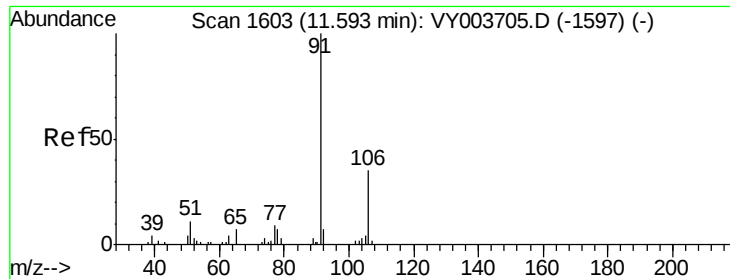

#53

Ethylbenzene

Concen: 0.623 ug/L

RT: 11.59 min Scan# 1603

Delta R.T. 0.00 min

Lab File: VY003708.D

Acq: 09 Dec 2020 18:05

Instrument :

MSVOA_Y

ClientSampleId :





GB1G1

Tgt Ion: 91 Resp: 7527

Ion Ratio Lower Upper

91 100

106 31.1 23.3 43.3

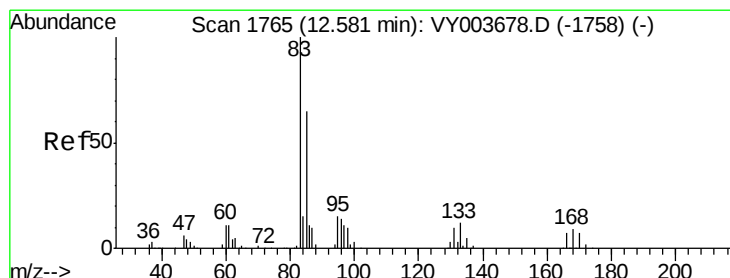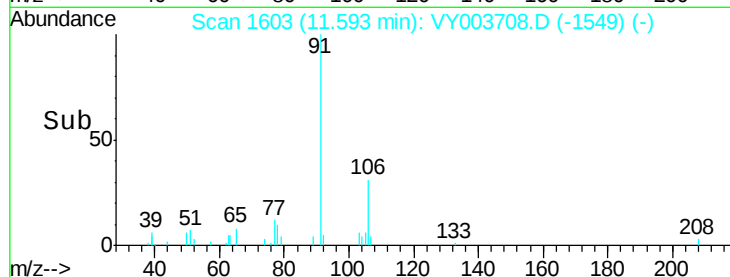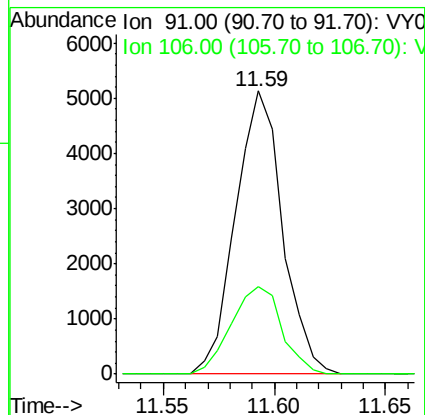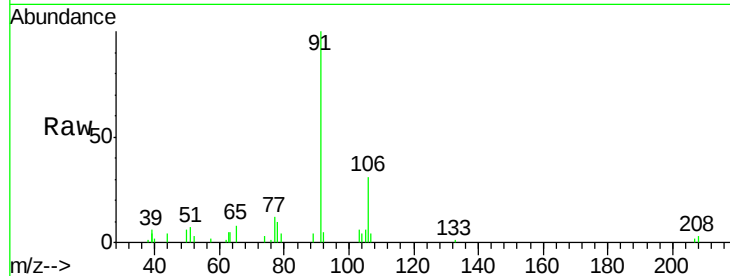

#58

1,1,2,2-Tetrachloroethane

Concen: 0.181 ug/L

RT: 12.56 min Scan# 1762

Delta R.T. -0.02 min

Lab File: VY003708.D

Acq: 09 Dec 2020 18:05




Tgt Ion: 83 Resp: 441


Ion Ratio Lower Upper

83 100

85 226.7 47.2 87.6#

131 278.8 8.4 12.6#

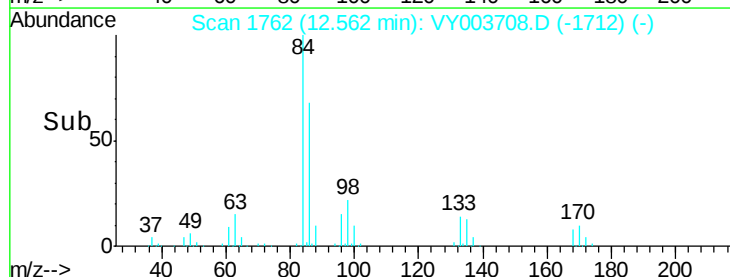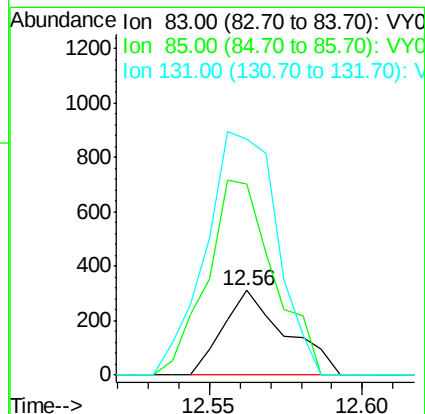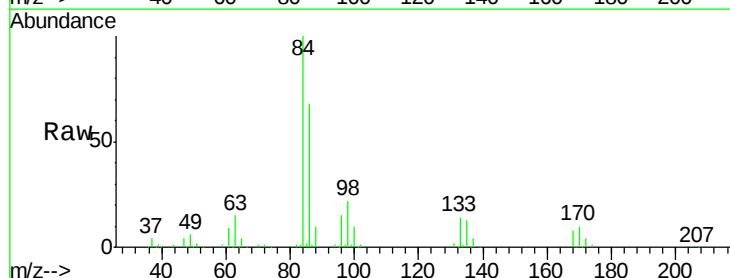

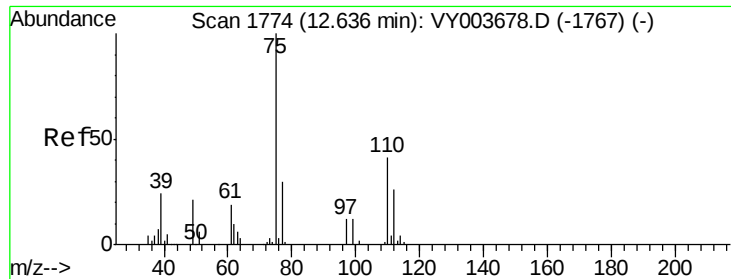

#59

1,2,3-Trichloropropane

Concen: 4.686 ug/L

RT: 13.42 min Scan# 1903

Delta R.T. 0.79 min

Lab File: VY003708.D

Acq: 09 Dec 2020 18:05

Instrument :

MSVOA_Y

ClientSampleId :


GB1G1

Tgt Ion: 75 Resp: 10186

Ion Ratio Lower Upper

75 100

77 32.6 25.9 38.9

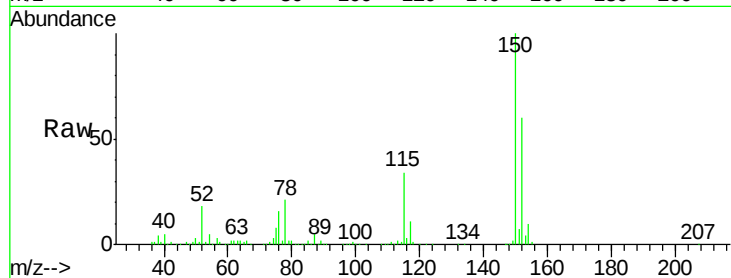

Abundance Ion 75.00 (74.70 to 75.70): VY0

Ion 77.00 (76.70 to 77.70): VY0

