

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA Y\DATA\VY120920\
 Data File : VY003692.D
 Acq On : 09 Dec 2020 10:58
 Operator : SY/MD
 Sample : VY1209SBL01
 Misc : 5.00G/10ML/MSVOA Y/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VBLK86

Manual Integrations
 APPROVED

MMDadoda
 12/11/2020 12:25:16 PM

Quant Time: Dec 10 02:28:44 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\SOM2YLM120420S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Dec 10 02:27:01 2020
 Response via : Initial Calibration

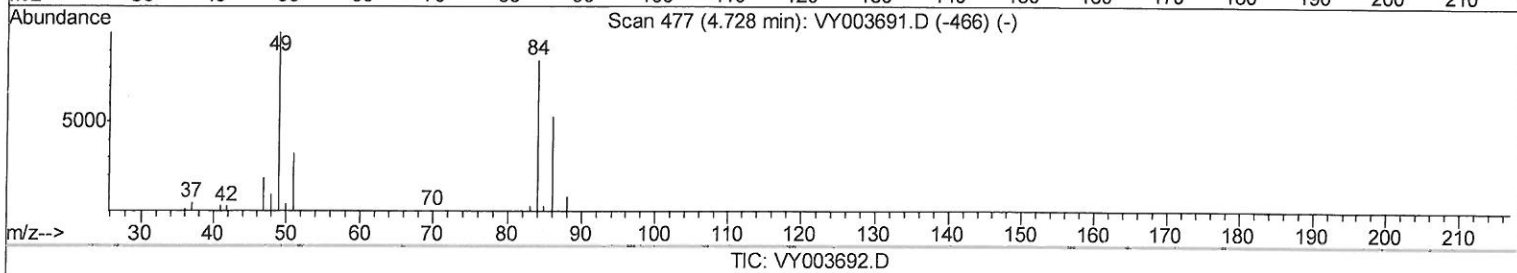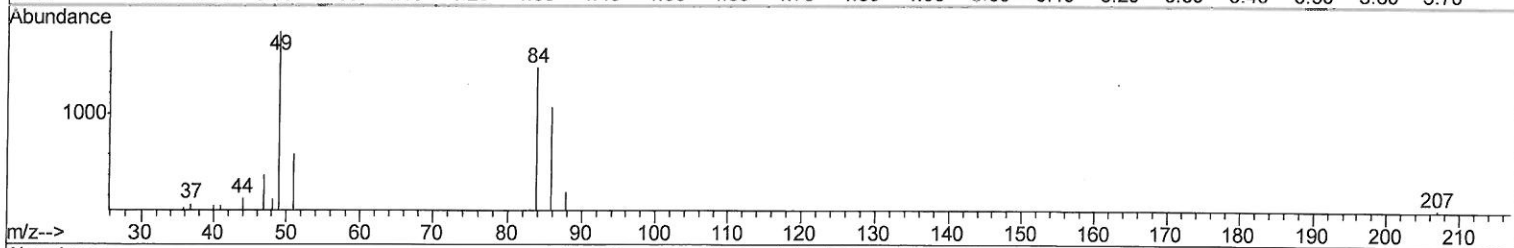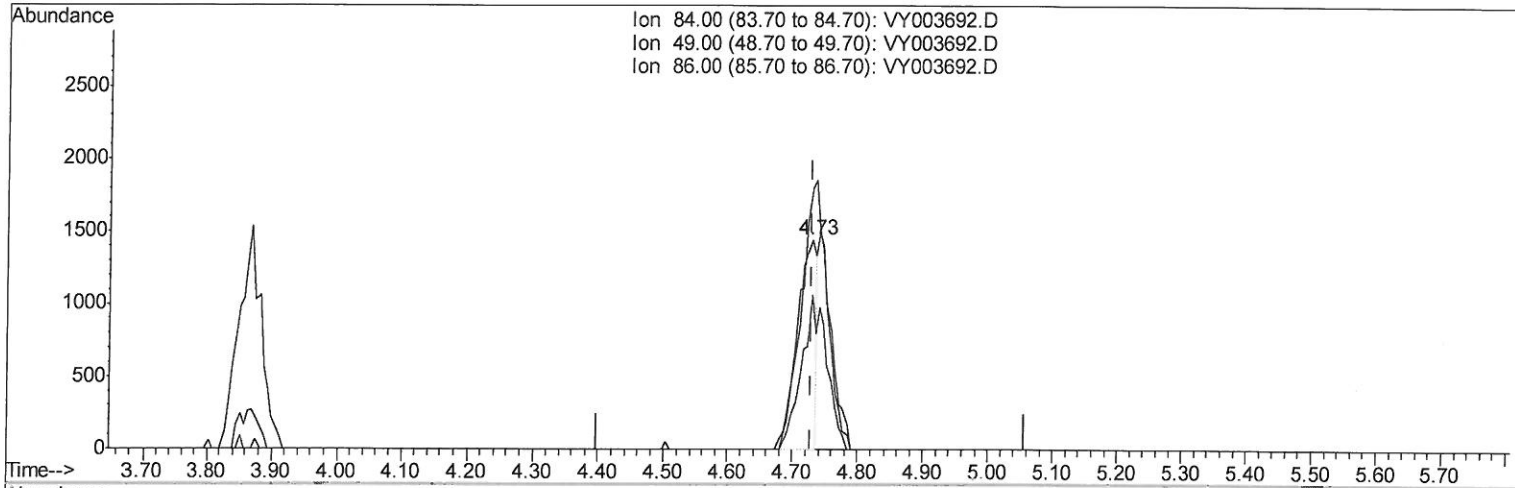

TIC: VY003692.D

(16) Methylene chloride (T)

4.729min (+0.001) 0.72ug/L

response 2831

Ion	Exp%	Act%
84.00	100	100
49.00	119.50	124.33
86.00	64.30	73.60
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA Y\DATA\VY120920\
 Data File : VY003692.D
 Acq On : 09 Dec 2020 10:58
 Operator : SY/MD
 Sample : VY1209SBL01
 Misc : 5.00G/10ML/MSVOA Y/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VBLK86

Manual Integrations
 APPROVED

MMDadoda
 12/11/2020 12:25:16 PM

Quant Time: Dec 10 02:28:44 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\SOM2YLM120420S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Dec 10 02:27:01 2020
 Response via : Initial Calibration

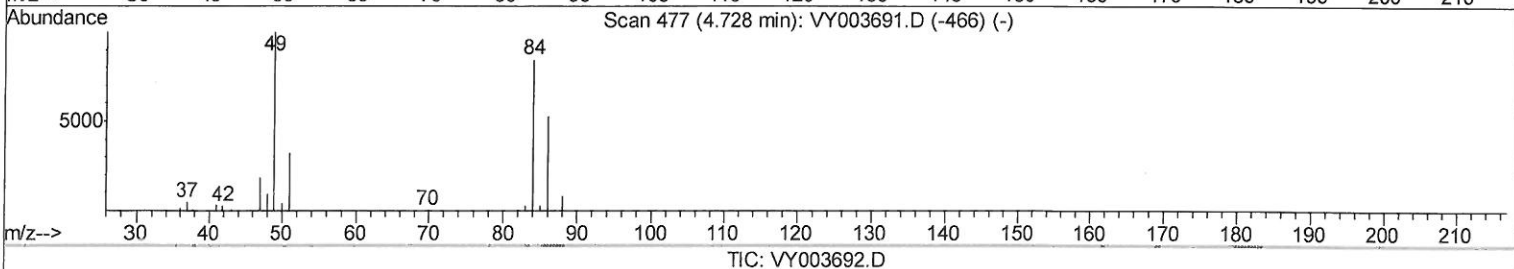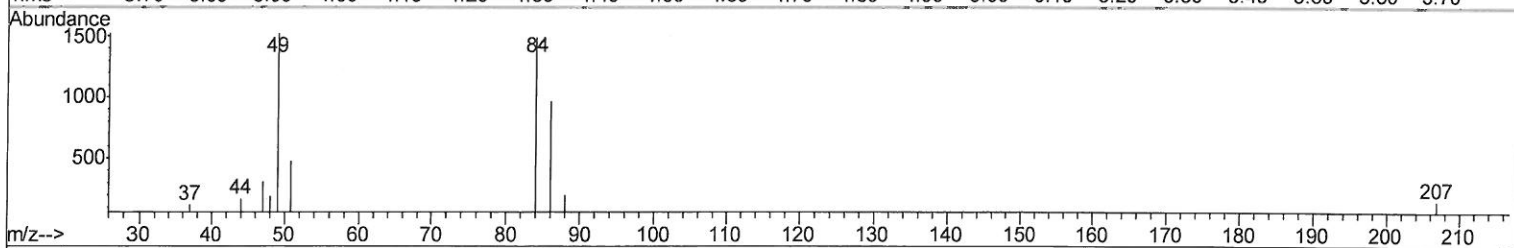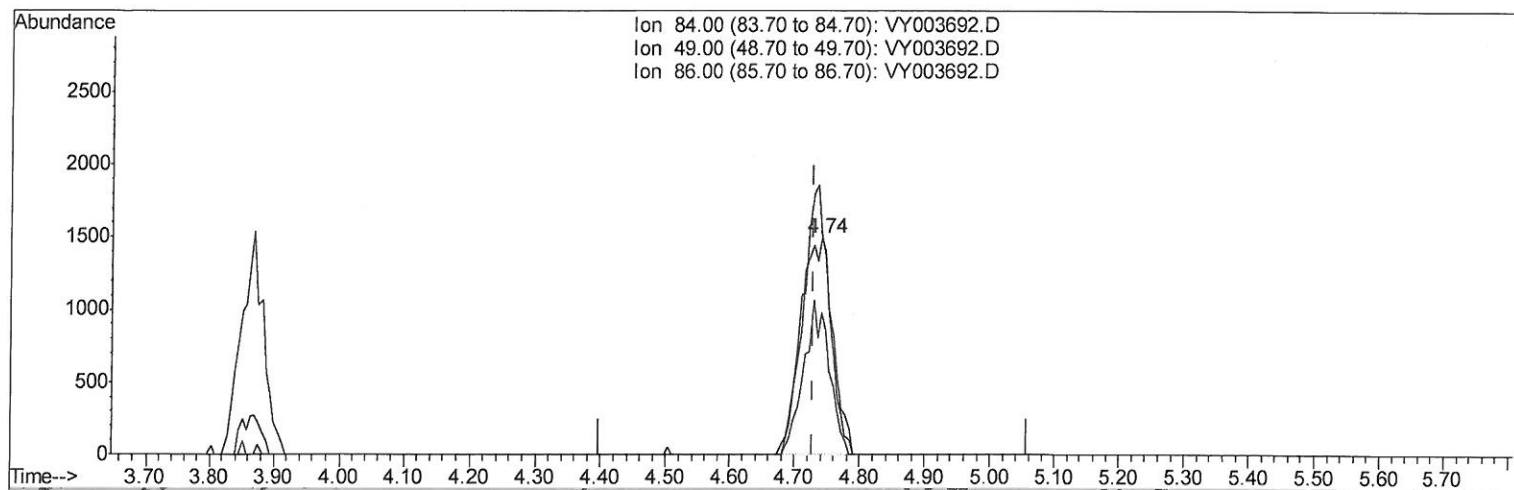

(16) Methylene chloride (T)

4.741min (+0.013) 1.22ug/L m

response 4824

Ion	Exp%	Act%
84.00	100	100
49.00	119.50	102.01
86.00	64.30	65.35
0.00	0.00	0.00

2 12/18/2020

Quantitation Report (QT Reviewed)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA Y\DATA\VY120920\
 Data File : VY003692.D
 Acq On : 09 Dec 2020 10:58
 Operator : SY/MD
 Sample : VY1209SBL01
 Misc : 5.00G/10ML/MSVOA Y/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 Client Sampled :
 VBLK86

Manual Integrations
 APPROVED

MMDadoda
 12/11/2020 12:25:16 PM

Quant Time: Dec 10 02:54:47 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\SOM2YLM120420S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Dec 10 02:27:01 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.70	114	225395	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.49	117	212549	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.43	152	105959	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.25	65	77268	24.24	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	96.96%
7) Chloroethane-d5	2.77	69	61053	25.39	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	101.56%
10) 1,1-Dichloroethene-d2	3.86	63	112852	18.81	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	75.24%
20) 2-Butanone-d5	6.90	46	46831	41.21	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	82.42%
24) Chloroform-d	7.49	84	141791	24.45	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	97.80%
26) 1,2-Dichloroethane-d4	8.15	65	80312	24.61	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	98.44%
29) Benzene-d6	8.12	84	312801	25.42	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	101.68%
33) 1,2-Dichloropropane-d6	9.12	67	93138	25.58	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	102.32%
37) Toluene-d8	10.18	98	287510	26.06	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	104.24%
38) trans-1,3-Dichloropropene-	10.44	79	44585	25.62	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	102.48%
39) 2-Hexanone-d5	10.79	63	38501	42.20	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	84.40%
48) 1,1,2,2-Tetrachloroethane-	12.56	84	79009	24.35	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	97.40%
61) 1,2-Dichlorobenzene-d4	13.72	152	103972	27.01	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	108.04%

Target Compounds

16) Methylene chloride	4.74	84	4824m	1.219	ug/L	Ovalue
------------------------	------	----	-------	-------	------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quantitation Report (QT Reviewed)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA Y\DATA\VY120920\
 Data File : VY003692.D
 Acq On : 09 Dec 2020 10:58
 Operator : SY/MD
 Sample : VY1209SBL01
 Misc : 5.00G/10ML/MSVOA Y/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 Client Sampled :
 VBLK86

Manual Integrations
 APPROVED

MMDadoda
 12/11/2020 12:25:16 PM

Quant Time: Dec 10 02:54:47 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\SOM2YLM120420S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Dec 10 02:27:01 2020
 Response via : Initial Calibration

