
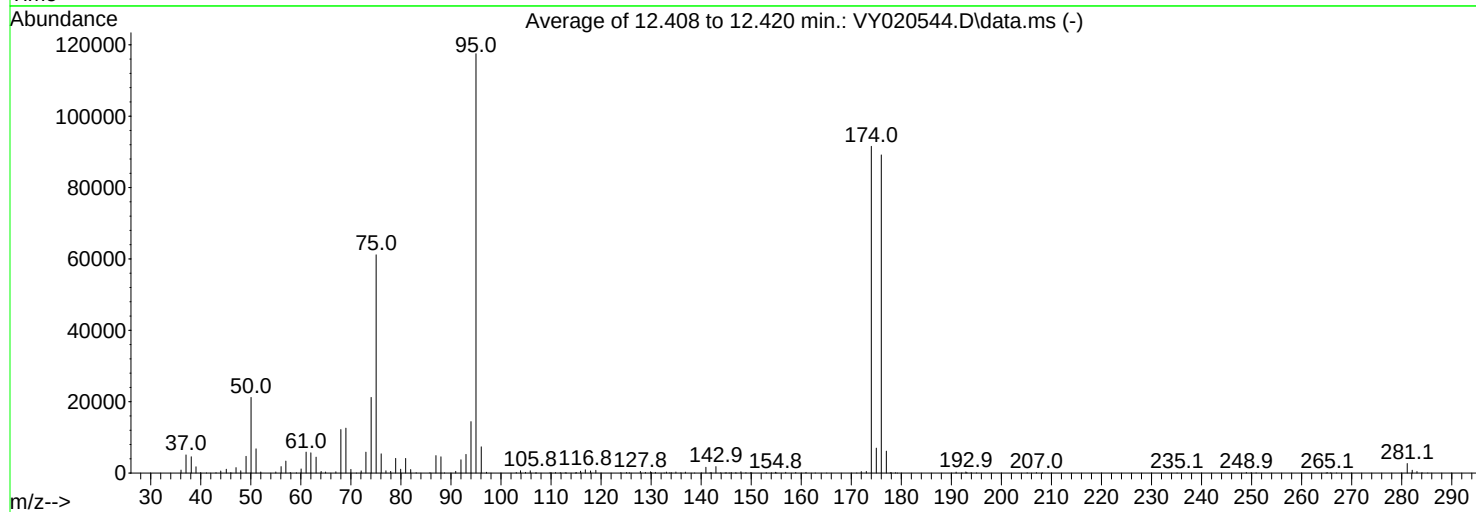


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY120924\
Data File : VY020544.D
Acq On : 09 Dec 2024 08:58
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y120224S.M
Title : SW846 8260
Last Update : Tue Dec 03 01:39:23 2024

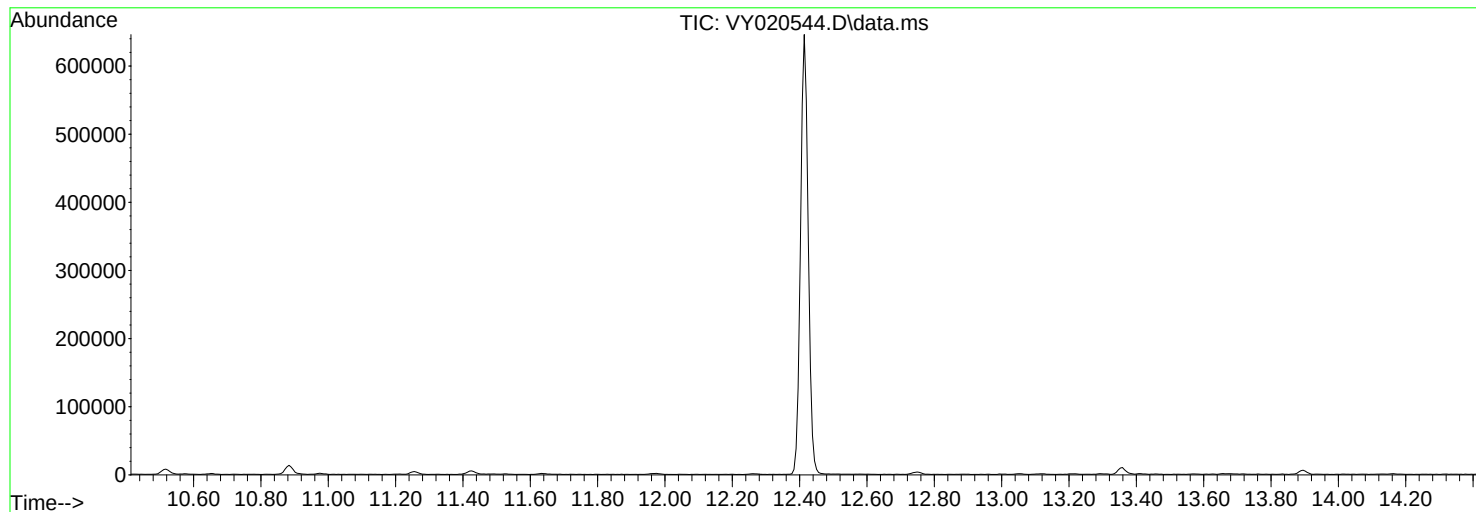

AutoFind: Scans 1753, 1754, 1755; Background Corrected with Scan 1745

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.0	21205	PASS
75	95	30	60	52.1	61160	PASS
95	95	100	100	100.0	117501	PASS
96	95	5	9	6.3	7362	PASS
173	174	0.00	2	0.5	453	PASS
174	95	50	100	77.9	91560	PASS
175	174	5	9	7.6	6996	PASS
176	174	95	101	97.4	89152	PASS
177	176	5	9	6.9	6148	PASS