

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY121024\
 Data File : VY020577.D
 Acq On : 10 Dec 2024 18:30
 Operator : SY/MD
 Sample : P5194-05
 Misc : 5.05g/5.0mL/MSVOA_Y/SOIL/A
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 WP-3

Quant Time: Dec 11 00:53:26 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y120224S.M
 Quant Title : SW846 8260
 QLast Update : Tue Dec 03 01:39:23 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.707	168	144830	50.000	ug/l	-0.01
34) 1,4-Difluorobenzene	8.610	114	254650	50.000	ug/l	-0.01
63) Chlorobenzene-d5	11.414	117	223520	50.000	ug/l	-0.01
72) 1,4-Dichlorobenzene-d4	13.347	152	90631	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.061	65	87593	59.468	ug/l	-0.01
Spiked Amount	50.000	Range	50 - 163	Recovery	=	118.940%
35) Dibromofluoromethane	7.634	113	82543	51.488	ug/l	-0.01
Spiked Amount	50.000	Range	54 - 147	Recovery	=	102.980%
50) Toluene-d8	10.103	98	309468	50.695	ug/l	-0.01
Spiked Amount	50.000	Range	58 - 134	Recovery	=	101.400%
62) 4-Bromofluorobenzene	12.402	95	96448	45.174	ug/l	-0.01
Spiked Amount	50.000	Range	29 - 146	Recovery	=	90.340%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY121024\
Data File : VY020577.D
Acq On : 10 Dec 2024 18:30
Operator : SY/MD
Sample : P5194-05
Misc : 5.05g/5.0mL/MSVOA_Y/SOIL/A
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
WP-3


Quant Time: Dec 11 00:53:26 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y120224S.M
Quant Title : SW846 8260
QLast Update : Tue Dec 03 01:39:23 2024
Response via : Initial Calibration

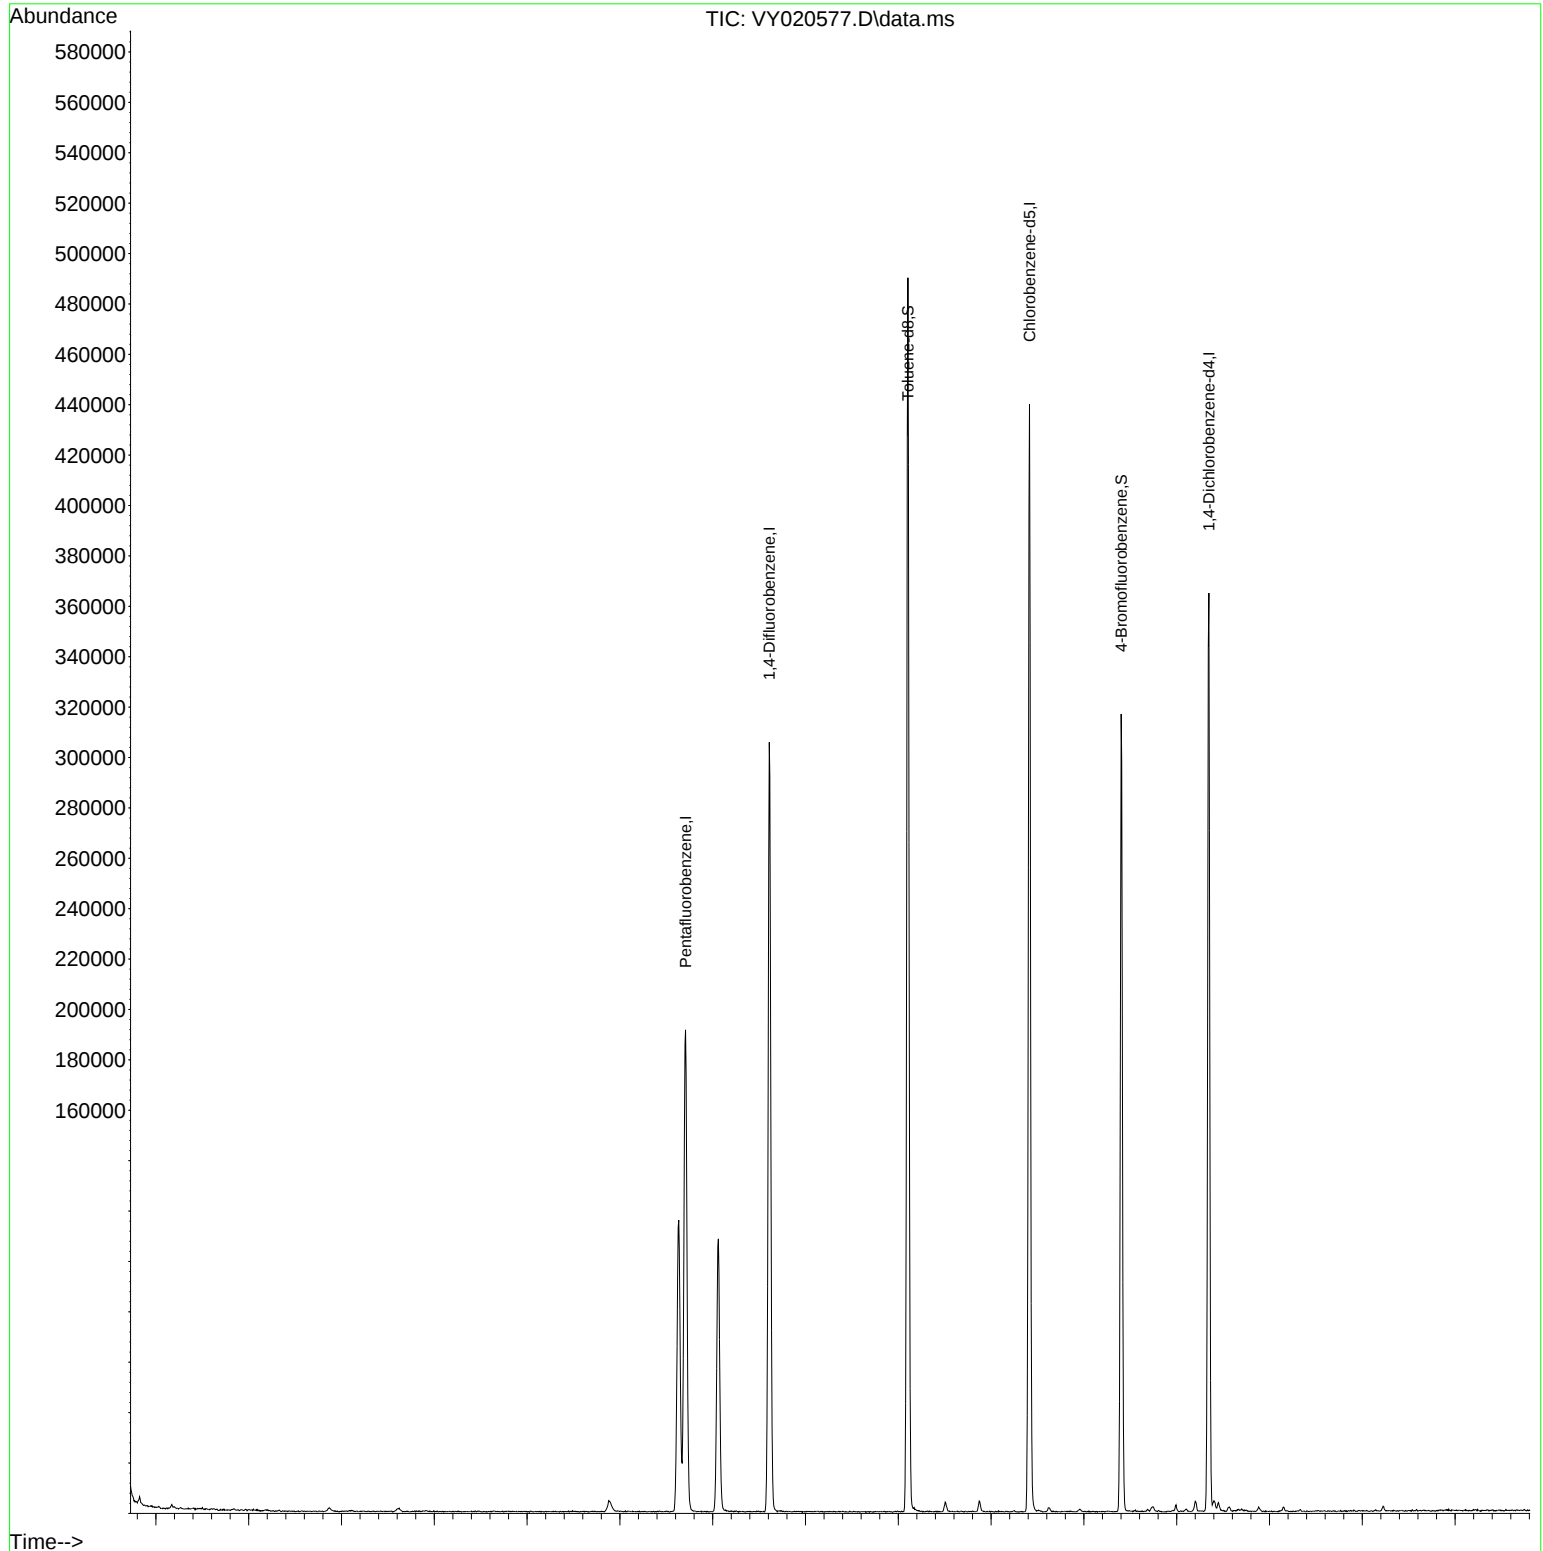



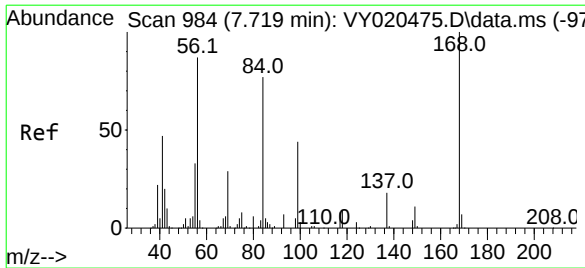


#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.707 min Scan# 98
Delta R.T. -0.012 min
Lab File: VY020577.D
Acq: 10 Dec 2024 18:30

Instrument :
MSVOA_Y
ClientSampleId :
WP-3



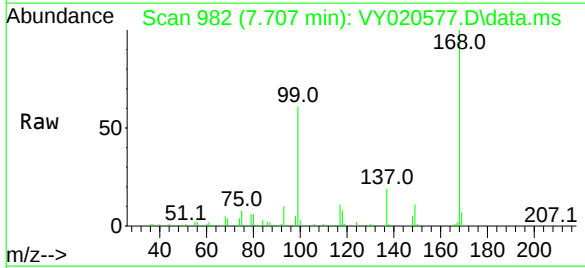



Tgt Ion:168 Resp: 144830
Ion Ratio Lower Upper
168 100
99 60.5 46.6 69.8

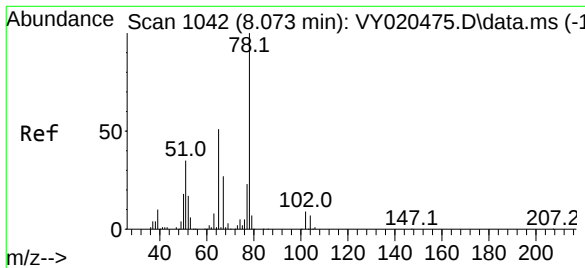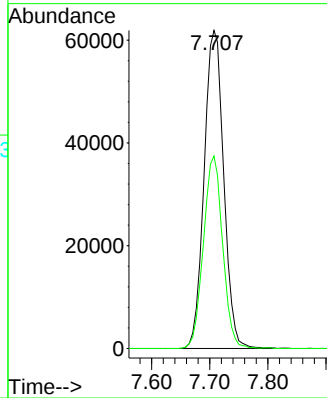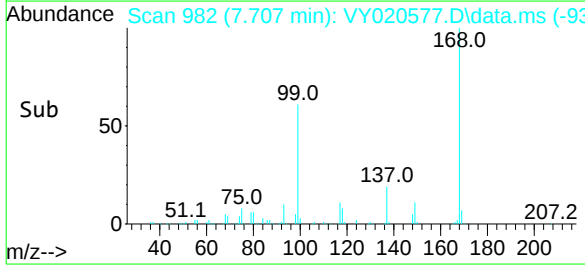

#33
1,2-Dichloroethane-d4
Concen: 59.468 ug/l
RT: 8.061 min Scan# 1040
Delta R.T. -0.012 min
Lab File: VY020577.D
Acq: 10 Dec 2024 18:30

Tgt Ion: 65 Resp: 87593
Ion Ratio Lower Upper
65 100
67 51.6 0.0 105.8


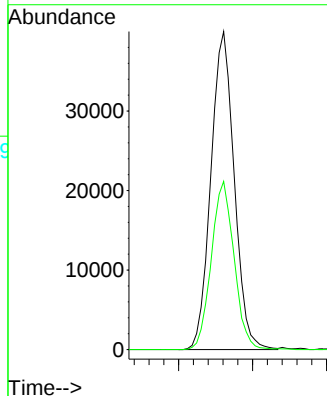
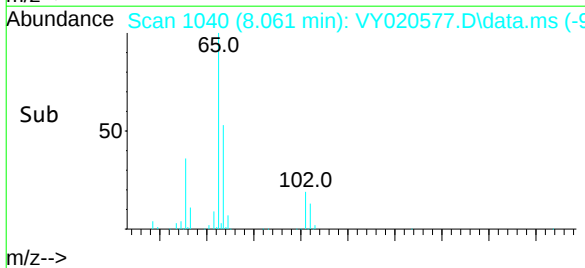
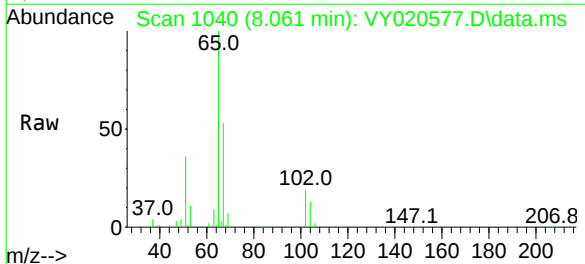


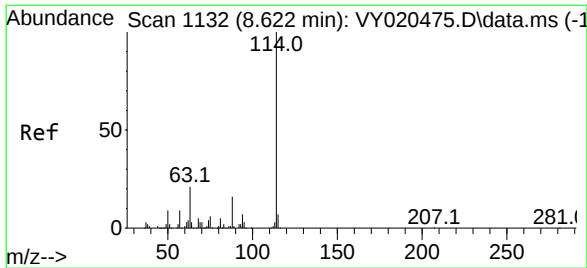

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.610 min Scan# 11
Delta R.T. -0.012 min
Lab File: VY020577.D
Acq: 10 Dec 2024 18:30




Instrument :
MSVOA_Y
ClientSampleId :
WP-3


Tgt Ion:	114	Resp:	254650
Ion	Ratio	Lower	Upper
114	100		
63	21.9	0.0	44.8
88	16.3	0.0	32.0

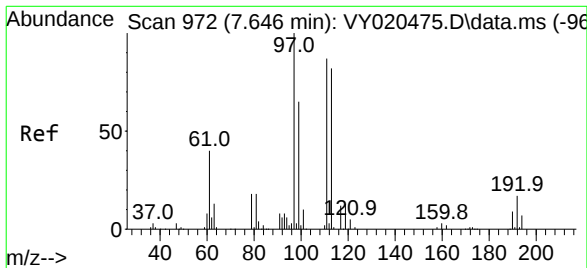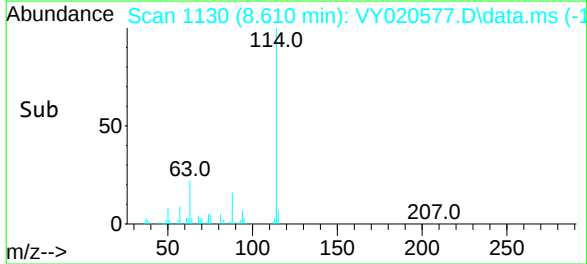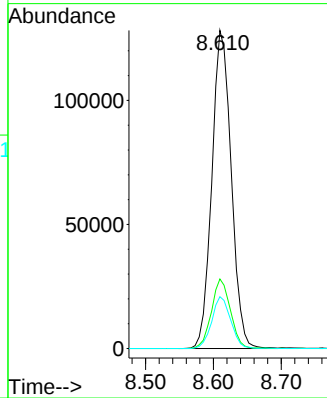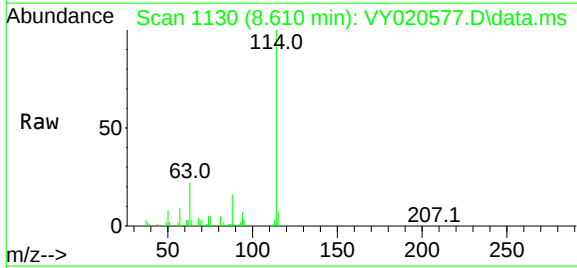

#35
Dibromofluoromethane
Concen: 51.488 ug/l
RT: 7.634 min Scan# 970
Delta R.T. -0.012 min
Lab File: VY020577.D
Acq: 10 Dec 2024 18:30

Tgt Ion:	113	Resp:	82543
Ion	Ratio	Lower	Upper
113	100		
111	104.0	81.4	122.0
192	19.2	15.1	22.7

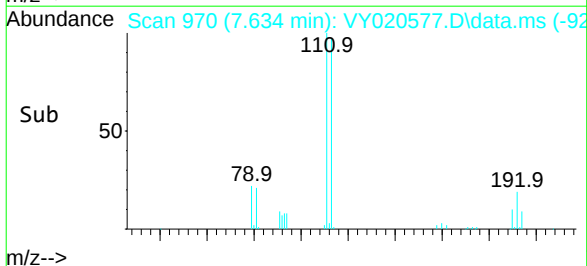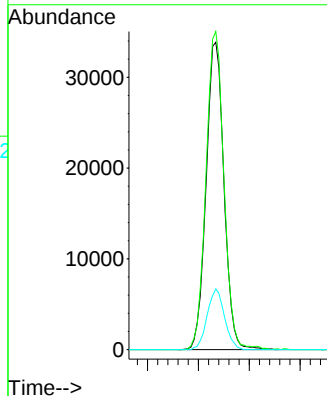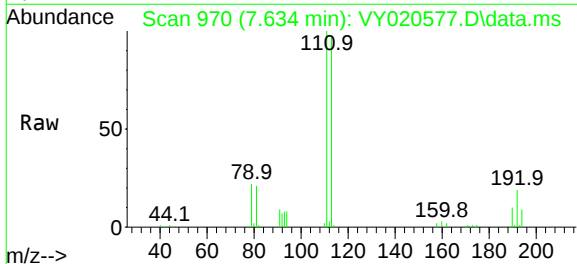

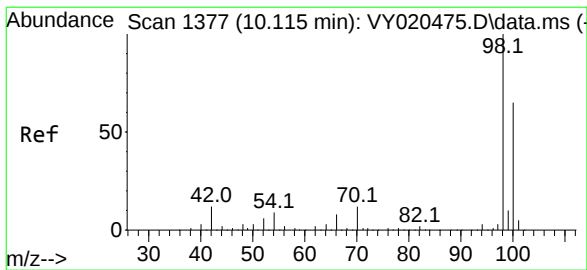

#50

Toluene-d8

Concen: 50.695 ug/l

RT: 10.103 min Scan# 1375

Delta R.T. -0.012 min

Lab File: VY020577.D

Acq: 10 Dec 2024 18:30

Instrument :

MSVOA_Y

ClientSampleId :





WP-3

Tgt Ion: 98 Resp: 309468

Ion Ratio Lower Upper

98 100

100 64.6 51.3 76.9

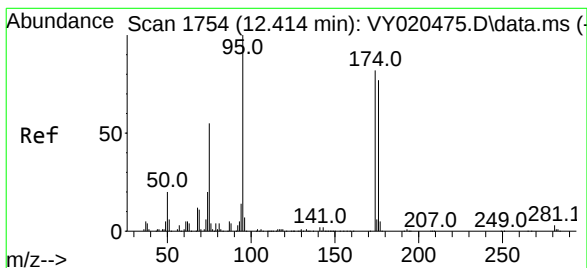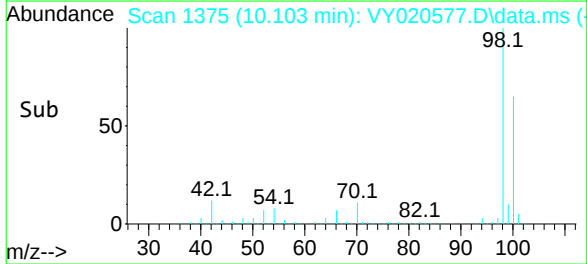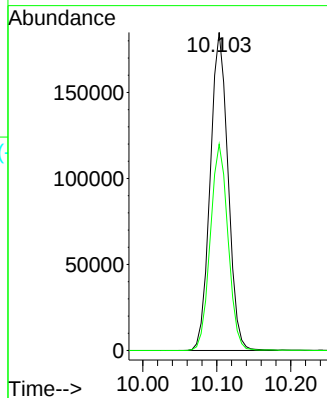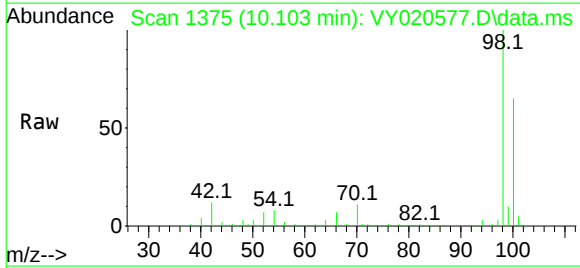

#62

4-Bromofluorobenzene

Concen: 45.174 ug/l

RT: 12.402 min Scan# 1752

Delta R.T. -0.012 min

Lab File: VY020577.D

Acq: 10 Dec 2024 18:30




Tgt Ion: 95 Resp: 96448


Ion Ratio Lower Upper

95 100

174 81.2 0.0 156.8

176 79.9 0.0 152.0

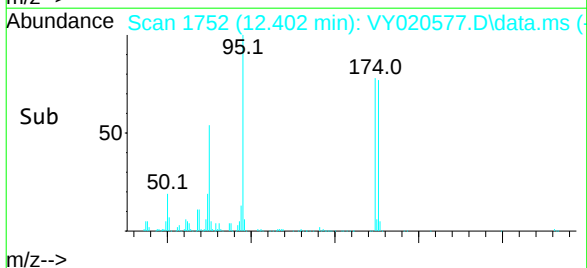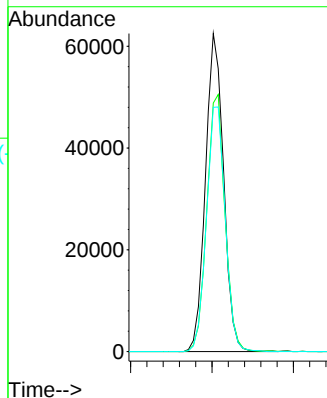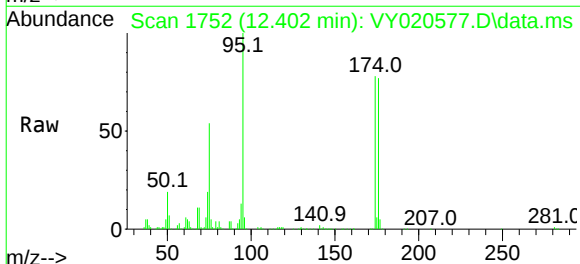

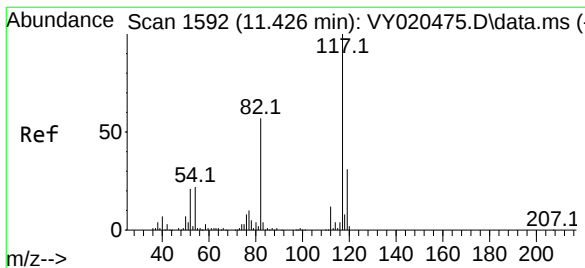

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.414 min Scan# 15

Delta R.T. -0.012 min

Lab File: VY020577.D

Acq: 10 Dec 2024 18:30

Instrument :

MSVOA_Y

ClientSampleId :

WP-3





Tgt Ion:117 Resp: 223520

Ion Ratio Lower Upper

117 100

82 55.5 48.2 72.4

119 31.9 25.8 38.8

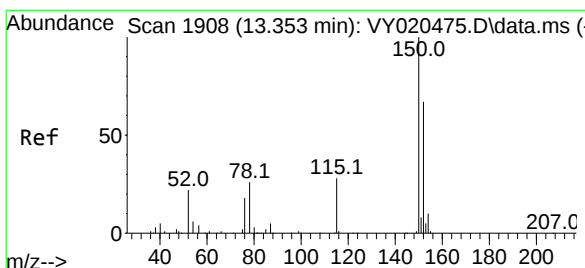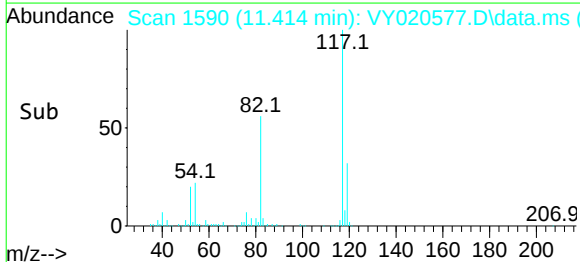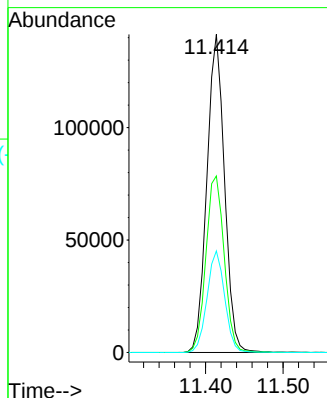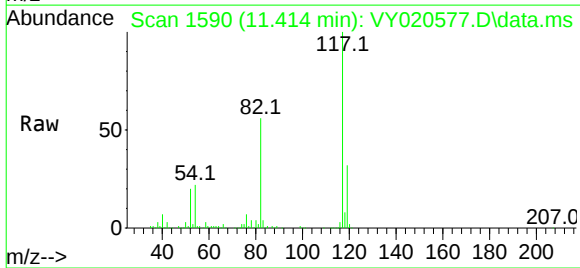

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.347 min Scan# 1907

Delta R.T. -0.006 min

Lab File: VY020577.D

Acq: 10 Dec 2024 18:30

Tgt Ion:152 Resp: 90631

Ion Ratio Lower Upper

152 100

115 59.5 30.0 90.0

150 157.4 0.0 348.2

