
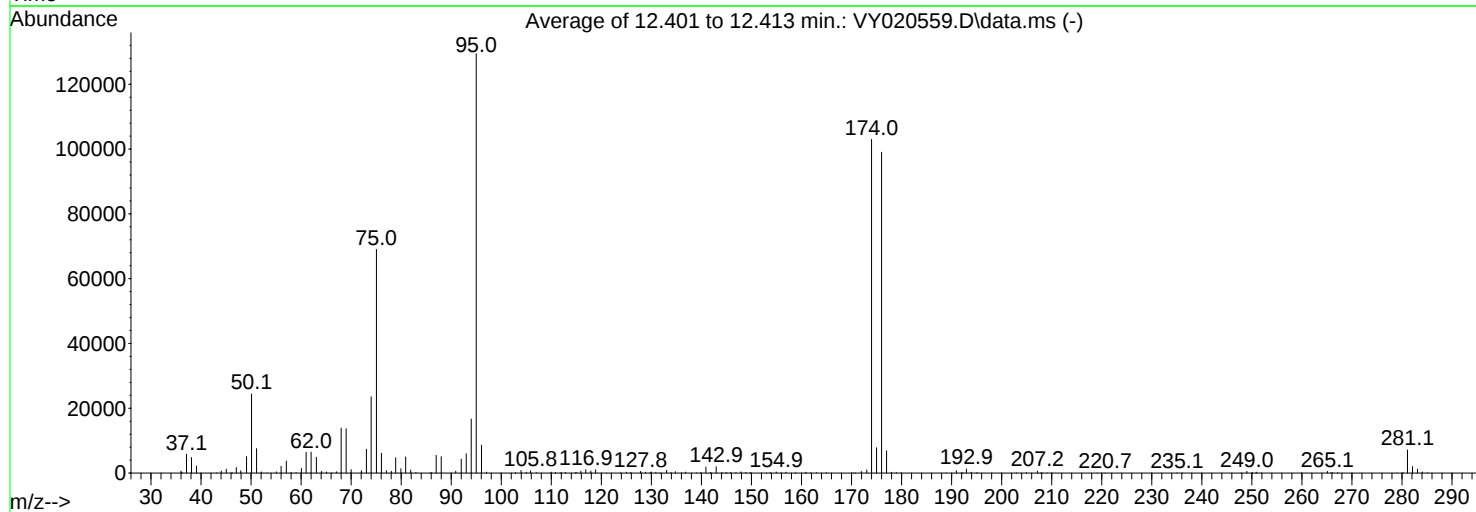


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY121024\
Data File : VY020559.D
Acq On : 10 Dec 2024 08:57
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y120224S.M
Title : SW846 8260
Last Update : Tue Dec 03 01:39:23 2024

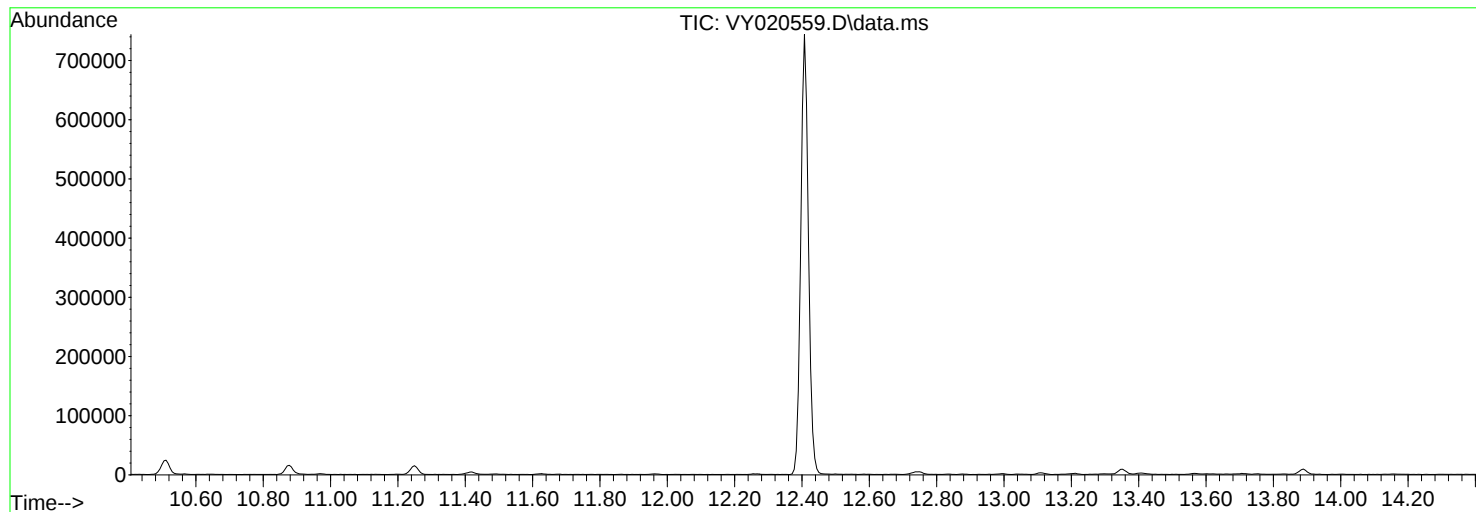

AutoFind: Scans 1752, 1753, 1754; Background Corrected with Scan 1744

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.9	24419	PASS
75	95	30	60	53.3	69019	PASS
95	95	100	100	100.0	129424	PASS
96	95	5	9	6.7	8631	PASS
173	174	0.00	2	0.9	976	PASS
174	95	50	100	79.6	102992	PASS
175	174	5	9	7.6	7803	PASS
176	174	95	101	96.2	99027	PASS
177	176	5	9	6.9	6876	PASS