

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA Y\DATA\VY121120\
 Data File : VY003732.D
 Acq On : 11 Dec 2020 17:12
 Operator : SY/MD
 Sample : L5063-04
 Misc : 4.09G/10ML/MSVOA Y/SOIL
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_Y
ClientSampleId :
 C0AD6

Manual Integrations
APPROVED

MMDadoda
 12/14/2020 9:13:23 AM

Quant Time: Dec 12 01:41:47 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\SOM2YLM120420S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 11 10:03:37 2020
 Response via : Initial Calibration

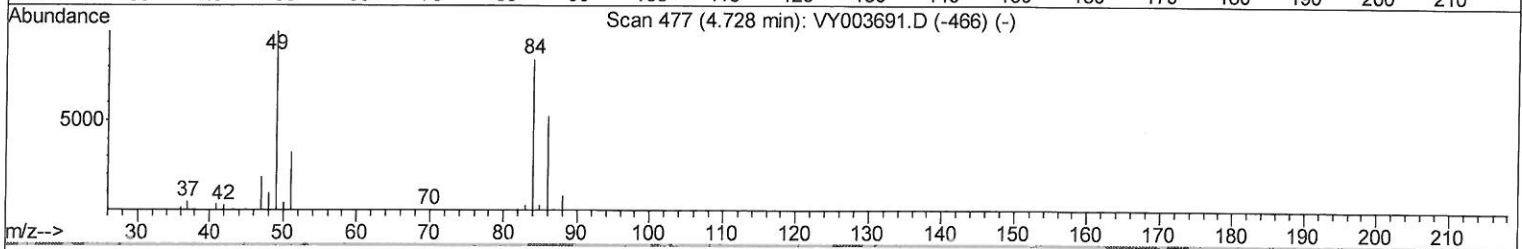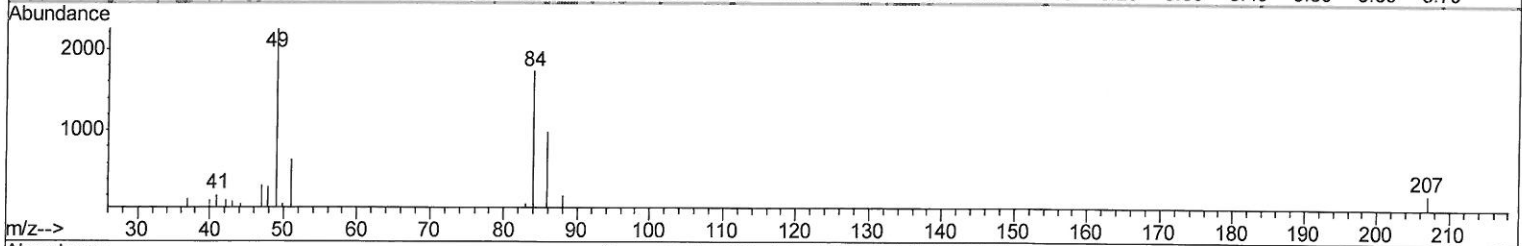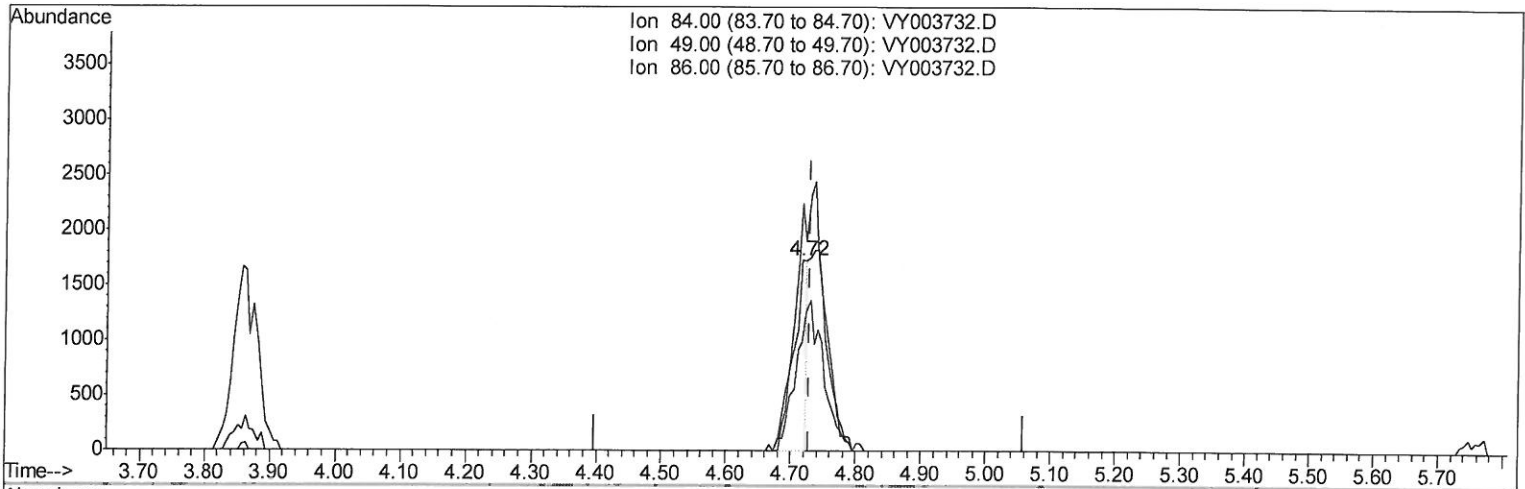

TIC: VY003732.D

(16) Methylene chloride (T)

4.716min (-0.012) 0.47ug/L

response 2495

Ion	Exp%	Act%
84.00	100	100
49.00	119.50	129.89
86.00	64.30	56.90
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA Y\DATA\VY121120\
 Data File : VY003732.D
 Acq On : 11 Dec 2020 17:12
 Operator : SY/MD
 Sample : L5063-04
 Misc : 4.09G/10ML/MSVOA Y/SOIL
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 C0AD6

Manual Integrations
 APPROVED

MMDadoda
 12/14/2020 9:13:23 AM

Quant Time: Dec 12 01:41:47 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\SOM2YLM120420S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 11 10:03:37 2020
 Response via : Initial Calibration

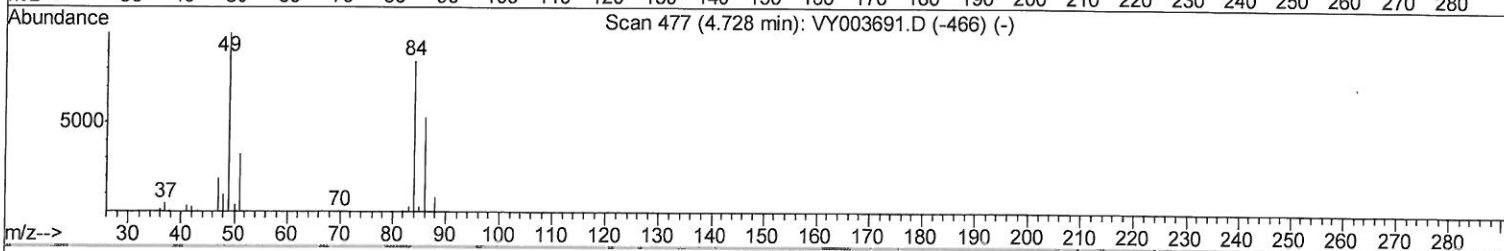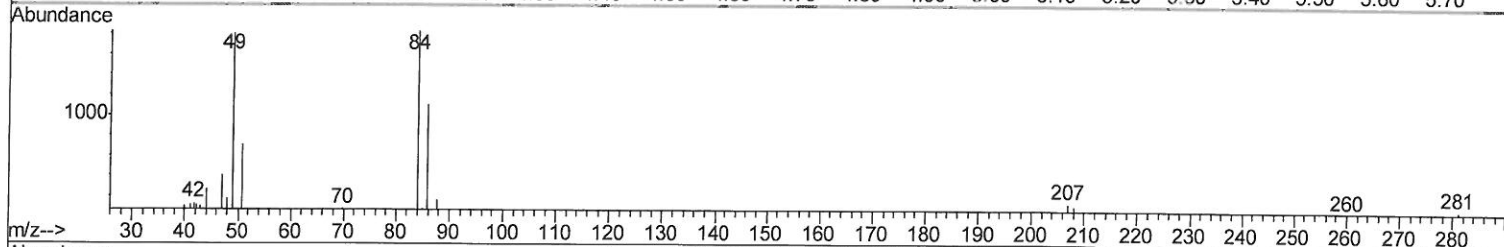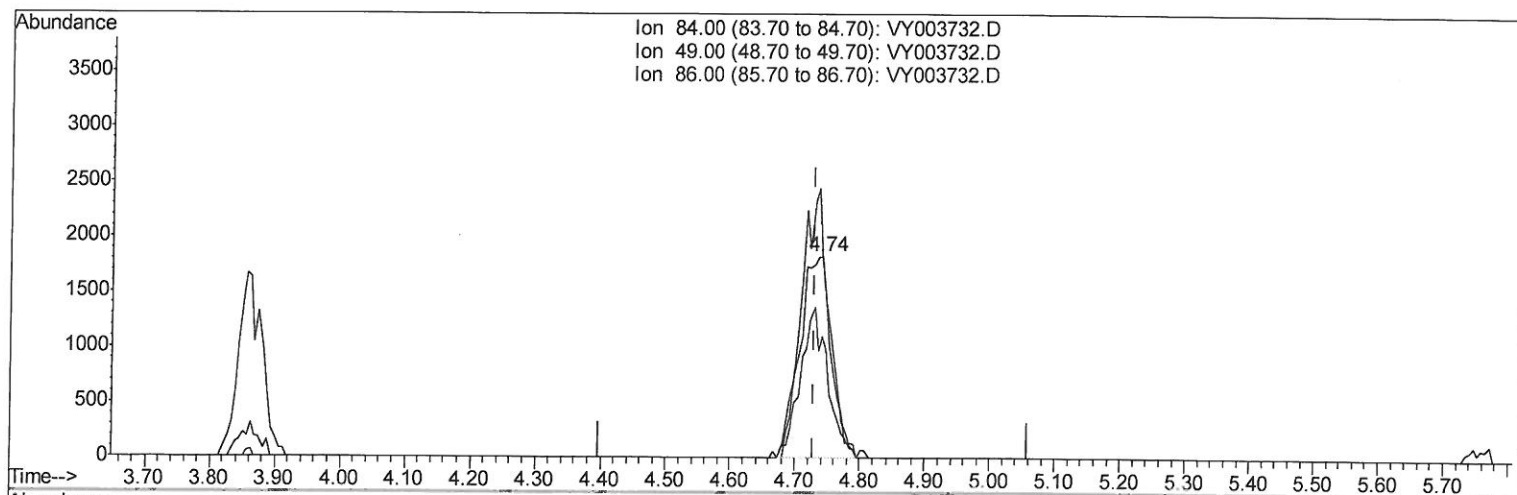

TIC: VY003732.D

(16) Methylene chloride (T)

4.741min (+0.012) 1.15ug/L m

response 6131

Ion	Exp%	Act%
84.00	100	100
49.00	119.50	98.74
86.00	64.30	60.20
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA Y\DATA\VY121120\
 Data File : VY003732.D
 Acq On : 11 Dec 2020 17:12
 Operator : SY/MD
 Sample : L5063-04
 Misc : 4.09G/10ML/MSVOA Y/SOIL
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleID :
 C0AD6

Manual Integrations
 APPROVED

MMDadoda
 12/14/2020 9:13:23 AM

Quant Time: Dec 12 04:22:01 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\SOM2YLM120420S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 11 10:03:37 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.70	114	304894	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.49	117	215150	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.42	152	54628	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.25	65	82049	19.03	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	76.12%
7) Chloroethane-d5	2.77	69	73254	22.52	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	90.08%
10) 1,1-Dichloroethene-d2	3.86	63	137365	16.93	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	67.72%
20) 2-Butanone-d5	6.90	46	71513	46.52	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	93.04%
24) Chloroform-d	7.48	84	191510	24.41	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	97.64%
26) 1,2-Dichloroethane-d4	8.15	65	106717	24.17	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	96.68%
29) Benzene-d6	8.12	84	392983	31.55	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	126.20%
33) 1,2-Dichloropropane-d6	9.12	67	119578	32.44	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	129.76%#
37) Toluene-d8	10.18	98	303868	27.21	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	108.84%
38) trans-1,3-Dichloropropene-	10.44	79	52312	29.69	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	118.76%
39) 2-Hexanone-d5	10.79	63	56227	60.89	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	121.78%
48) 1,1,2,2-Tetrachloroethane-	12.56	84	78051	23.77	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	95.08%
61) 1,2-Dichlorobenzene-d4	13.72	152	48131	24.25	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	97.00%

Target Compounds

					Ovalue
13) Acetone	3.96	43	3123	2.772	ug/L 83
14) Carbon disulfide	4.21	76	12584	1.035	ug/L 98
16) Methylene chloride	4.74	84	6131m	1.145	ug/L 87
44) Toluene	10.25	91	8979	0.692	ug/L 97
53) Ethylbenzene	11.59	91	4224	0.298	ug/L 98
54) m,p-Xylene	11.70	106	3263	0.597	ug/L 95
55) o-xylene	12.03	106	3433	0.655	ug/L 91
57) Isopropylbenzene	12.32	105	9915	0.723	ug/L # 91

(#) = qualifier out of range (m) = manual integration (+) = signals summed

12/28/2020

Data Path : Z:\VOASRV\HPCHEM1\MSVOA Y\DATA\VY121120\
Data File : VY003732.D
Acq On : 11 Dec 2020 17:12
Operator : SY/MD
Sample : L5063-04
Misc : 4.09G/10ML/MSVOA Y/SOIL
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
C0AD6

Manual Integrations
APPROVED

MMDadoda
12/14/2020 9:13:23 AM

Quant Time: Dec 12 04:22:01 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\SOM2YLM120420S.M
Quant Title : VOC Analysis
QLast Update : Fri Dec 11 10:03:37 2020
Response via : Initial Calibration

