

Data Path : Z:\VOASRV\HPCHEM1\MSVOA Y\DATA\VY121420\
 Data File : VY003754.D
 Acq On : 14 Dec 2020 17:40
 Operator : SY/MD
 Sample : VIBLK63
 Misc : 5.00G/10ML/MSVOA Y/SOIL
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VIBLK63

Quant Time: Dec 15 04:52:44 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\SOM2YLM121420S.M
 Quant Title : VOC Analysis
 QLast Update : Tue Dec 15 03:40:13 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.70	114	367069	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.49	117	347236	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.43	152	186063	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.25	65	129471	25.85	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	103.40%
7) Chloroethane-d5	2.77	69	95807	25.65	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	102.60%
10) 1,1-Dichloroethene-d2	3.86	63	193904	18.42	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	73.68%
20) 2-Butanone-d5	6.90	46	116536	53.38	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	106.76%
24) Chloroform-d	7.49	84	224485	23.55	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	94.20%
26) 1,2-Dichloroethane-d4	8.15	65	135981	25.23	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	100.92%
29) Benzene-d6	8.12	84	478763	23.82	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	95.28%
33) 1,2-Dichloropropane-d6	9.13	67	150302	24.02	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	96.08%
37) Toluene-d8	10.18	98	440388	24.21	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	96.84%
38) trans-1,3-Dichloropropene-	10.44	79	76535	25.09	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	100.36%
39) 2-Hexanone-d5	10.79	63	95033	55.07	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	110.14%
48) 1,1,2,2-Tetrachloroethane-	12.56	84	139526	25.50	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	102.00%
61) 1,2-Dichlorobenzene-d4	13.72	152	170402	25.50	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	102.00%


Target Compounds					Ovalue
13) Acetone	3.97	43	1731	1.150 ug/L	74
16) Methylene chloride	4.73	84	10610	1.610 ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA Y\DATA\VY121420\
Data File : VY003754.D
Acq On : 14 Dec 2020 17:40
Operator : SY/MD
Sample : VIBLK63
Misc : 5.00G/10ML/MSVOA Y/SOIL
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VIBLK63

Quant Time: Dec 15 04:52:44 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_Y\METHODS\SOM2YLM121420S.M
Quant Title : VOC Analysis
QLast Update : Tue Dec 15 03:40:13 2020
Response via : Initial Calibration




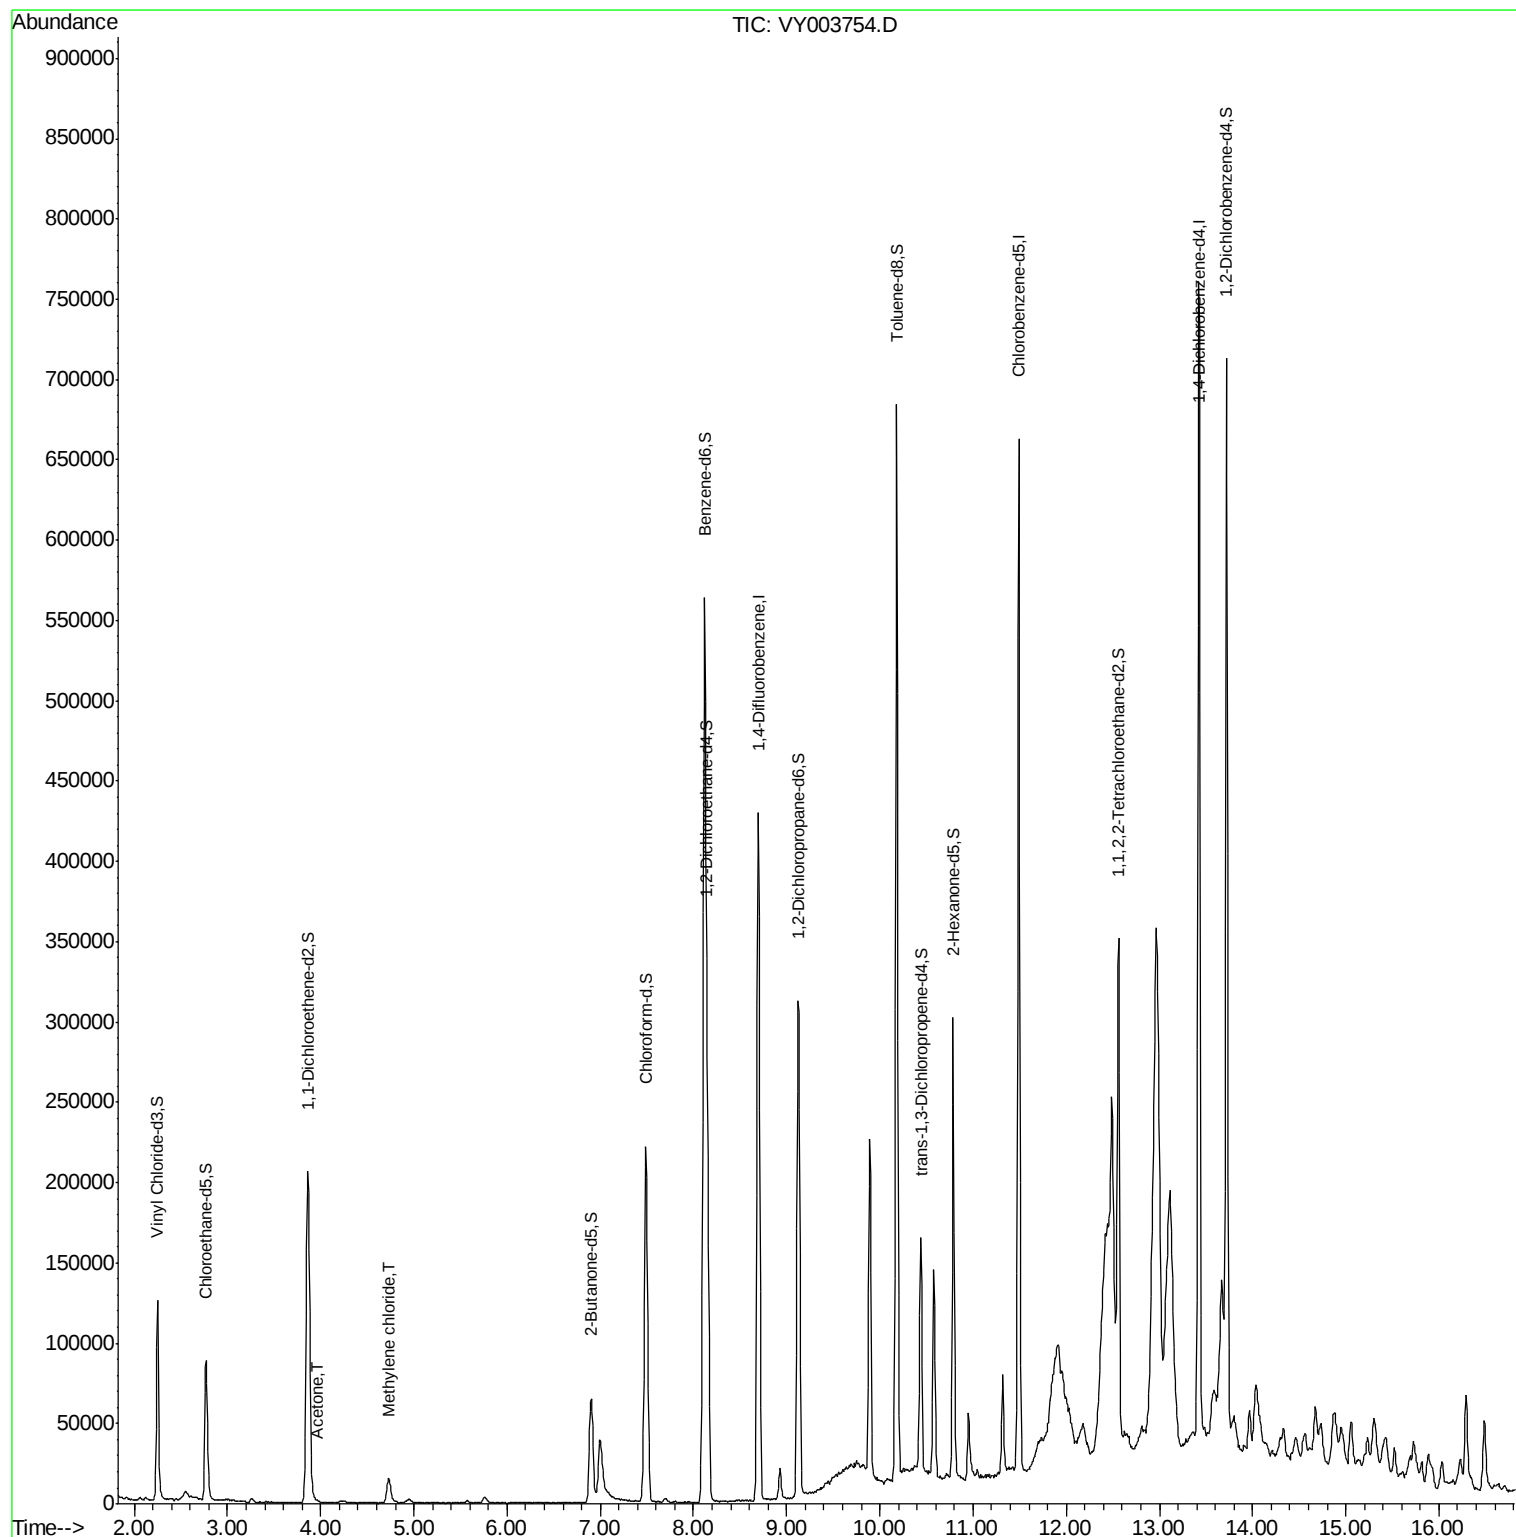


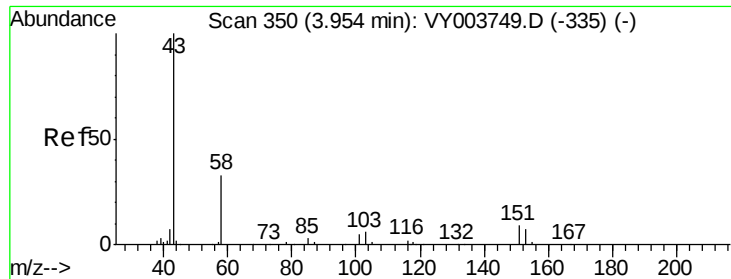

#13
Acetone
Concen: 1.150 ug/L
RT: 3.97 min Scan# 352
Delta R.T. 0.01 min
Lab File: VY003754.D
Acq: 14 Dec 2020 17:40

Instrument :
MSVOA_Y
ClientSampleId :
VIBLK63

Tot Ion: 43 Resp: 1731
Ion Ratio Lower Upper
43 100
58 17.9 0.0 65.4

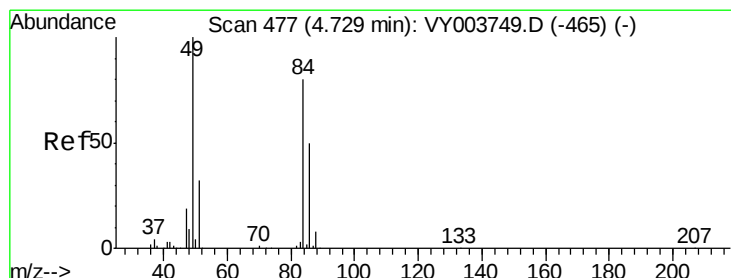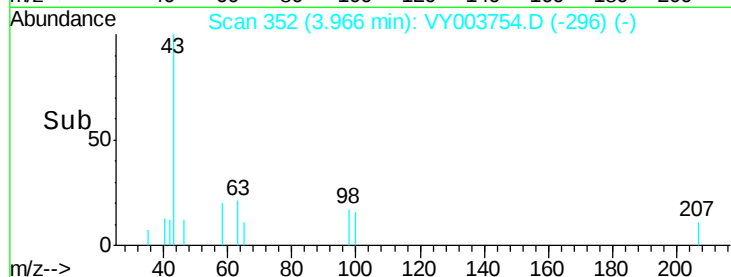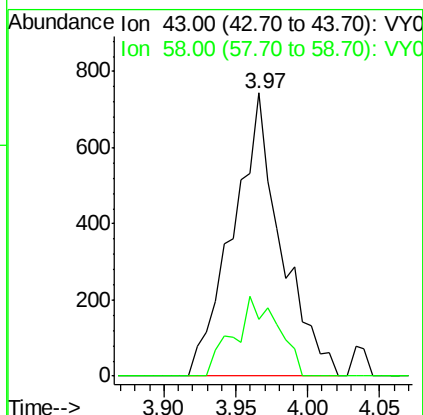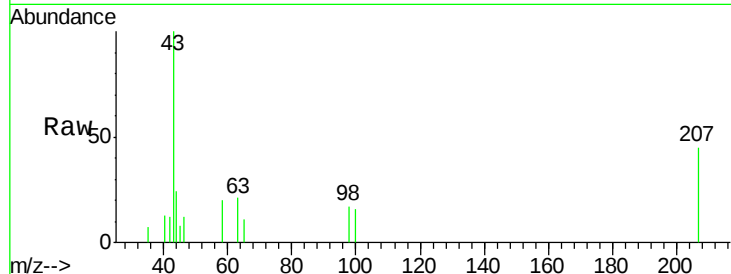

#16
Methylene chloride
Concen: 1.610 ug/L
RT: 4.73 min Scan# 477
Delta R.T. -0.00 min
Lab File: VY003754.D
Acq: 14 Dec 2020 17:40

Tgt Ion: 84 Resp: 10610
Ion Ratio Lower Upper
84 100
49 140.2 88.2 163.8
86 59.5 43.0 79.8

