

Data Path : Z:\VOASRV\HPCHEM1\MSVOA Y\DATA\VY121420\
 Data File : VY003763.D
 Acq On : 14 Dec 2020 21:28
 Operator : SY/MD
 Sample : L4980-10
 Misc : 5.00G/10ML/MSVOA Y/SOIL
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VHBLK01

Quant Time: Dec 15 05:27:42 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\SOM2YLM121420S.M
 Quant Title : VOC Analysis
 QLast Update : Tue Dec 15 03:40:13 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.70	114	337993	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.49	117	314205	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.42	152	160464	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.25	65	116870	25.34	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	101.36%
7) Chloroethane-d5	2.77	69	90276	26.25	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	105.00%
10) 1,1-Dichloroethene-d2	3.86	63	174615	18.02	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	72.08%
20) 2-Butanone-d5	6.90	46	106172	52.82	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	105.64%
24) Chloroform-d	7.49	84	213939	24.37	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	97.48%
26) 1,2-Dichloroethane-d4	8.15	65	131867	26.57	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	106.28%
29) Benzene-d6	8.12	84	447179	24.59	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	98.36%
33) 1,2-Dichloropropane-d6	9.12	67	139476	24.63	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	98.52%
37) Toluene-d8	10.18	98	410844	24.96	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	99.84%
38) trans-1,3-Dichloropropene-	10.44	79	70029	25.37	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	101.48%
39) 2-Hexanone-d5	10.79	63	82037	52.53	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	105.06%
48) 1,1,2,2-Tetrachloroethane-	12.56	84	125191	25.29	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	101.16%
61) 1,2-Dichlorobenzene-d4	13.72	152	154580	26.82	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	107.28%


Target Compounds					Ovalue
16) Methylene chloride	4.73	84	9441	1.556 ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA Y\DATA\VY121420\
Data File : VY003763.D
Acq On : 14 Dec 2020 21:28
Operator : SY/MD
Sample : L4980-10
Misc : 5.00G/10ML/MSVOA Y/SOIL
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VHBLK01

Quant Time: Dec 15 05:27:42 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_Y\METHODS\SOM2YLM121420S.M
Quant Title : VOC Analysis
QLast Update : Tue Dec 15 03:40:13 2020
Response via : Initial Calibration

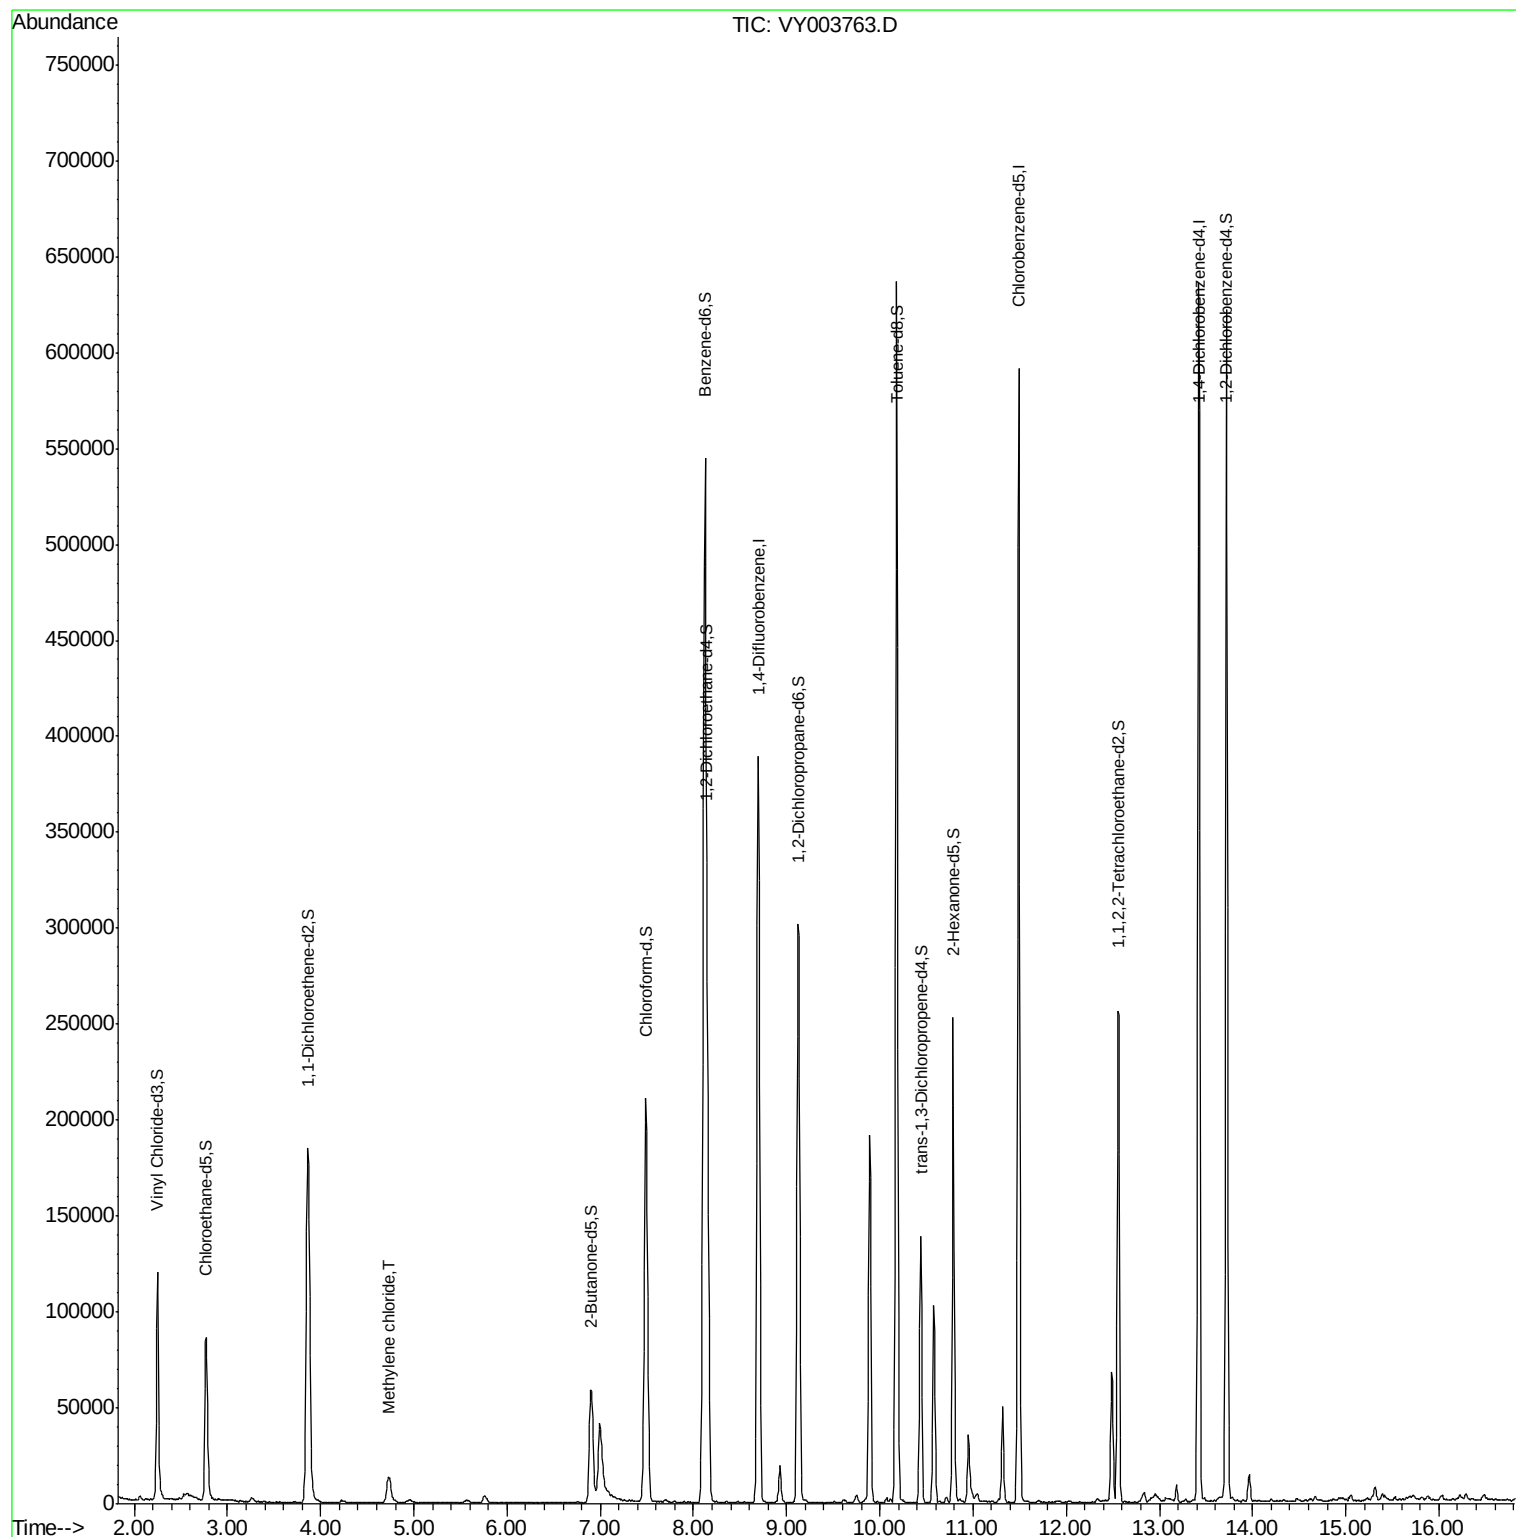

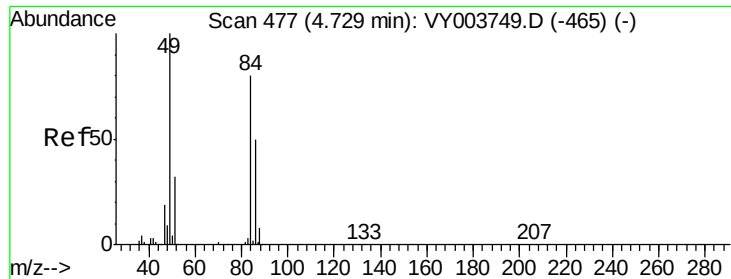

#16
 Methvlene chloride
 Concen: 1.556 ug/L
 RT: 4.73 min Scan# 477
 Delta R.T. -0.00 min
 Lab File: VY003763.D
 Acq: 14 Dec 2020 21:28

Instrument :
 MSVOA_Y
 ClientSampleId :
 VHBLK01

Tot Ion: 84 Resp: 9441
 Ion Ratio Lower Upper
 84 100
 49 131.6 88.2 163.8
 86 63.2 43.0 79.8

