


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY121525\
Data File : VY023962.D
Acq On : 15 Dec 2025 07:00
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y121025S.M
Title : SW846 8260
Last Update : Thu Dec 11 03:57:51 2025

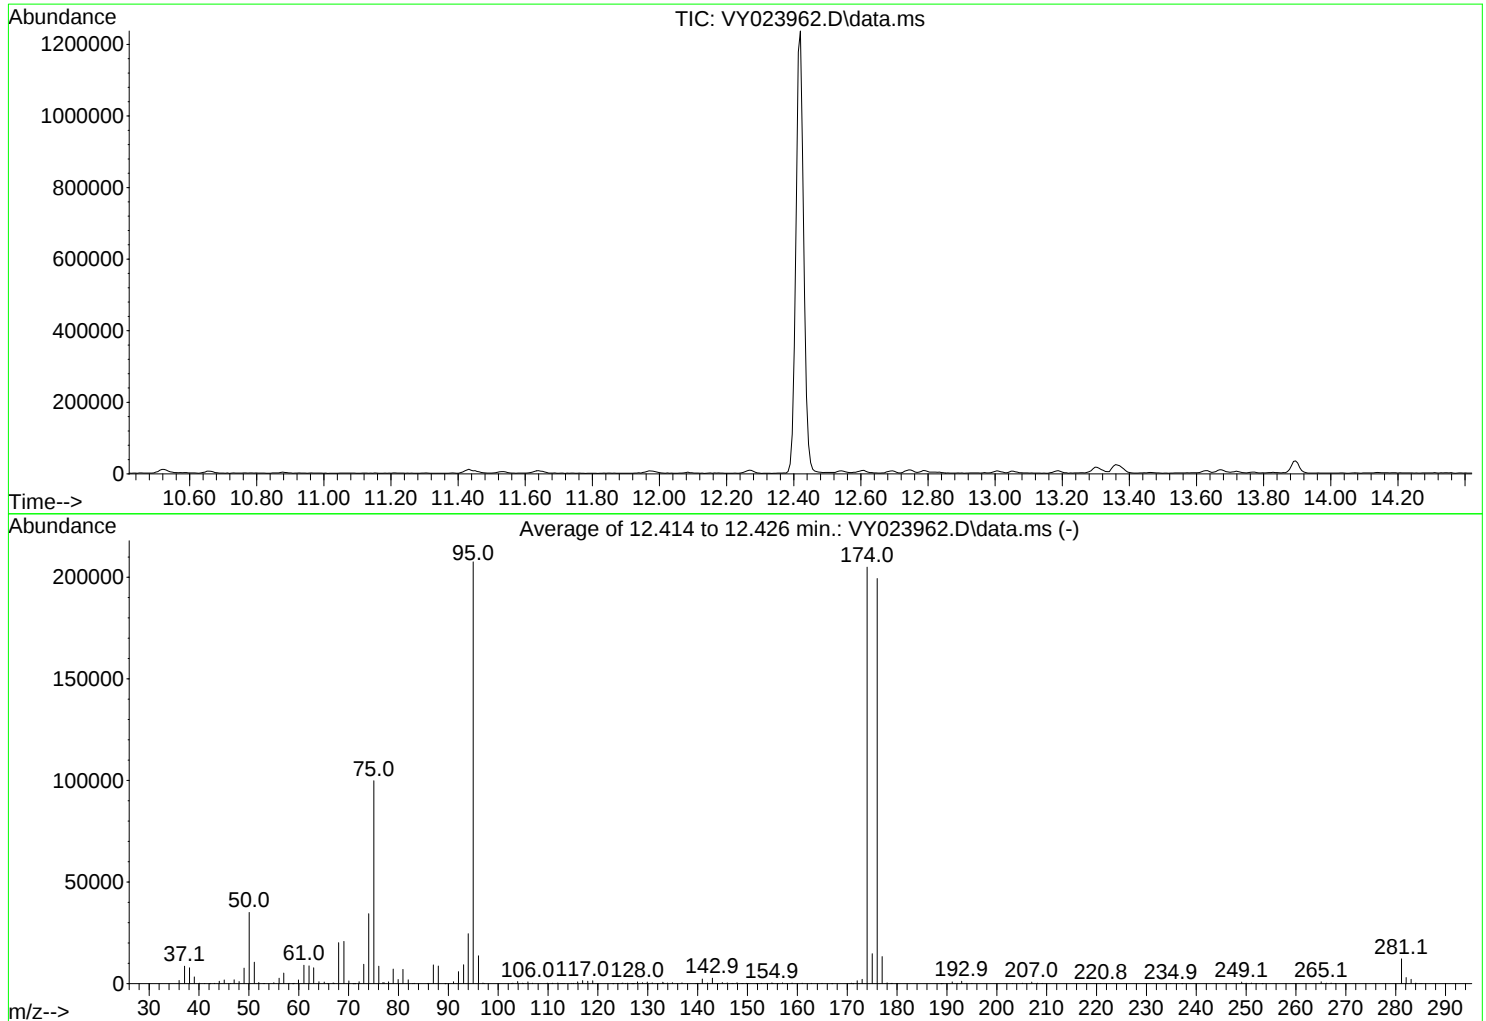

AutoFind: Scans 1754, 1755, 1756; Background Corrected with Scan 1745

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.9	35053	PASS
75	95	30	60	48.1	99837	PASS
95	95	100	100	100.0	207616	PASS
96	95	5	9	6.6	13743	PASS
173	174	0.00	2	1.1	2153	PASS
174	95	50	100	98.7	204992	PASS
175	174	5	9	7.2	14750	PASS
176	174	95	101	97.3	199424	PASS
177	176	5	9	6.7	13286	PASS