

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY121620\
 Data File : VY003801.D
 Acq On : 16 Dec 2020 13:52
 Operator : SY/MD
 Sample : L5118-01
 Misc : 3.47G/5ML/MSVOA_Y/SOIL
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 R-LA-37-2-WC

Quant Time: Dec 17 02:52:27 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y121520S.M
 Quant Title : Sw846 8260
 QLast Update : Wed Dec 16 05:00:50 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.801	168	192761	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.697	114	333705	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.489	117	307341	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.422	152	142982	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.148	65	114880	48.06	ug/l	0.00
Spiked Amount 50.000	Range 50 - 163		Recovery =	96.12%		
35) Dibromofluoromethane	7.728	113	103593	42.91	ug/l	0.00
Spiked Amount 50.000	Range 54 - 147		Recovery =	85.82%		
50) Toluene-d8	10.179	98	401201	41.98	ug/l	0.00
Spiked Amount 50.000	Range 49 - 140		Recovery =	83.96%		
62) 4-Bromofluorobenzene	12.483	95	127689	38.89	ug/l	0.00
Spiked Amount 50.000	Range 25 - 144		Recovery =	77.78%		


Target Compounds Qvalue


 (#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY121620\
Data File : VY003801.D
Acq On : 16 Dec 2020 13:52
Operator : SY/MD
Sample : L5118-01
Misc : 3.47G/5ML/MSVOA_Y/SOIL
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
R-LA-37-2-WC

Quant Time: Dec 17 02:52:27 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y121520S.M
Quant Title : SW846 8260
QLast Update : Wed Dec 16 05:00:50 2020
Response via : Initial Calibration




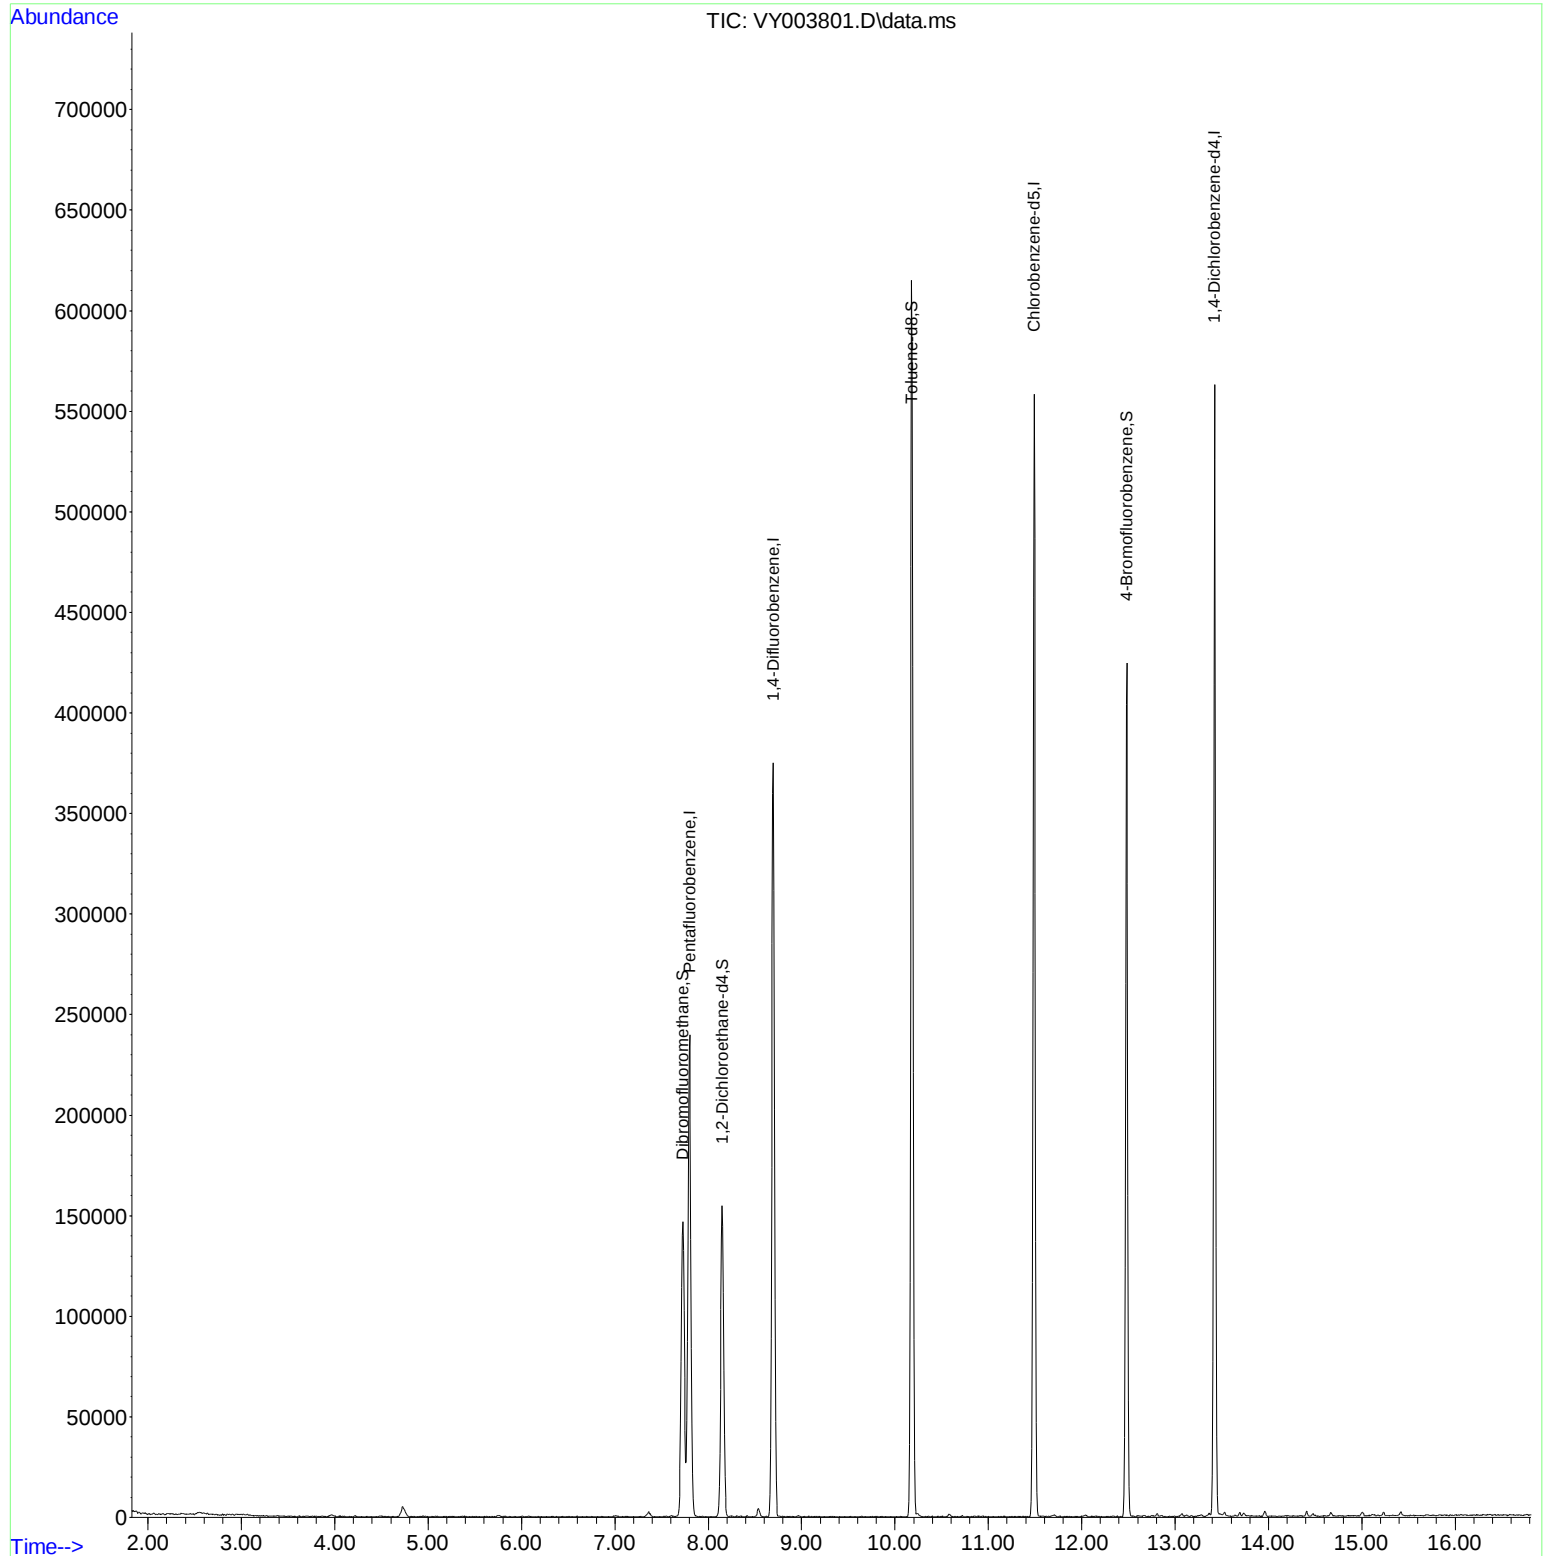


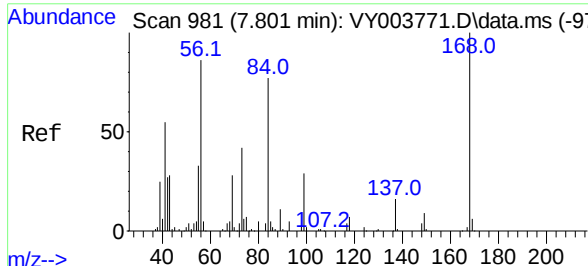

Pentafluorobenzene
 Concen: 50.00 ug/l
 RT: 7.801 min Scan# 981
 Delta R.T. -0.000 min
 Lab File: VY003801.D
 Acq: 16 Dec 2020 13:52




Instrument :
 MSVOA_Y
 ClientSampleId :
 R-LA-37-2-WC

Tgt Ion:168 Resp: 192761
 Ion Ratio Lower Upper
 168 100
 99 48.1 41.9 62.9

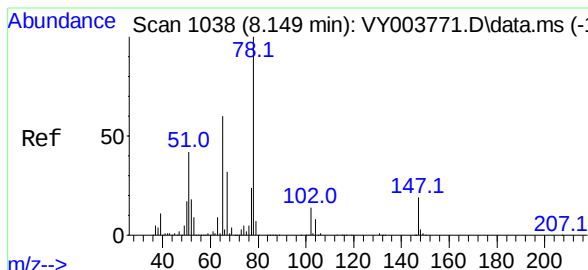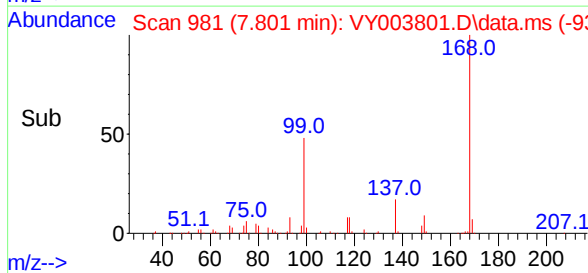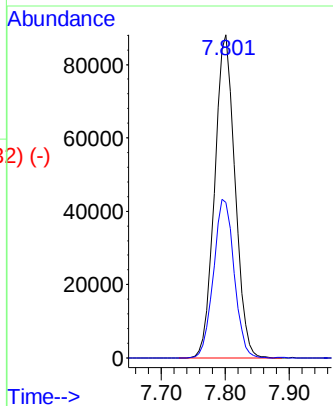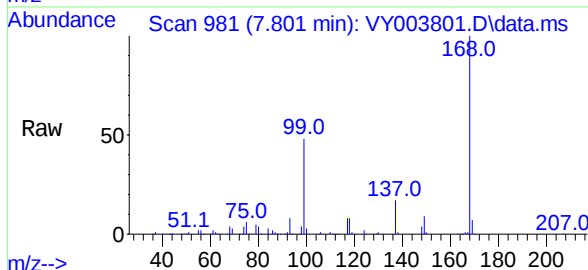


1,2-Dichloroethane-d4
 Concen: 48.06 ug/l
 RT: 8.148 min Scan# 1038
 Delta R.T. -0.000 min
 Lab File: VY003801.D
 Acq: 16 Dec 2020 13:52

Tgt Ion: 65 Resp: 114880
 Ion Ratio Lower Upper
 65 100
 67 54.0 0.0 107.6

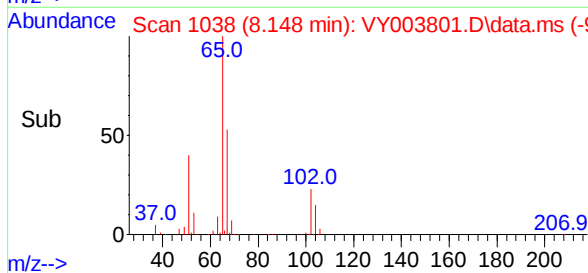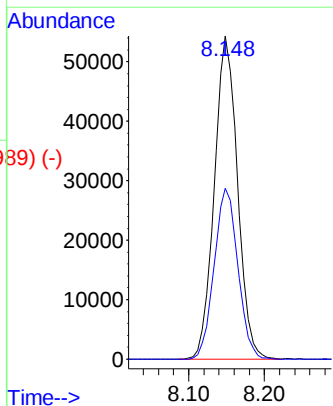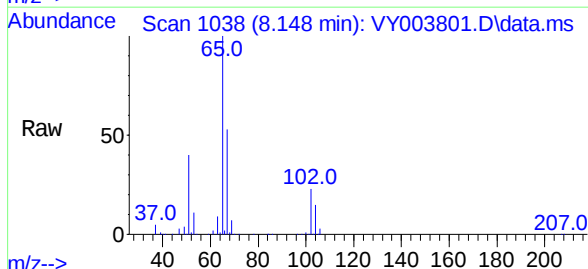




Abundance Scan 1128 (8.697 min): VY003771.D\data.ms (-1118)

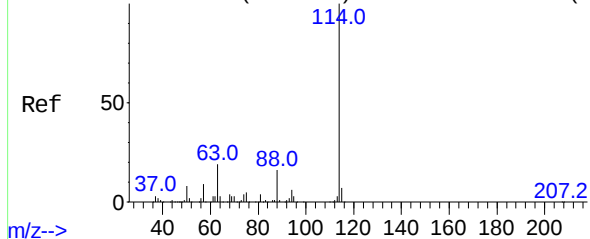


1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 8.697 min Scan# 1128
Delta R.T. -0.000 min
Lab File: VY003801.D
Acq: 16 Dec 2020 13:52

Instrument :
MSVOA_Y
ClientSampled :
R-LA-37-2-WC

Tgt Ion:	114	Resp:	333705
Ion	Ratio	Lower	Upper
114	100		
63	18.5	0.0	38.4
88	14.9	0.0	31.8

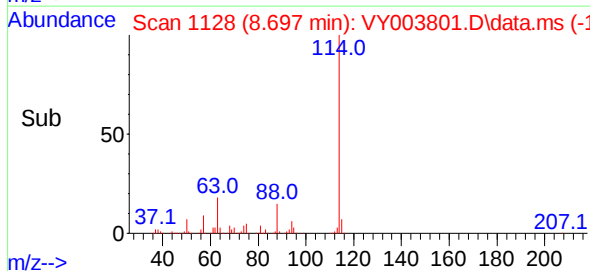
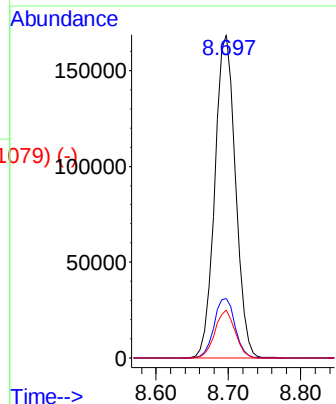
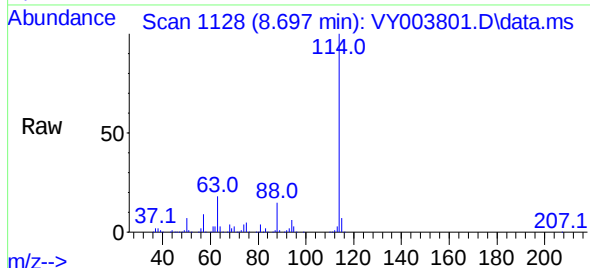



Abundance Scan 969 (7.728 min): VY003771.D\data.ms (-958)

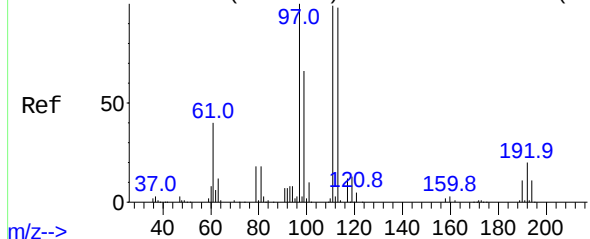

Dibromofluoromethane
Concen: 42.91 ug/l
RT: 7.728 min Scan# 969
Delta R.T. -0.000 min
Lab File: VY003801.D
Acq: 16 Dec 2020 13:52

Tgt Ion:	113	Resp:	103593
Ion	Ratio	Lower	Upper
113	100		
111	100.7	82.2	123.2
192	21.8	16.7	25.1


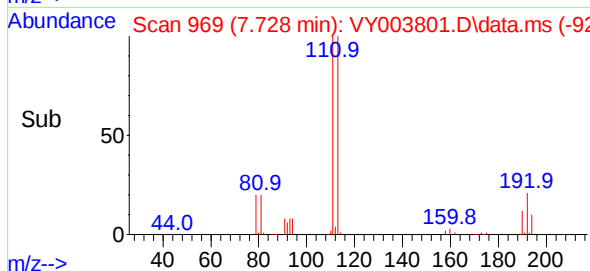
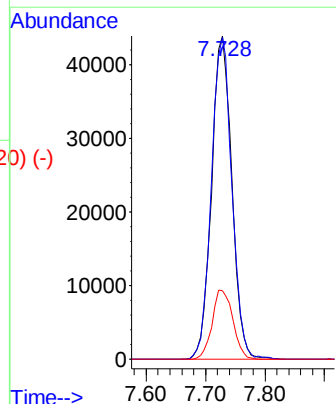
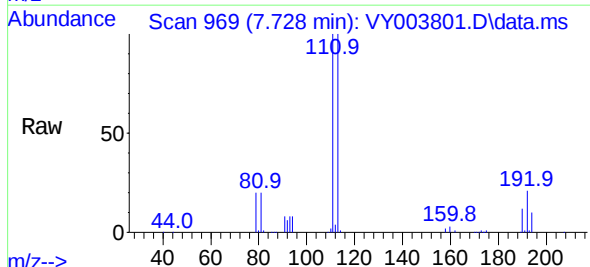


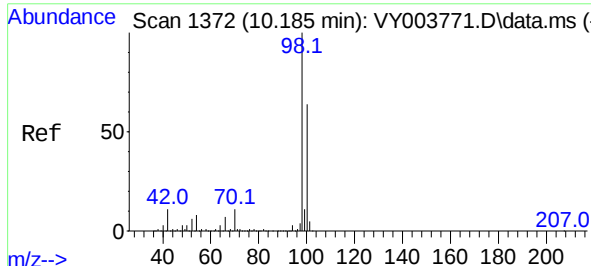

Toluene-d8
Concen: 41.98 ug/l
RT: 10.179 min Scan# 1371
Delta R.T. -0.006 min
Lab File: VY003801.D
Acq: 16 Dec 2020 13:52




Instrument :
MSVOA_Y
ClientSampleId :
R-LA-37-2-WC


Tgt Ion: 98 Resp: 401201
Ion Ratio Lower Upper
98 100
100 64.7 51.6 77.4

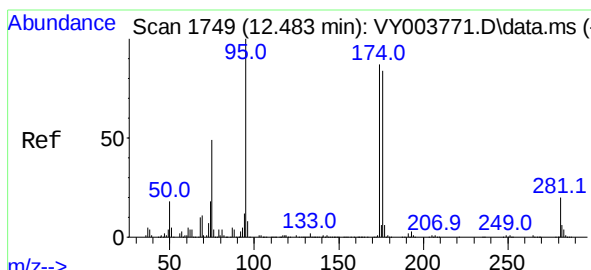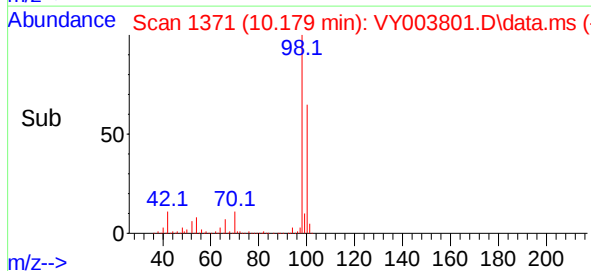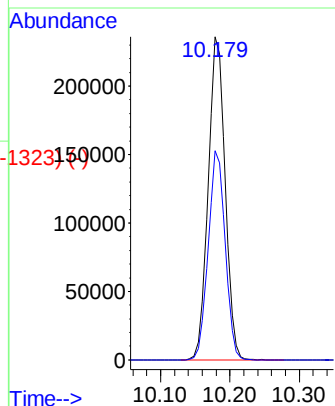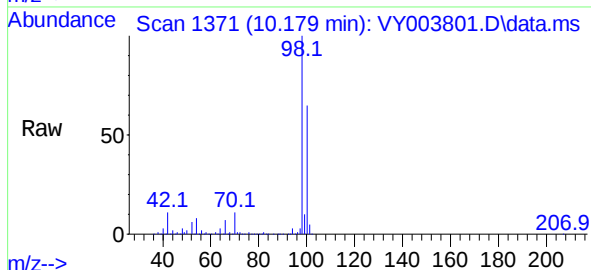

4-Bromofluorobenzene
Concen: 38.89 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. -0.000 min
Lab File: VY003801.D
Acq: 16 Dec 2020 13:52

Tgt Ion: 95 Resp: 127689
Ion Ratio Lower Upper
95 100
174 90.8 0.0 170.8
176 88.0 0.0 165.0


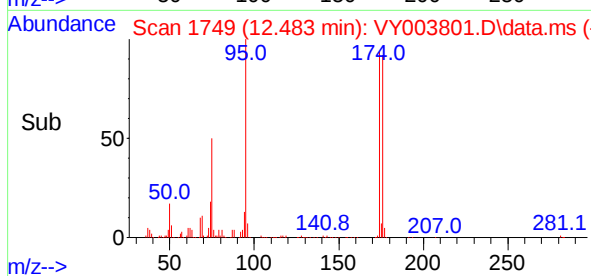
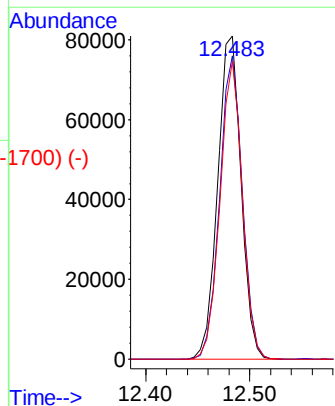
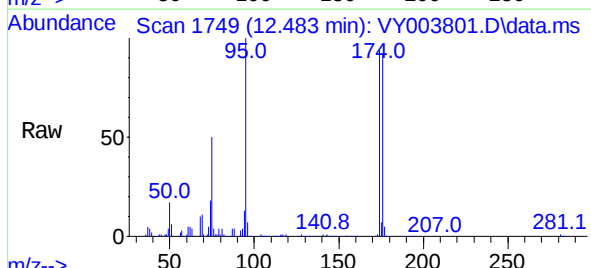


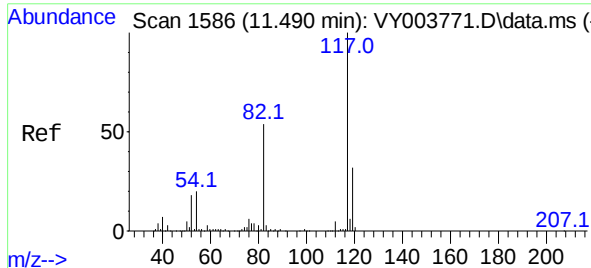

#63 (-)
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.489 min Scan# 1586
Delta R.T. -0.000 min
Lab File: VY003801.D
Acq: 16 Dec 2020 13:52

Instrument :
MSVOA_Y
ClientSampleId :
R-LA-37-2-WC

Tgt Ion:	117	Resp:	307341
Ion	Ratio	Lower	Upper
117	100		
82	53.8	43.0	64.6
119	31.0	25.7	38.5

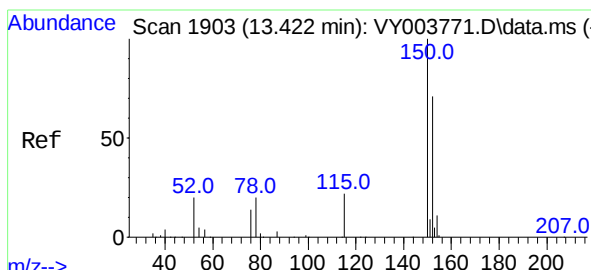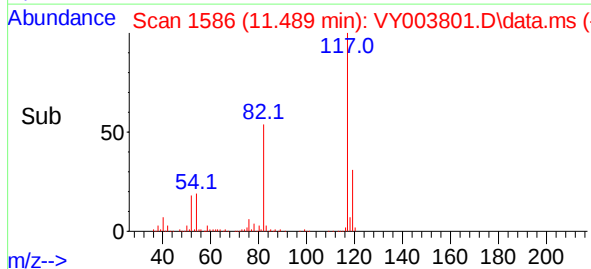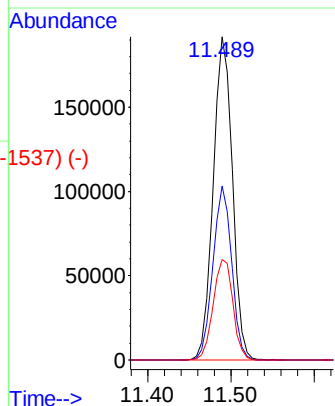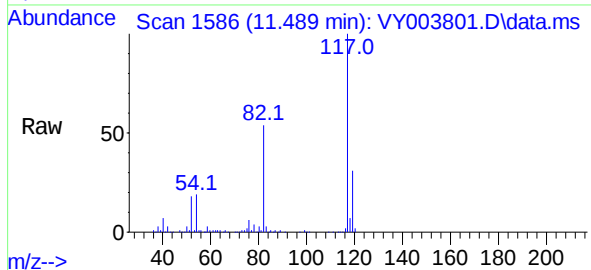

#63 (-)
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.422 min Scan# 1903
Delta R.T. -0.000 min
Lab File: VY003801.D
Acq: 16 Dec 2020 13:52

Tgt Ion:	152	Resp:	142982
Ion	Ratio	Lower	Upper
152	100		
115	55.0	28.0	83.9
150	159.0	0.0	347.6

