
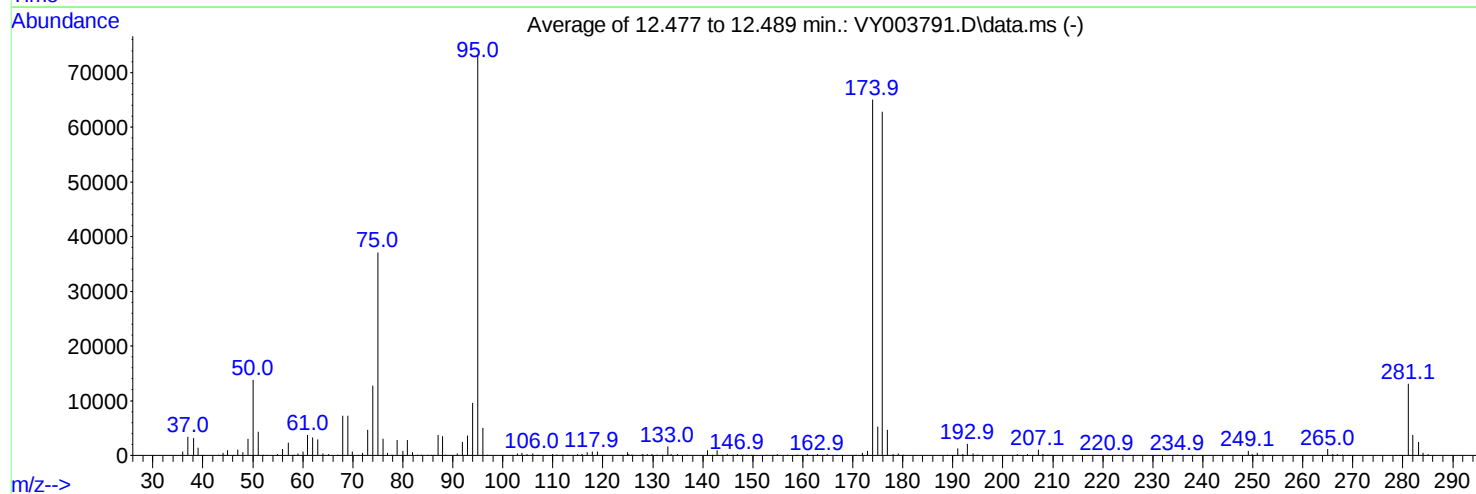


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY121620\
 Data File : VY003791.D
 Acq On : 16 Dec 2020 09:13
 Operator : SY/MD
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA_Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y121520S.M
 Title : SW846 8260
 Last Update : Wed Dec 16 05:00:50 2020

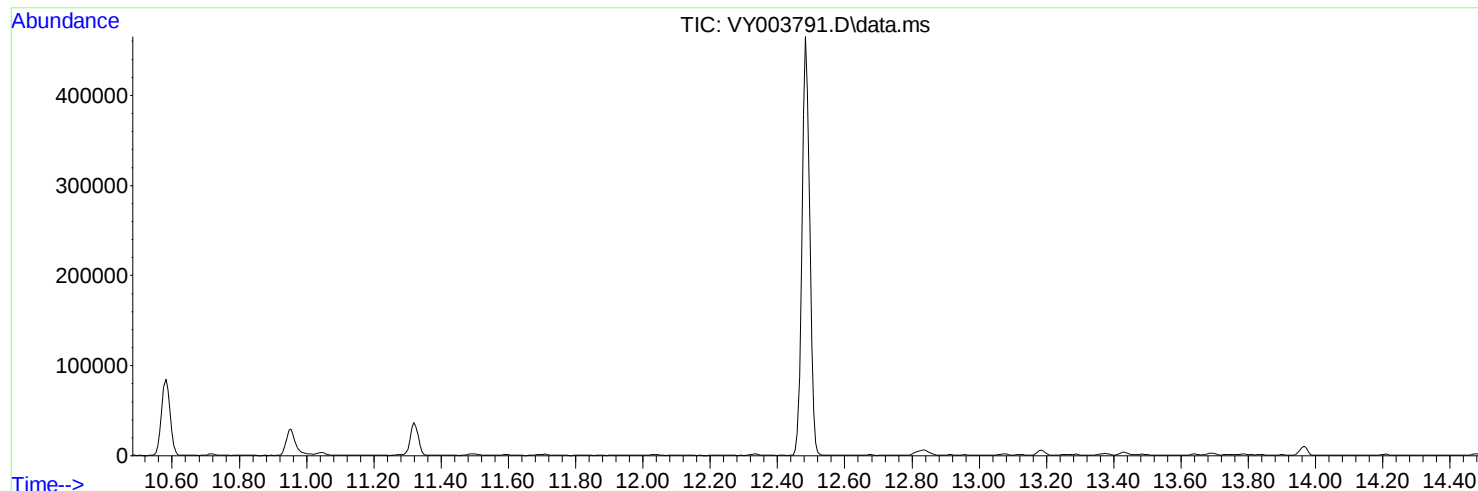

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.0	13842	PASS
75	95	30	60	50.9	37147	PASS
95	95	100	100	100.0	72987	PASS
96	95	5	9	6.9	5053	PASS
173	174	0.00	2	1.2	789	PASS
174	95	50	100	89.1	65005	PASS
175	174	5	9	8.1	5295	PASS
176	174	95	101	96.6	62779	PASS
177	176	5	9	7.5	4685	PASS