
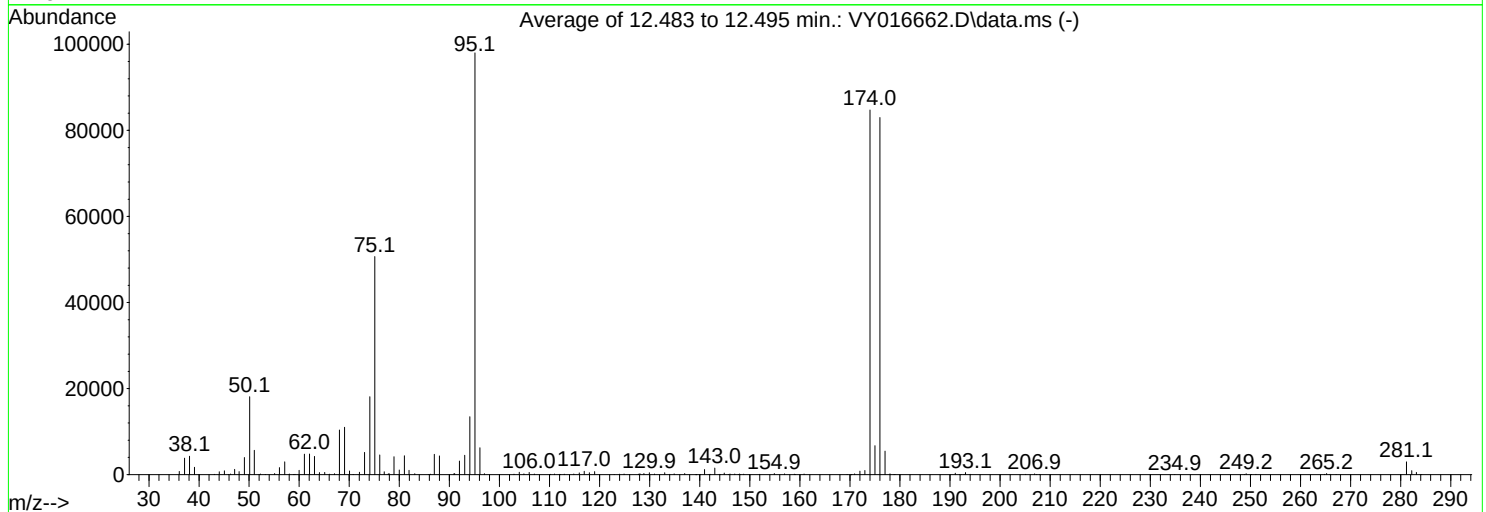


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY121623\
Data File : VY016662.D
Acq On : 16 Dec 2023 09:40
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y121523S.M
Title : SW846 8260
Last Update : Sat Dec 16 00:39:52 2023

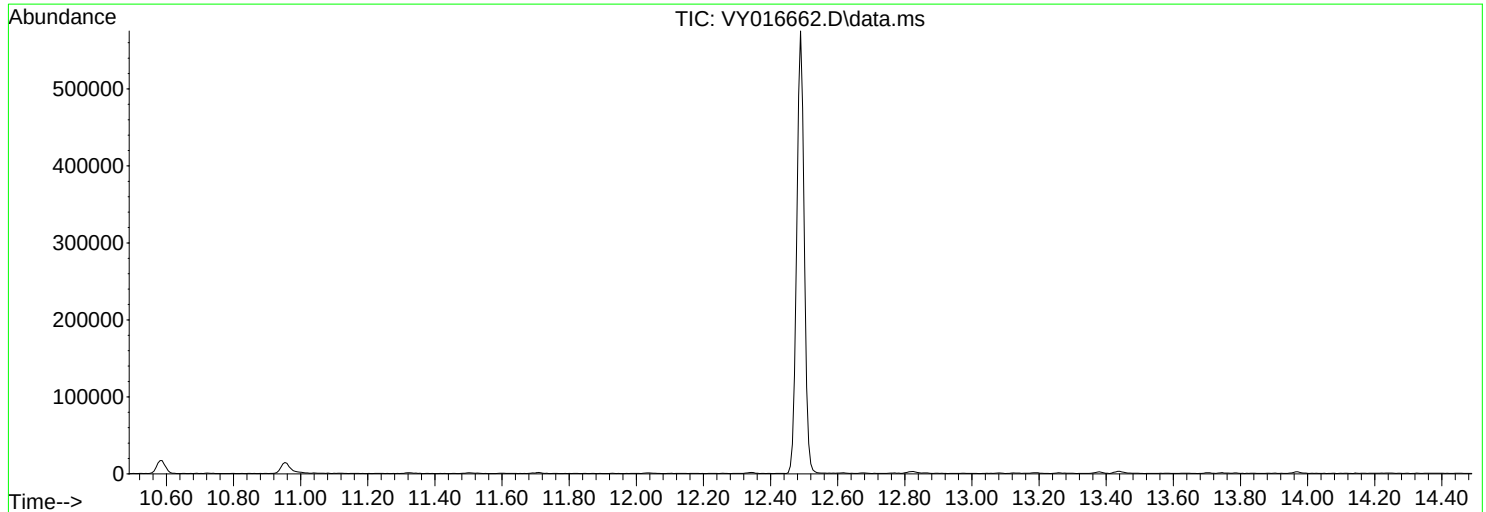

AutoFind: Scans 1749, 1750, 1751; Background Corrected with Scan 1741

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	18103	PASS
75	95	30	60	51.7	50691	PASS
95	95	100	100	100.0	98013	PASS
96	95	5	9	6.4	6256	PASS
173	174	0.00	2	1.1	961	PASS
174	95	50	100	86.5	84733	PASS
175	174	5	9	7.9	6734	PASS
176	174	95	101	97.9	82987	PASS
177	176	5	9	6.6	5475	PASS