


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY121625\
Data File : VY023983.D
Acq On : 16 Dec 2025 07:40
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y121625S.M
Title : SW846 8260
Last Update : Wed Dec 17 04:12:33 2025

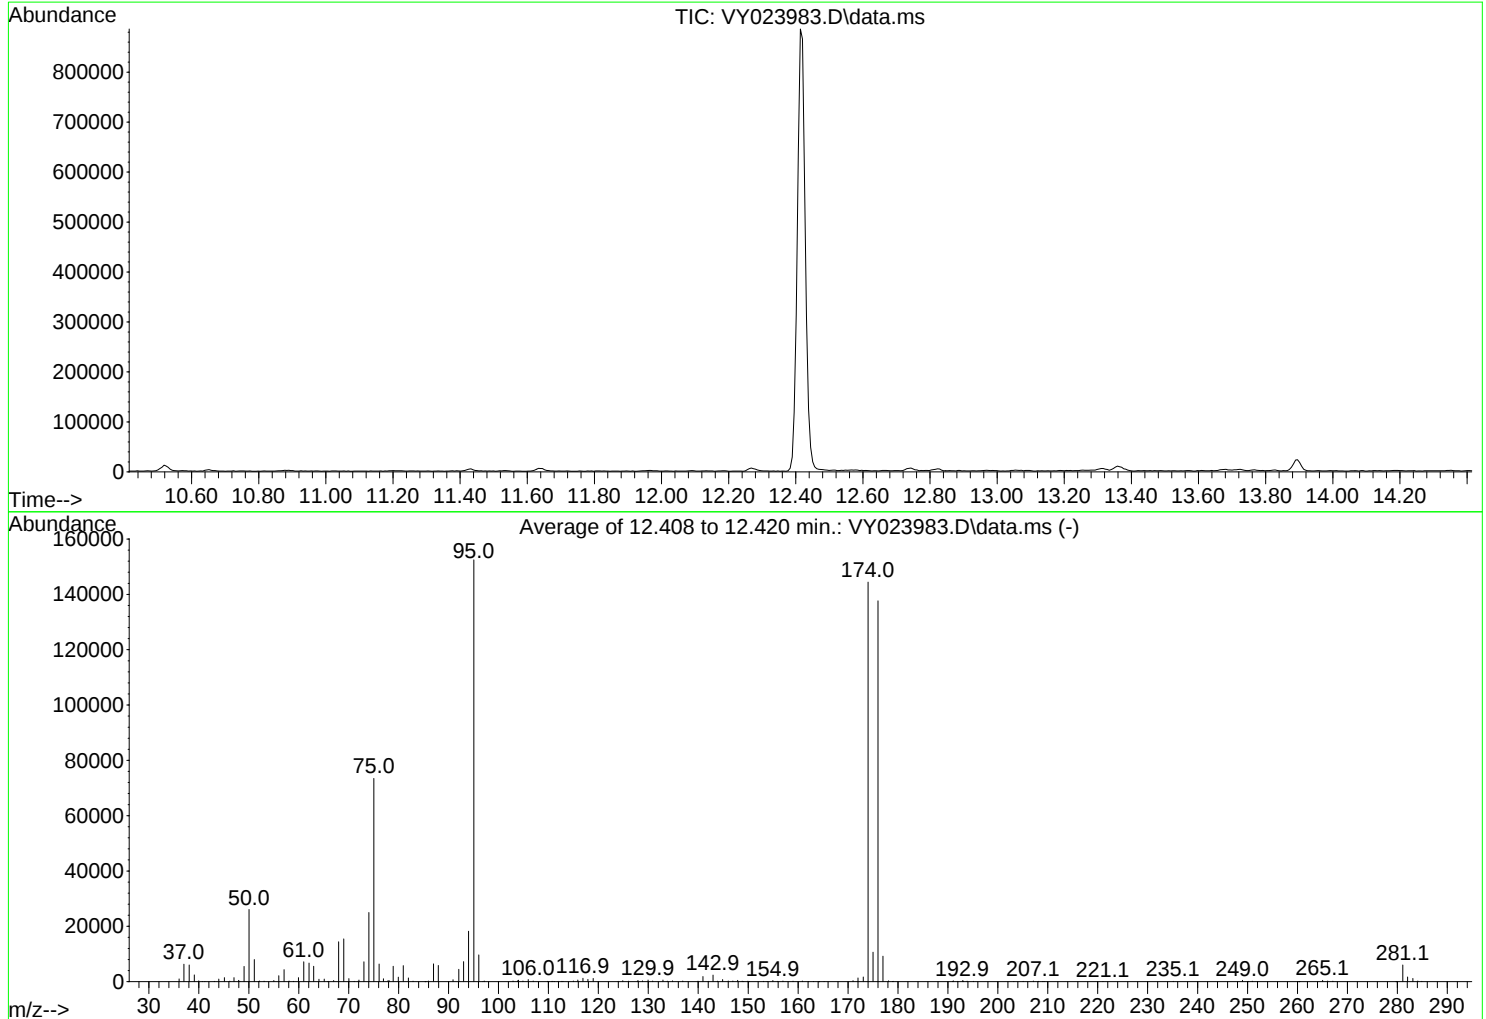

AutoFind: Scans 1753, 1754, 1755; Background Corrected with Scan 1744

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.1	26075	PASS
75	95	30	60	48.2	73464	PASS
95	95	100	100	100.0	152491	PASS
96	95	5	9	6.4	9689	PASS
173	174	0.00	2	1.2	1711	PASS
174	95	50	100	94.7	144437	PASS
175	174	5	9	7.4	10634	PASS
176	174	95	101	95.3	137688	PASS
177	176	5	9	6.7	9201	PASS