


Data Path : Z:\voasrv\HPCHEM1\MSVOA Y\Data\VY121719\
Data File : VY000969.D
Acq On : 17 Dec 2019 09:54
Operator : SY/MD
Sample : BFB
Misc : 5.00G/5ML/MSVOA Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y112719S.M
Title : SW846 8260
Last Update : Wed Nov 27 12:40:47 2019

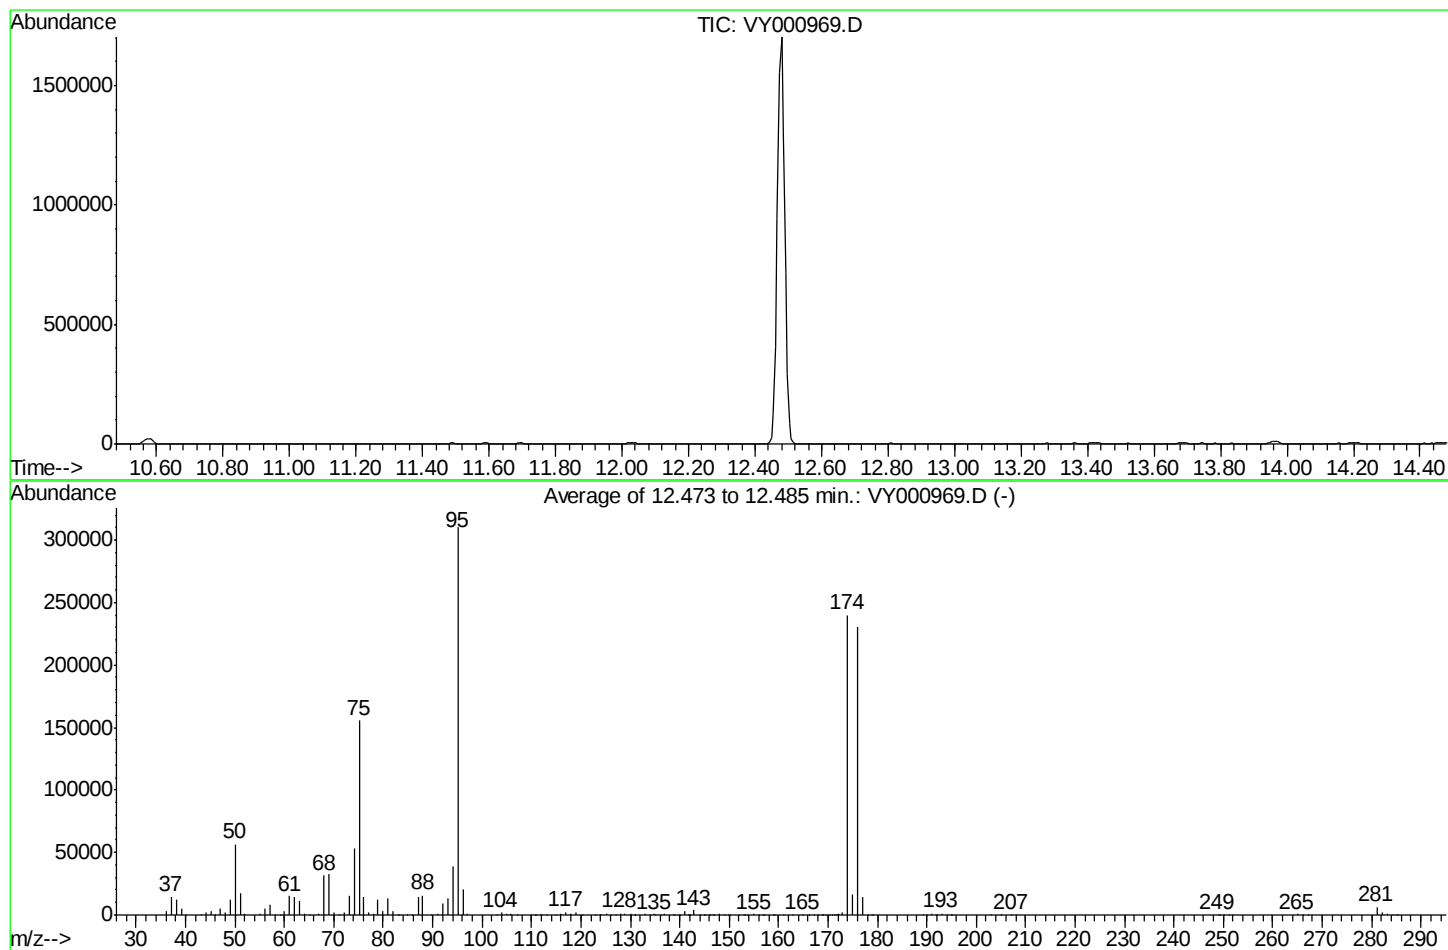

AutoFind: Scans 1761, 1762, 1763; Background Corrected with Scan 1752

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.2	56485	PASS
75	95	30	60	50.1	155461	PASS
95	95	100	100	100.0	310122	PASS
96	95	5	9	6.5	20130	PASS
173	174	0.00	2	0.7	1600	PASS
174	95	50	100	77.4	240106	PASS
175	174	5	9	6.9	16560	PASS
176	174	95	101	95.9	230229	PASS
177	176	5	9	6.4	14689	PASS