
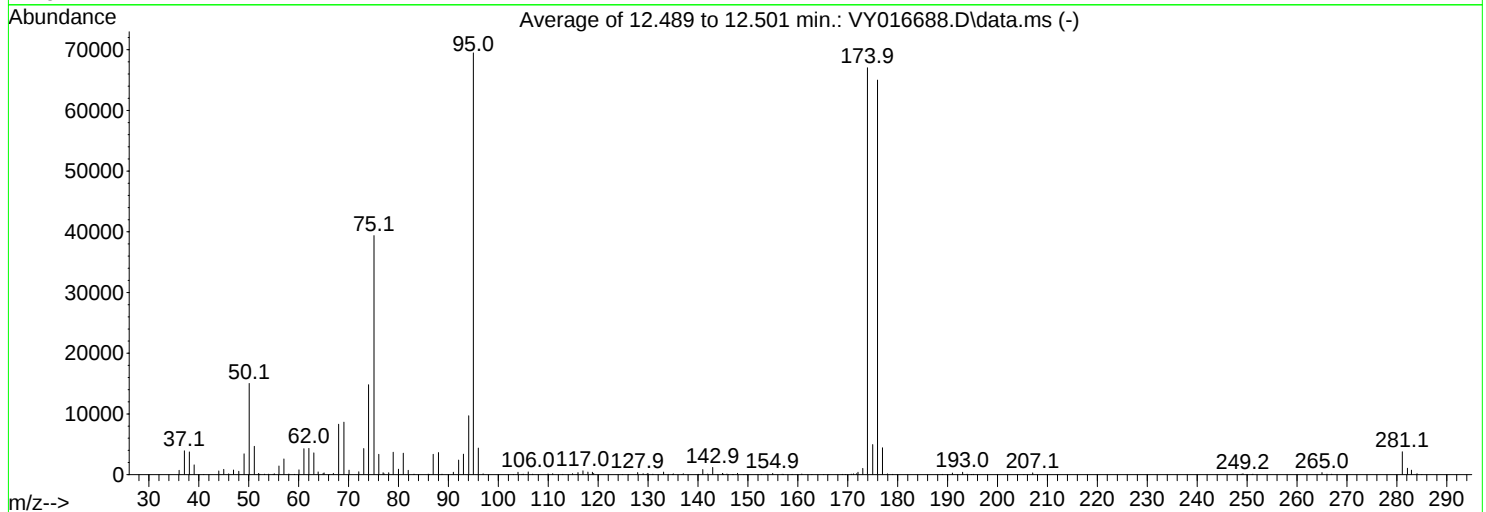


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY121923\
Data File : VY016688.D
Acq On : 19 Dec 2023 09:57
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y121923S.M
Title : SW846 8260
Last Update : Wed Dec 20 12:57:23 2023

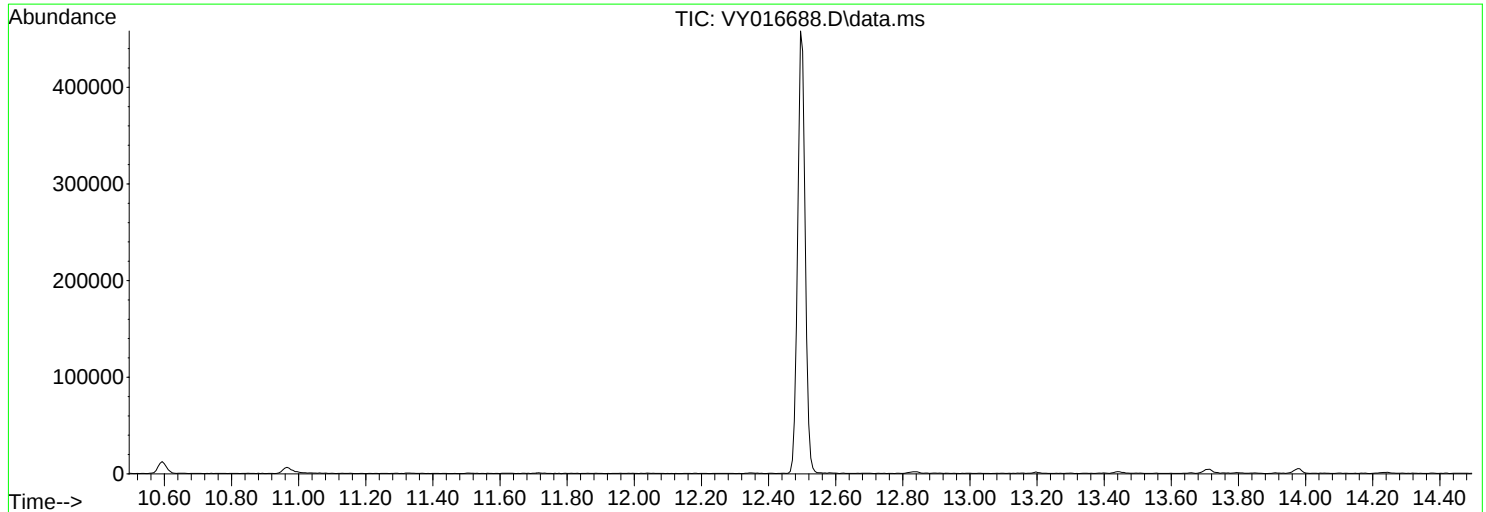

AutoFind: Scans 1750, 1751, 1752; Background Corrected with Scan 1742

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	21.6	15020	PASS
75	95	30	60	56.7	39376	PASS
95	95	100	100	100.0	69488	PASS
96	95	5	9	6.3	4368	PASS
173	174	0.00	2	1.5	1025	PASS
174	95	50	100	96.5	67043	PASS
175	174	5	9	7.4	4958	PASS
176	174	95	101	97.0	65008	PASS
177	176	5	9	6.8	4419	PASS