


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY121923\
Data File : VY016698.D
Acq On : 19 Dec 2023 15:58
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y121923S.M
Title : SW846 8260
Last Update : Wed Dec 20 12:57:23 2023

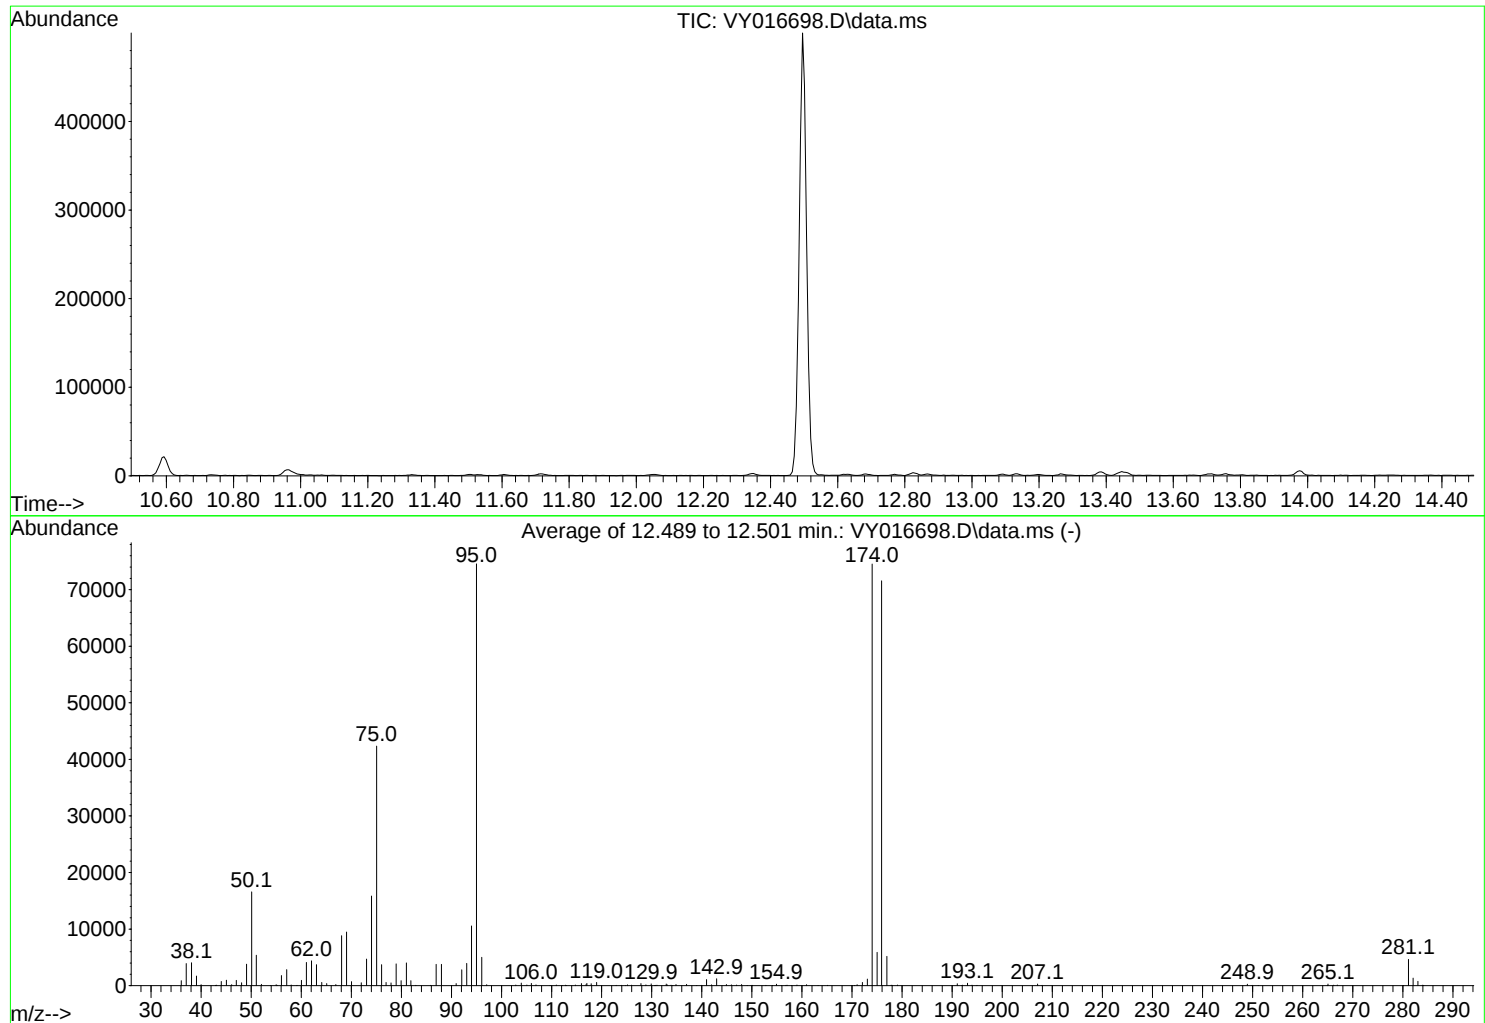

AutoFind: Scans 1750, 1751, 1752; Background Corrected with Scan 1742

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.2	16584	PASS
75	95	30	60	56.8	42344	PASS
95	95	100	100	100.0	74571	PASS
96	95	5	9	6.7	5005	PASS
173	174	0.00	2	1.6	1166	PASS
174	95	50	100	100.0	74544	PASS
175	174	5	9	7.9	5876	PASS
176	174	95	101	96.0	71568	PASS
177	176	5	9	7.2	5181	PASS