
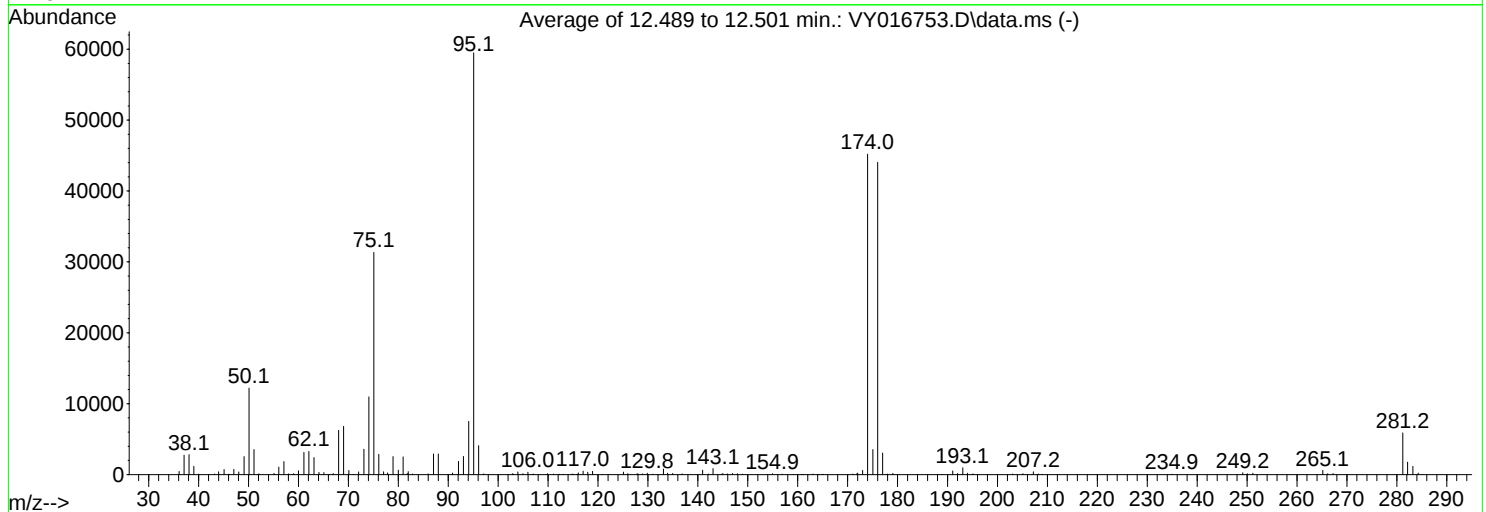


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY122123\
Data File : VY016753.D
Acq On : 21 Dec 2023 10:41
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y122023S.M
Title : SW846 8260
Last Update : Thu Dec 21 01:49:45 2023

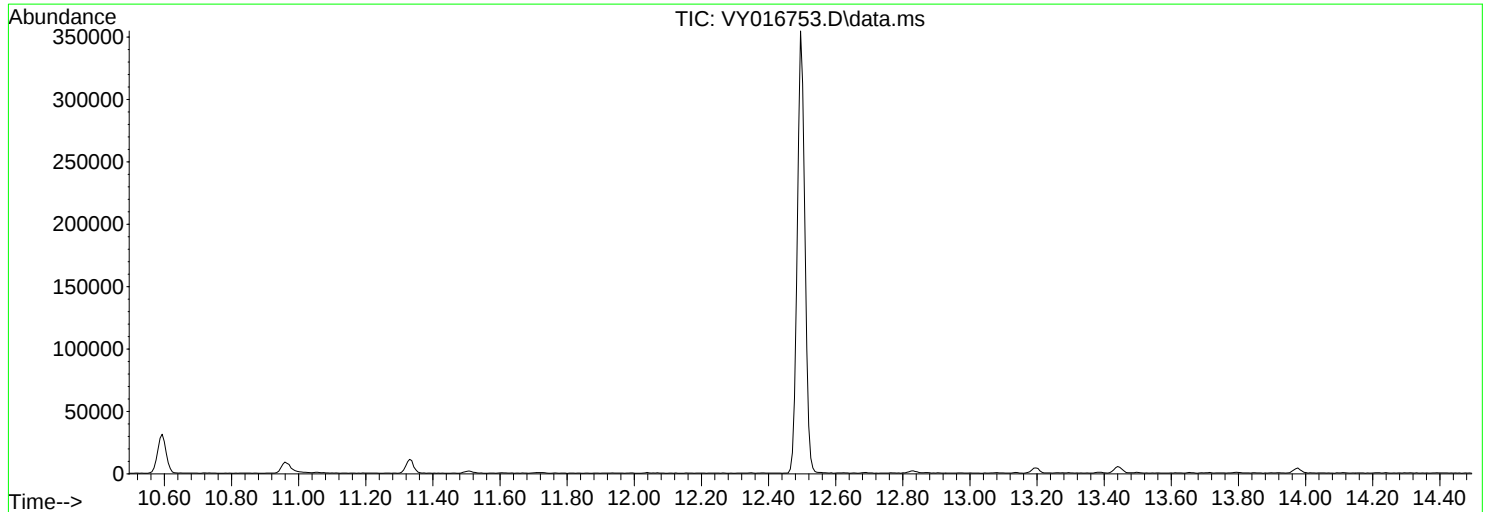

AutoFind: Scans 1750, 1751, 1752; Background Corrected with Scan 1742

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.5	12213	PASS
75	95	30	60	52.7	31352	PASS
95	95	100	100	100.0	59485	PASS
96	95	5	9	6.9	4089	PASS
173	174	0.00	2	1.3	602	PASS
174	95	50	100	76.0	45197	PASS
175	174	5	9	7.9	3548	PASS
176	174	95	101	97.4	44037	PASS
177	176	5	9	6.9	3040	PASS