
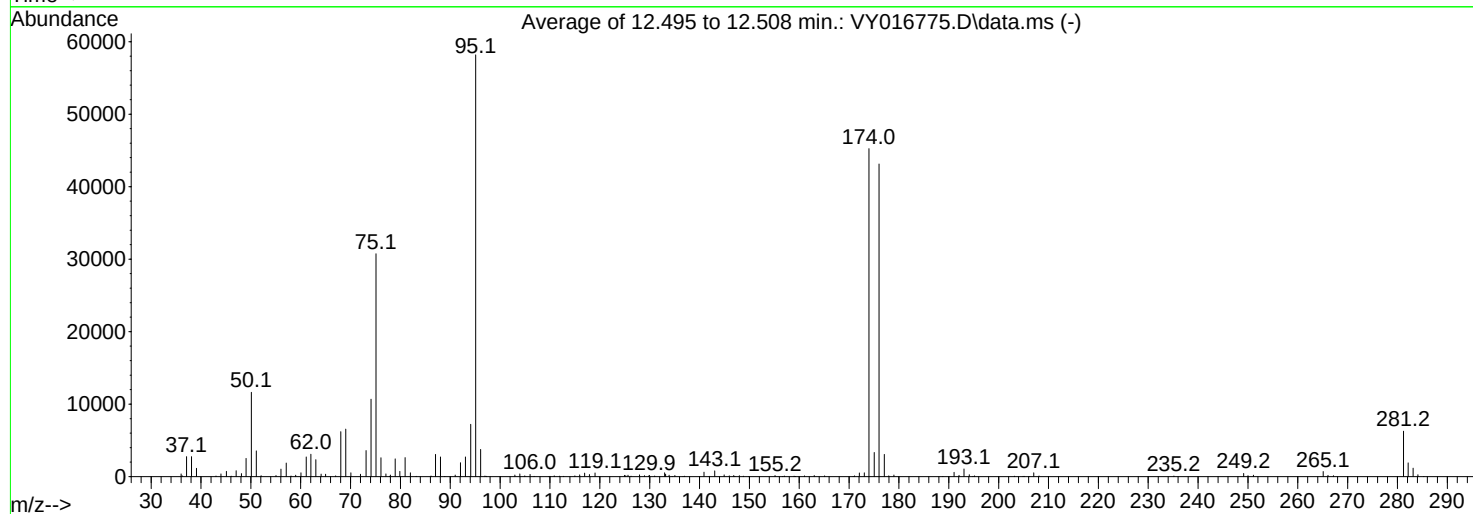


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY122123\
Data File : VY016775.D
Acq On : 21 Dec 2023 22:49
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y122023S.M
Title : SW846 8260
Last Update : Thu Dec 21 01:49:45 2023

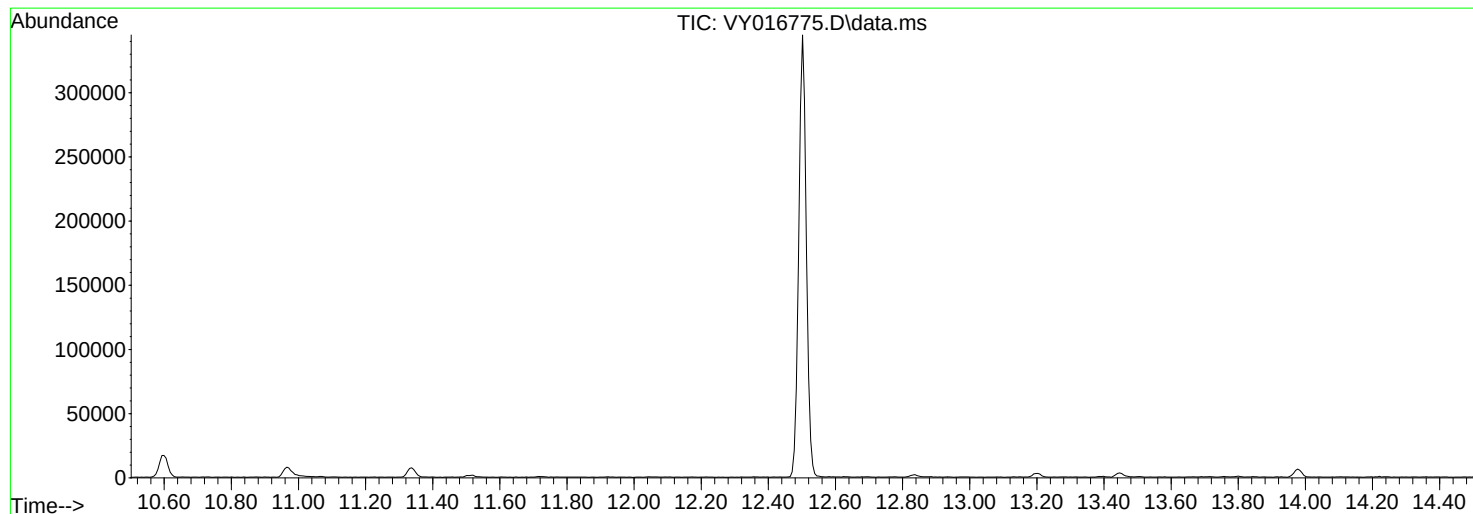

AutoFind: Scans 1751, 1752, 1753; Background Corrected with Scan 1743

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.0	11635	PASS
75	95	30	60	52.8	30747	PASS
95	95	100	100	100.0	58184	PASS
96	95	5	9	6.4	3749	PASS
173	174	0.00	2	1.2	523	PASS
174	95	50	100	77.8	45253	PASS
175	174	5	9	7.4	3333	PASS
176	174	95	101	95.3	43139	PASS
177	176	5	9	7.1	3058	PASS