
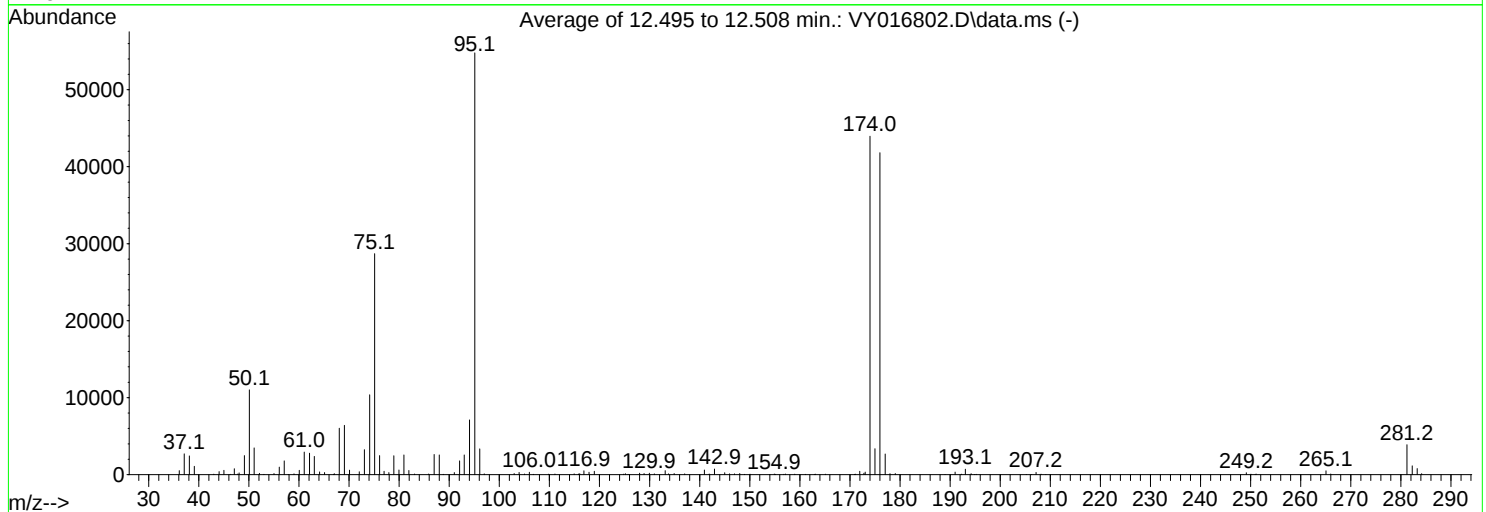


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY122223\
Data File : VY016802.D
Acq On : 22 Dec 2023 11:58
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y122023S.M
Title : SW846 8260
Last Update : Thu Dec 21 01:49:45 2023

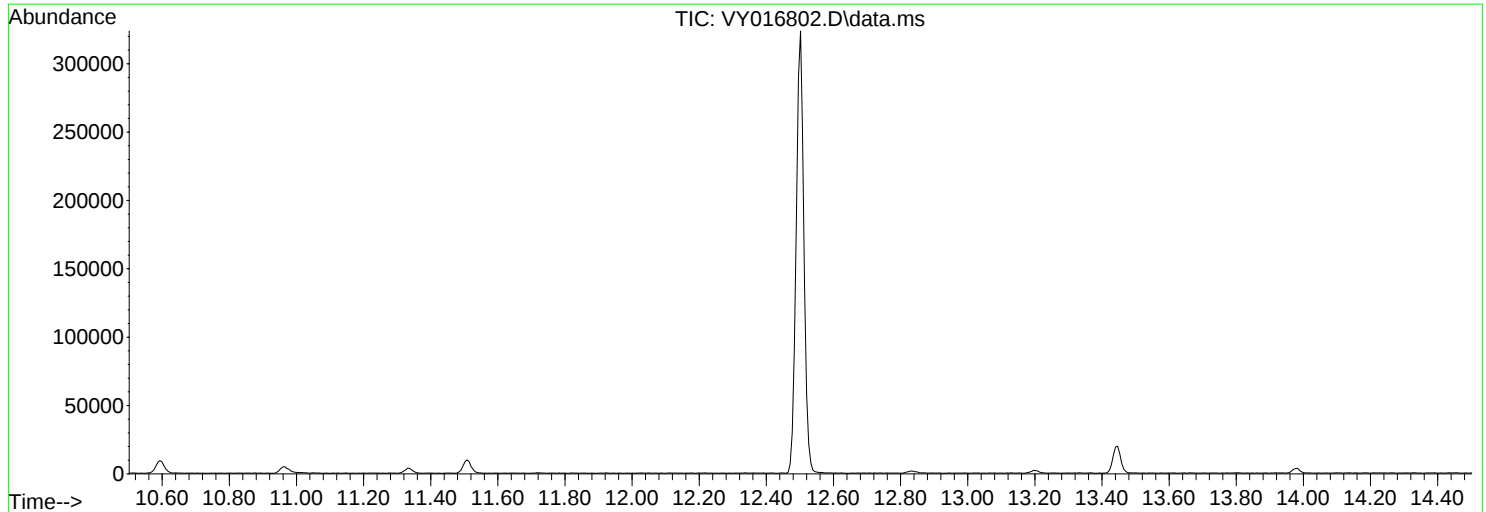

AutoFind: Scans 1751, 1752, 1753; Background Corrected with Scan 1743

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.1	11027	PASS
75	95	30	60	52.4	28709	PASS
95	95	100	100	100.0	54789	PASS
96	95	5	9	6.1	3354	PASS
173	174	0.00	2	0.8	338	PASS
174	95	50	100	80.2	43957	PASS
175	174	5	9	7.7	3364	PASS
176	174	95	101	95.1	41813	PASS
177	176	5	9	6.4	2681	PASS