
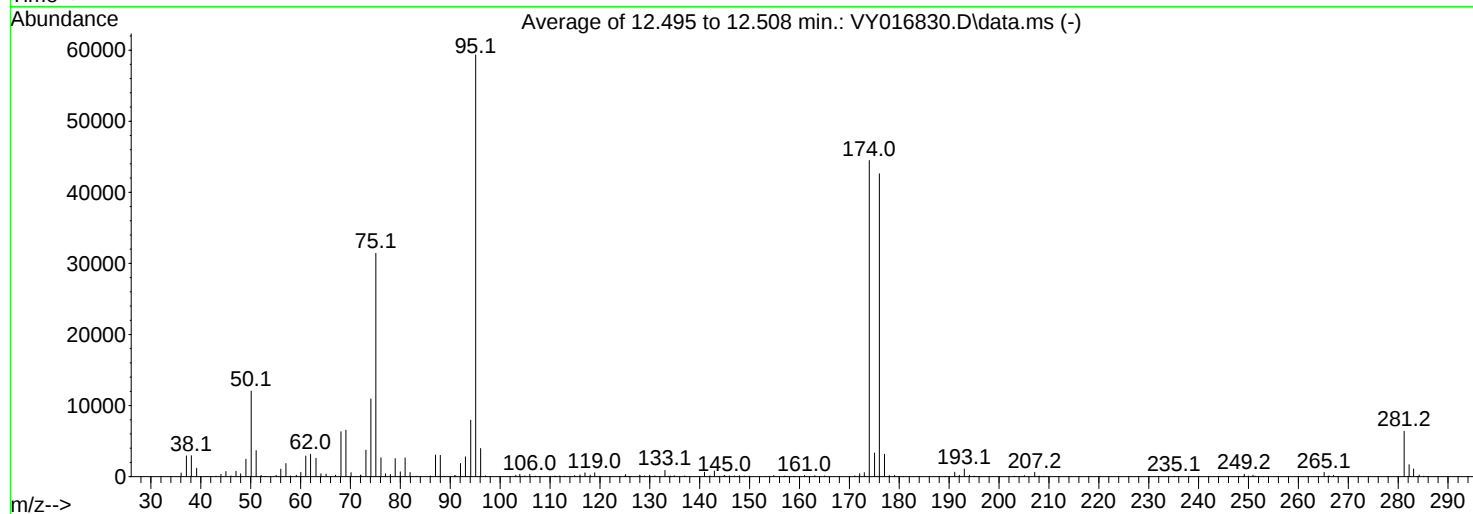


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY122223\
Data File : VY016830.D
Acq On : 23 Dec 2023 00:09
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y122023S.M
Title : SW846 8260
Last Update : Thu Dec 21 01:49:45 2023

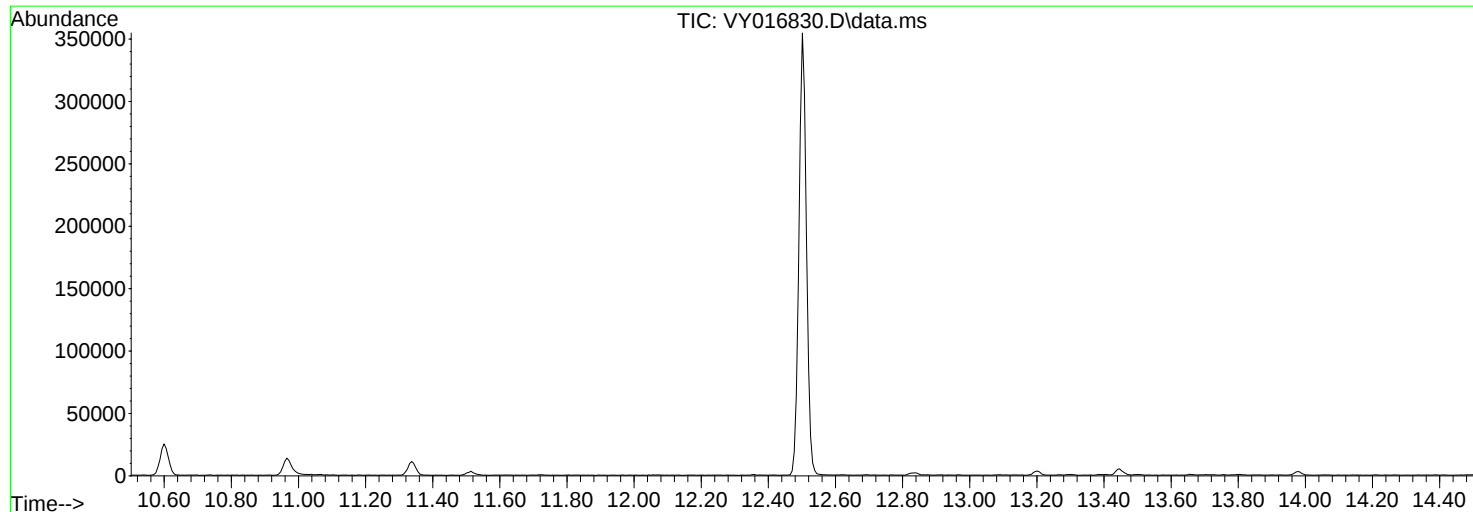

AutoFind: Scans 1751, 1752, 1753; Background Corrected with Scan 1743

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.3	12055	PASS
75	95	30	60	52.9	31416	PASS
95	95	100	100	100.0	59341	PASS
96	95	5	9	6.7	3953	PASS
173	174	0.00	2	1.3	570	PASS
174	95	50	100	74.9	44472	PASS
175	174	5	9	7.5	3328	PASS
176	174	95	101	95.8	42605	PASS
177	176	5	9	7.4	3153	PASS