

Data Path : Z:\VOASRV\HPCHEM1\MSVOA Y\DATA\VY122319\
 Data File : VY001028.D
 Acq On : 23 Dec 2019 15:07
 Operator : SY/MD
 Sample : K6395-03
 Misc : 5.18G/5ML/MSVOA Y/SOIL
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 TP-4

Quant Time: Jan 06 00:02:04 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y122319S.M
 Quant Title : SW846 8260
 QLast Update : Mon Dec 23 12:07:44 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.80	168	262856	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.69	114	491104	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.49	117	432682	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.42	152	190614	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.15	65	140996	54.39	ug/l	0.00
Spiked Amount 50.000			Recovery	=	108.78%	
35) Dibromofluoromethane	7.72	113	140264	48.50	ug/l	0.00
Spiked Amount 50.000			Recovery	=	97.00%	
50) Toluene-d8	10.18	98	577359	51.09	ug/l	0.00
Spiked Amount 50.000			Recovery	=	102.18%	
62) 4-Bromofluorobenzene	12.48	95	188429	45.60	ug/l	0.00
Spiked Amount 50.000			Recovery	=	91.20%	
Target Compounds						
16) Acetone	3.96	43	5177	8.668	ug/l #	Qvalue 75


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA Y\DATA\VY122319\
Data File : VY001028.D
Acq On : 23 Dec 2019 15:07
Operator : SY/MD
Sample : K6395-03
Misc : 5.18G/5ML/MSVOA Y/SOIL
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
TP-4

Quant Time: Jan 06 00:02:04 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_Y\METHODS\82Y122319S.M
Quant Title : SW846 8260
QLast Update : Mon Dec 23 12:07:44 2019
Response via : Initial Calibration

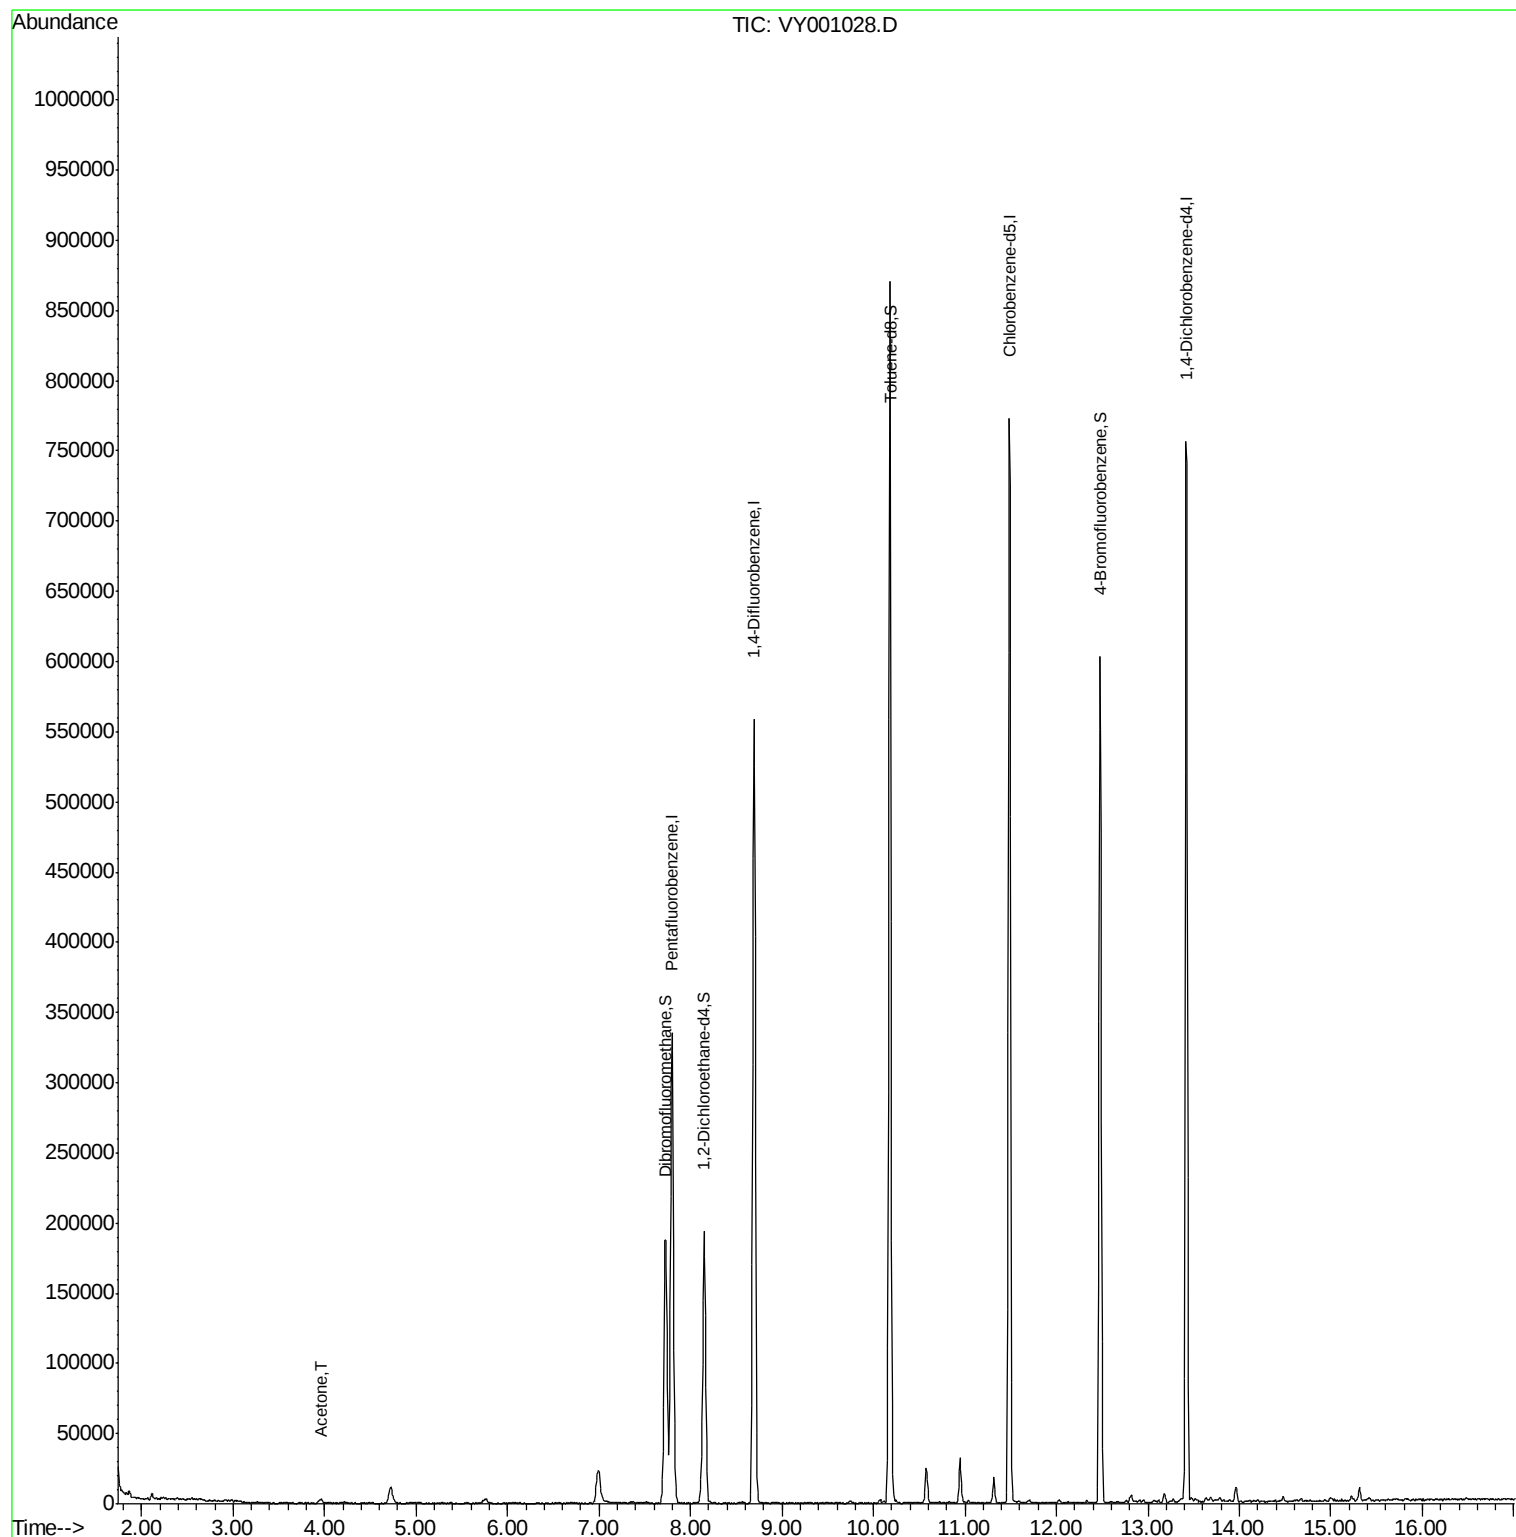

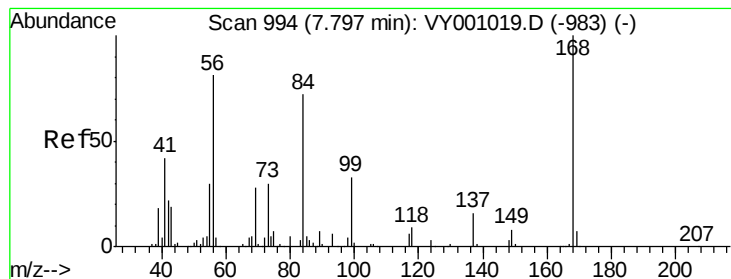

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.80 min Scan# 994

Delta R.T. 0.00 min

Lab File: VY001028.D

Acq: 23 Dec 2019 15:07

Instrument :

MSVOA_Y

ClientSampled :


TP-4

Tot Ion:168 Resp: 262856

Ion Ratio Lower Upper




168 100

99 54.4 44.0 66.0

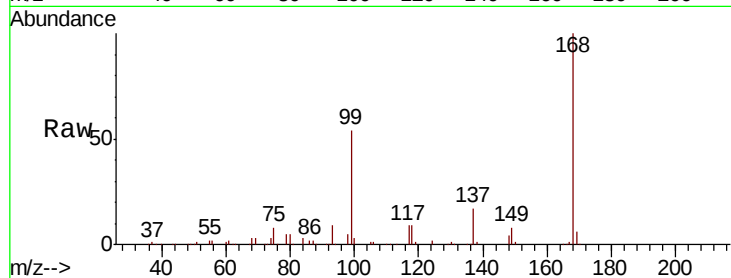

Abundance Ion 167.90 (167.60 to 168.60): VY001019.D (-983) (-)

Ion 98.90 (98.60 to 99.60): VY001019.D (-983) (-)

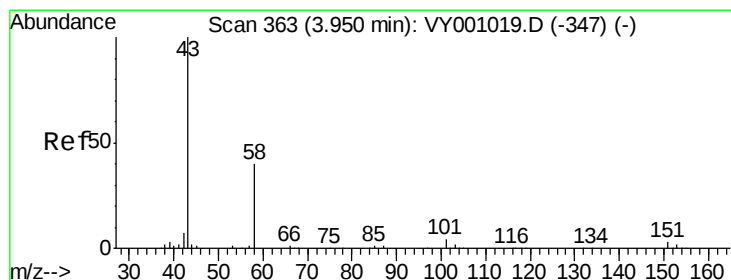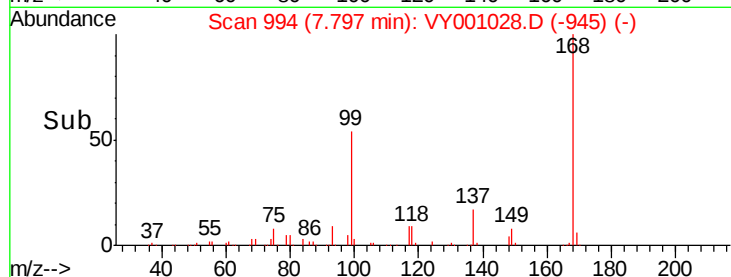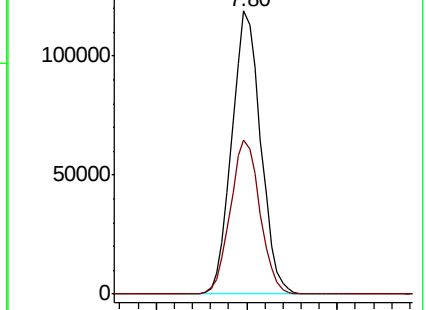

#16

Acetone

Concen: 8.668 ug/l

RT: 3.96 min Scan# 365

Delta R.T. 0.01 min

Lab File: VY001028.D


Acq: 23 Dec 2019 15:07

Tgt Ion: 43 Resp: 5177

Ion Ratio Lower Upper



43 100


58 24.8 32.1 48.1#

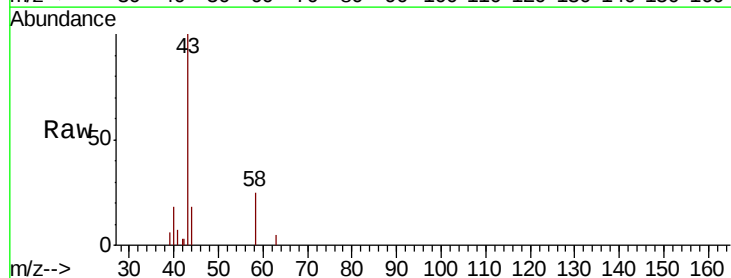

Abundance Ion 43.00 (42.70 to 43.70): VY001019.D (-347) (-)

Ion 58.00 (57.70 to 58.70): VY001019.D (-347) (-)



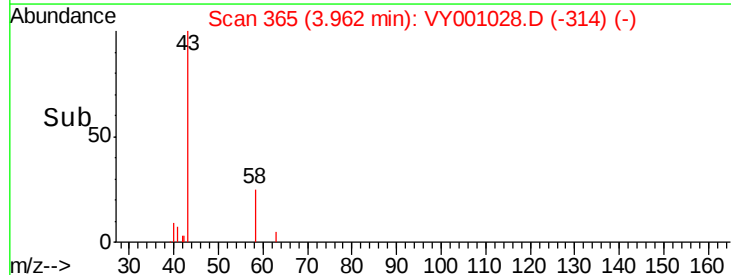
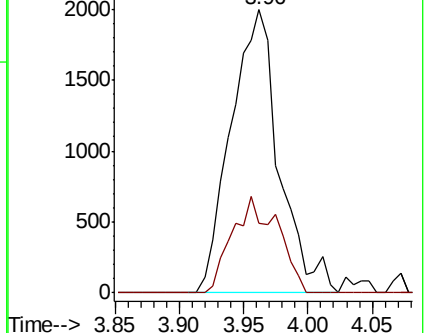


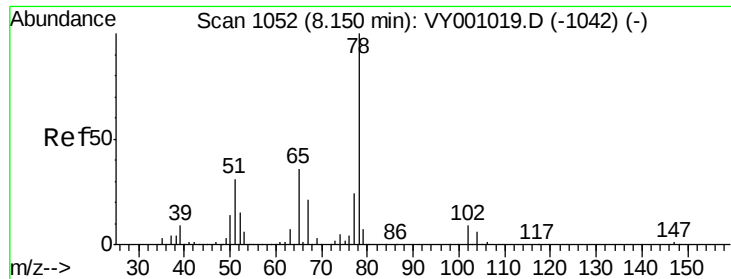

#33
 1,2-Dichloroethane-d4
 Concen: 54.386 ug/l
 RT: 8.15 min Scan# 1052
 Delta R.T. 0.00 min
 Lab File: VY001028.D
 Acq: 23 Dec 2019 15:07




Instrument :
 MSVOA_Y
 ClientSampleId :
 TP-4


Tot Ion: 65 Resp: 140996
 Ion Ratio Lower Upper
 65 100
 67 55.5 0.0 112.8

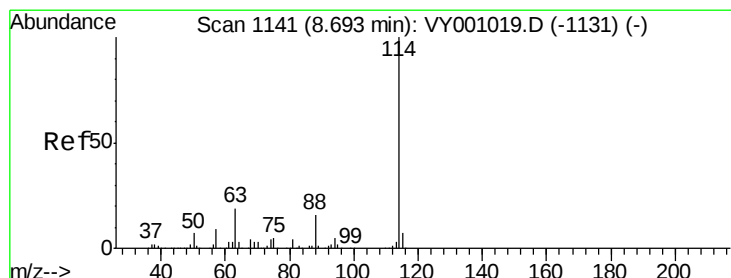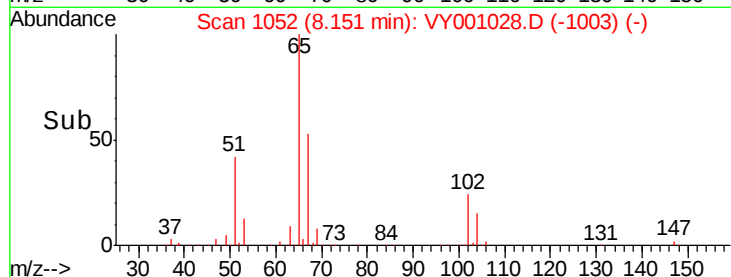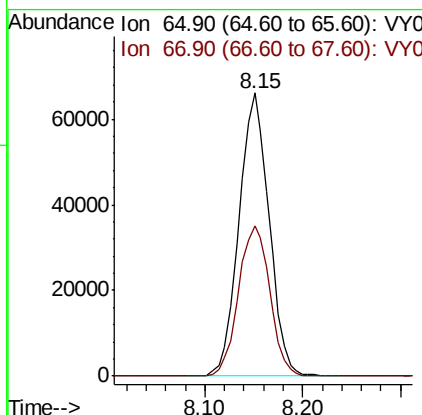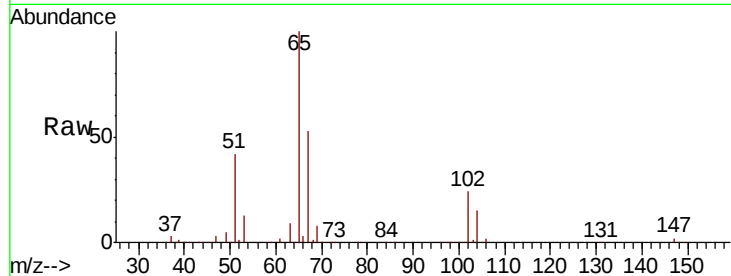

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.69 min Scan# 1141
 Delta R.T. 0.00 min
 Lab File: VY001028.D
 Acq: 23 Dec 2019 15:07

Tgt Ion: 114 Resp: 491104
 Ion Ratio Lower Upper
 114 100
 63 19.2 0.0 37.0
 88 14.2 0.0 32.0

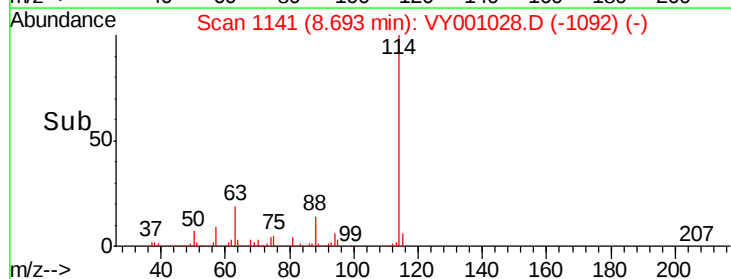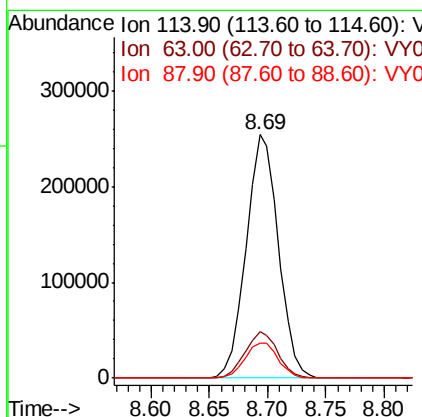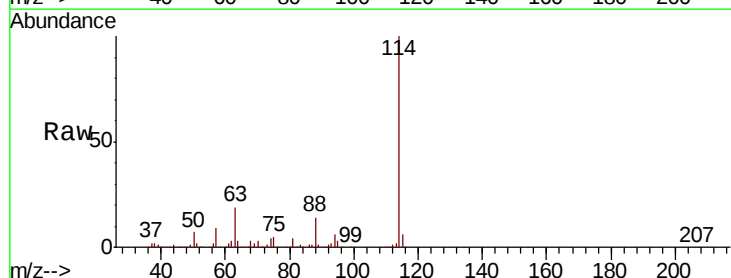

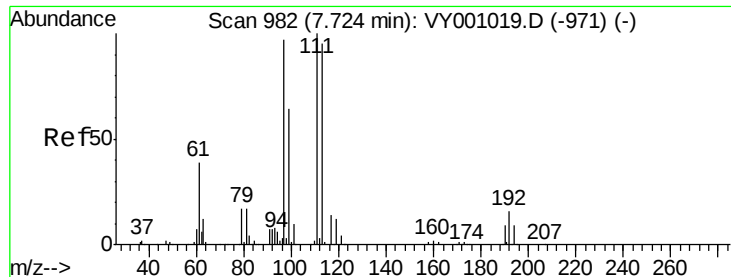

#35

Dibromofluoromethane

Concen: 48.502 ug/l

RT: 7.72 min Scan# 982

Delta R.T. 0.00 min

Lab File: VY001028.D

Acq: 23 Dec 2019 15:07

Instrument :

MSVOA_Y

ClientSampleId :

TP-4


Tot Ion:113 Resp: 140264

Ion Ratio Lower Upper

113 100

111 104.2 83.0 124.4




192 17.1 14.6 21.8

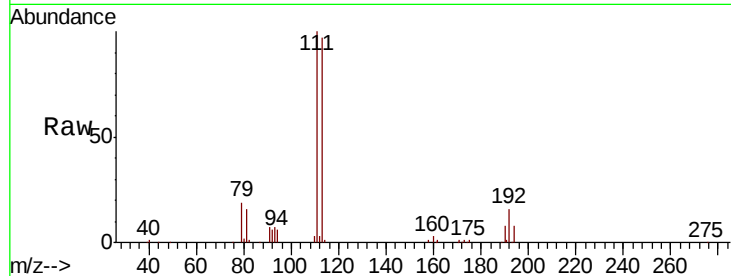

Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

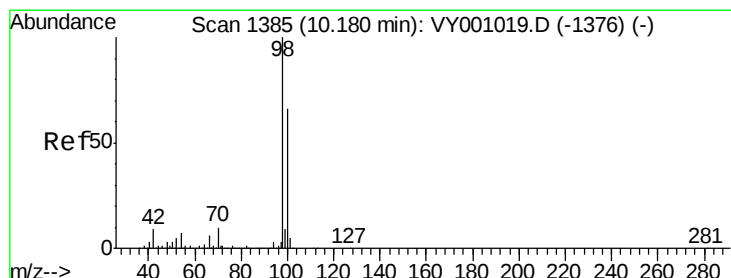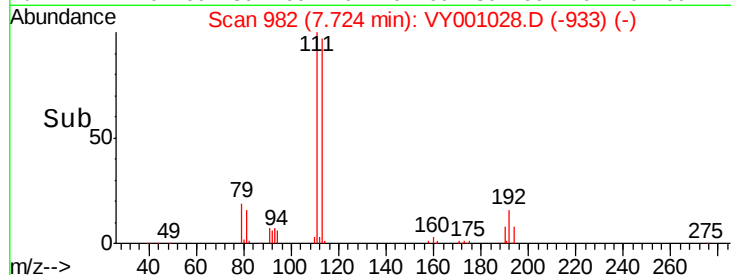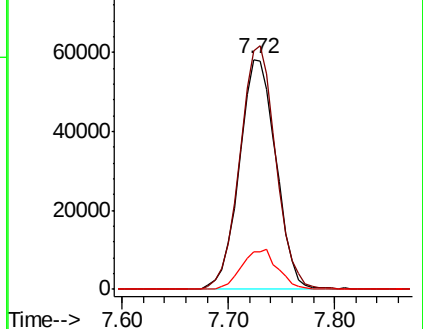

#50

Toluene-d8

Concen: 51.087 ug/l

RT: 10.18 min Scan# 1385

Delta R.T. 0.00 min

Lab File: VY001028.D


Acq: 23 Dec 2019 15:07

Tgt Ion: 98 Resp: 577359

Ion Ratio Lower Upper



98 100


100 66.6 53.0 79.4

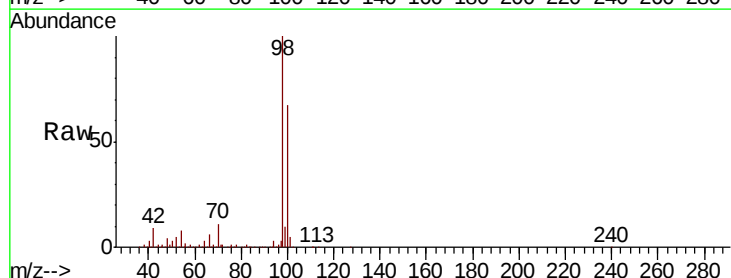

Abundance Ion 98.00 (97.70 to 98.70): VY0

Ion 100.00 (99.70 to 100.70): VY



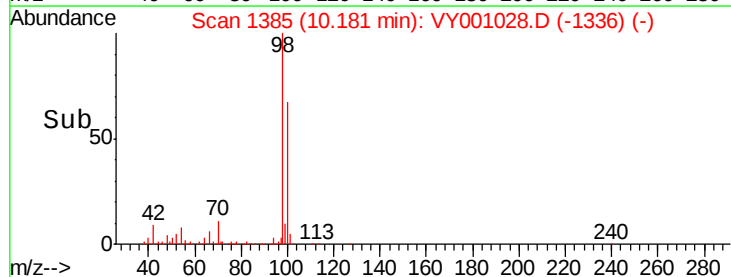
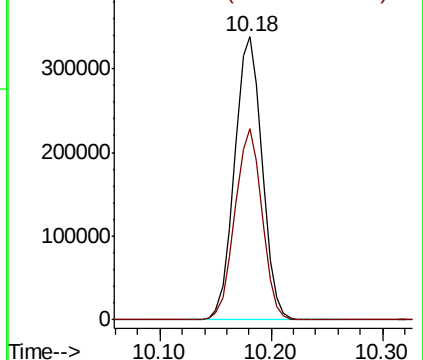


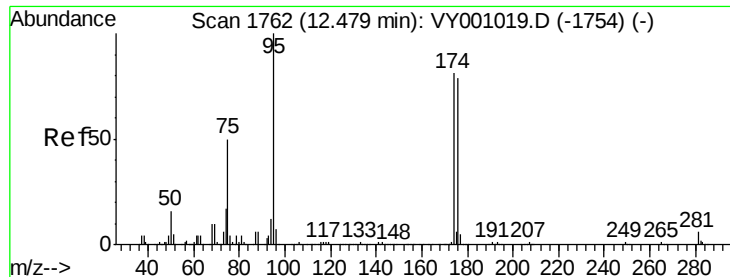

#62
4-Bromofluorobenzene
Concen: 45.602 ug/l
RT: 12.48 min Scan# 1762
Delta R.T. 0.00 min
Lab File: VY001028.D
Acq: 23 Dec 2019 15:07




Instrument :
MSVOA_Y
ClientSampleId :
TP-4


Tot Ion	95	Resp	188429
Ion Ratio	100	Lower	Upper
174	76.9	0.0	156.4
176	73.9	0.0	155.0

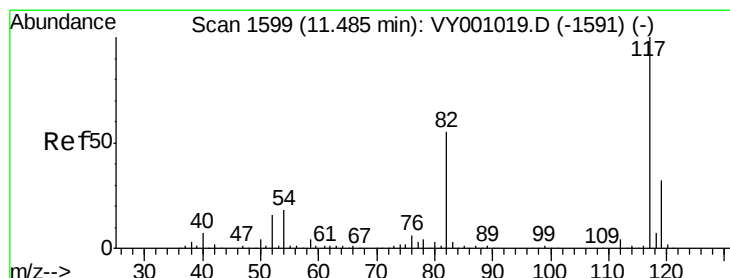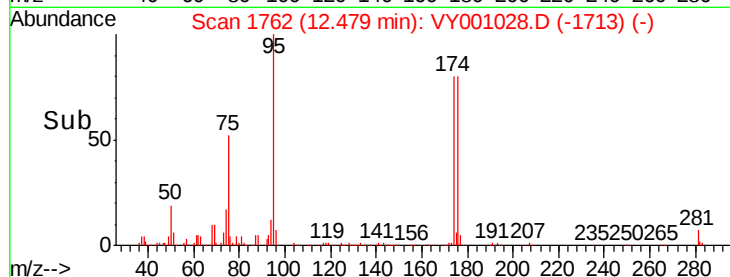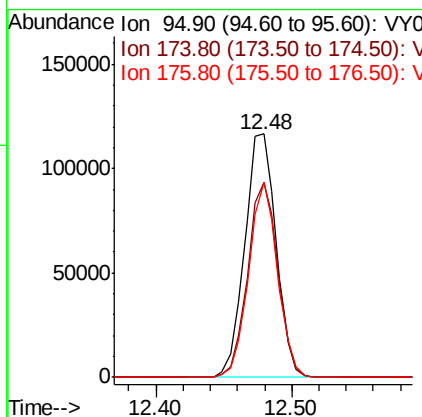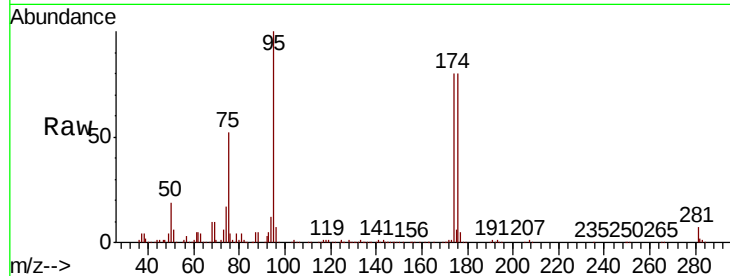

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.49 min Scan# 1599
Delta R.T. 0.00 min
Lab File: VY001028.D
Acq: 23 Dec 2019 15:07

Tgt Ion	117	Resp	432682
Ion Ratio	100	Lower	Upper
82	55.6	43.8	65.8
119	32.9	25.8	38.6

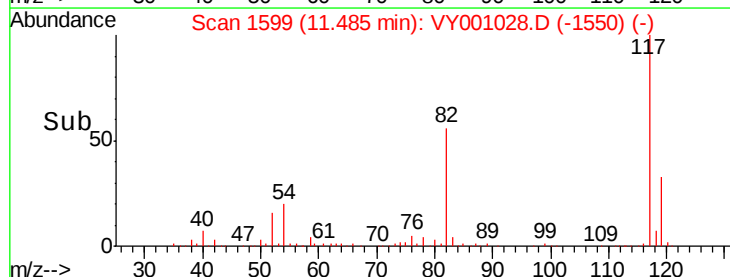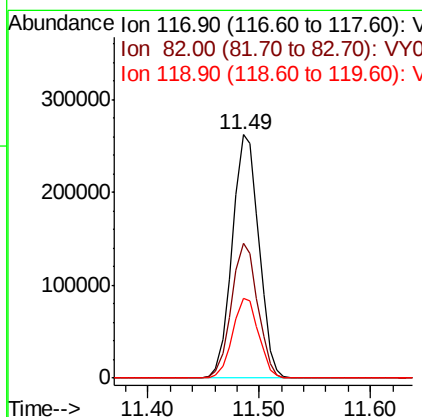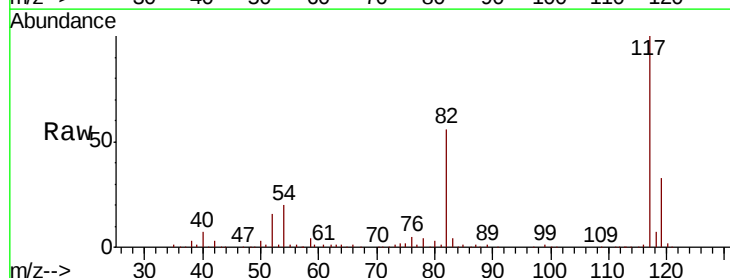

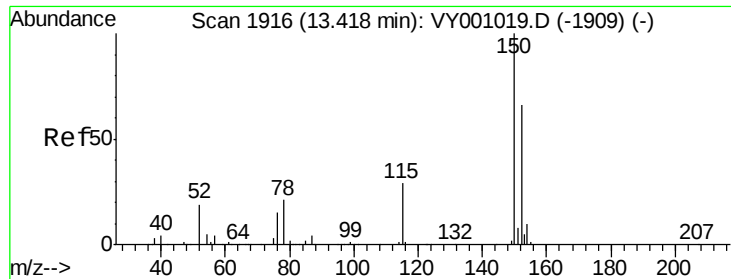

#72

1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.42 min Scan# 1917
Delta R.T. 0.01 min
Lab File: VY001028.D
Acq: 23 Dec 2019 15:07

Instrument :
MSVOA_Y
ClientSampleId :
TP-4

Tot Ion	Ratio	Lower	Upper
152	100		
115	57.2	29.8	89.3
150	158.2	0.0	352.6

