
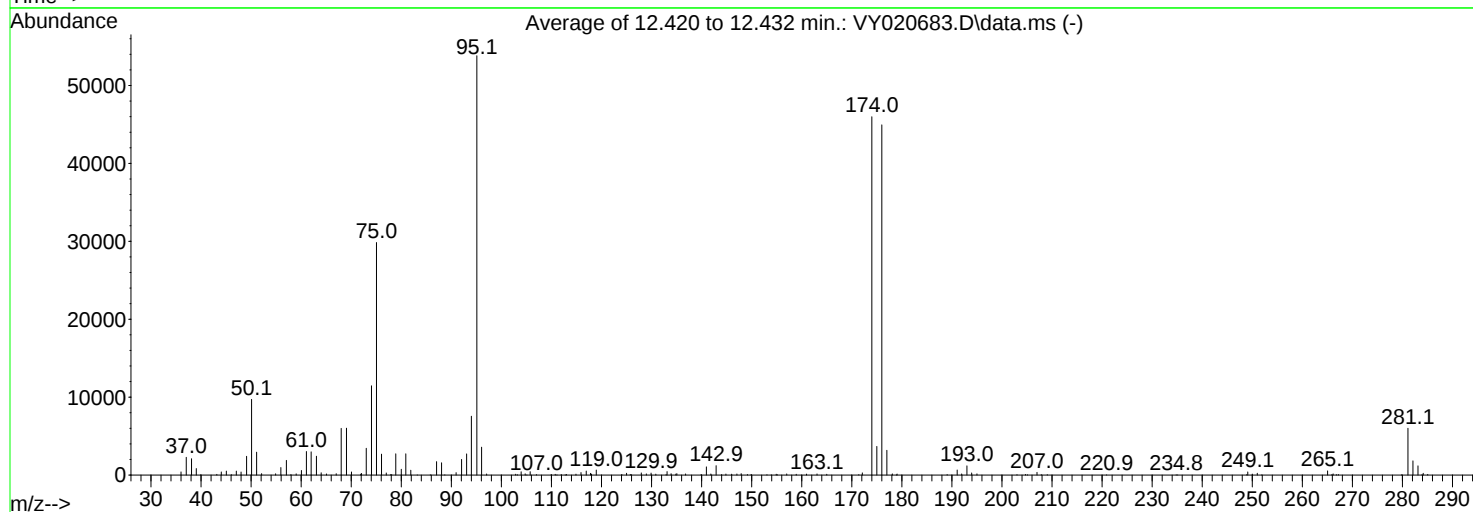


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY122324\
Data File : VY020683.D
Acq On : 23 Dec 2024 08:45
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y122324S.M
Title : SW846 8260
Last Update : Wed Dec 25 00:58:45 2024

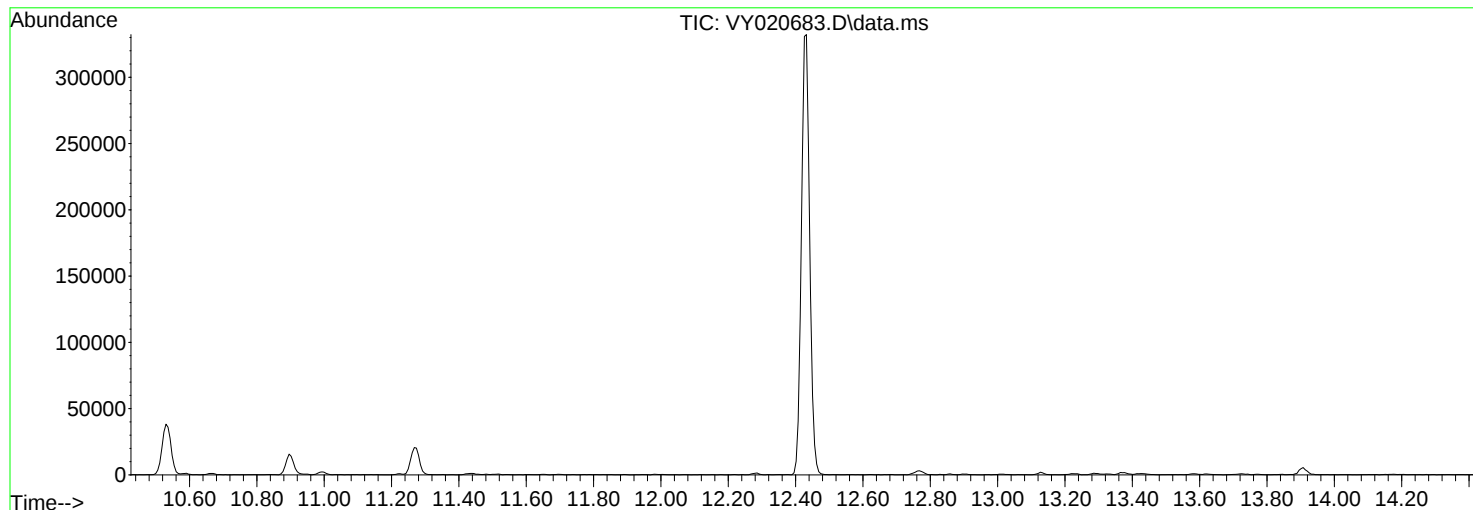

AutoFind: Scans 1755, 1756, 1757; Background Corrected with Scan 1748

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	9719	PASS
75	95	30	60	55.5	29848	PASS
95	95	100	100	100.0	53819	PASS
96	95	5	9	6.7	3579	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	85.5	45989	PASS
175	174	5	9	8.0	3681	PASS
176	174	95	101	97.7	44944	PASS
177	176	5	9	7.1	3183	PASS