


Data Path : Z:\voasrv\HPCHEM1\MSVOA Y\Data\vv122419\
 Data File : VY001035.D
 Acq On : 24 Dec 2019 09:11
 Operator : SY/MD
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y122319S.M
 Title : SW846 8260
 Last Update : Mon Dec 23 12:07:44 2019

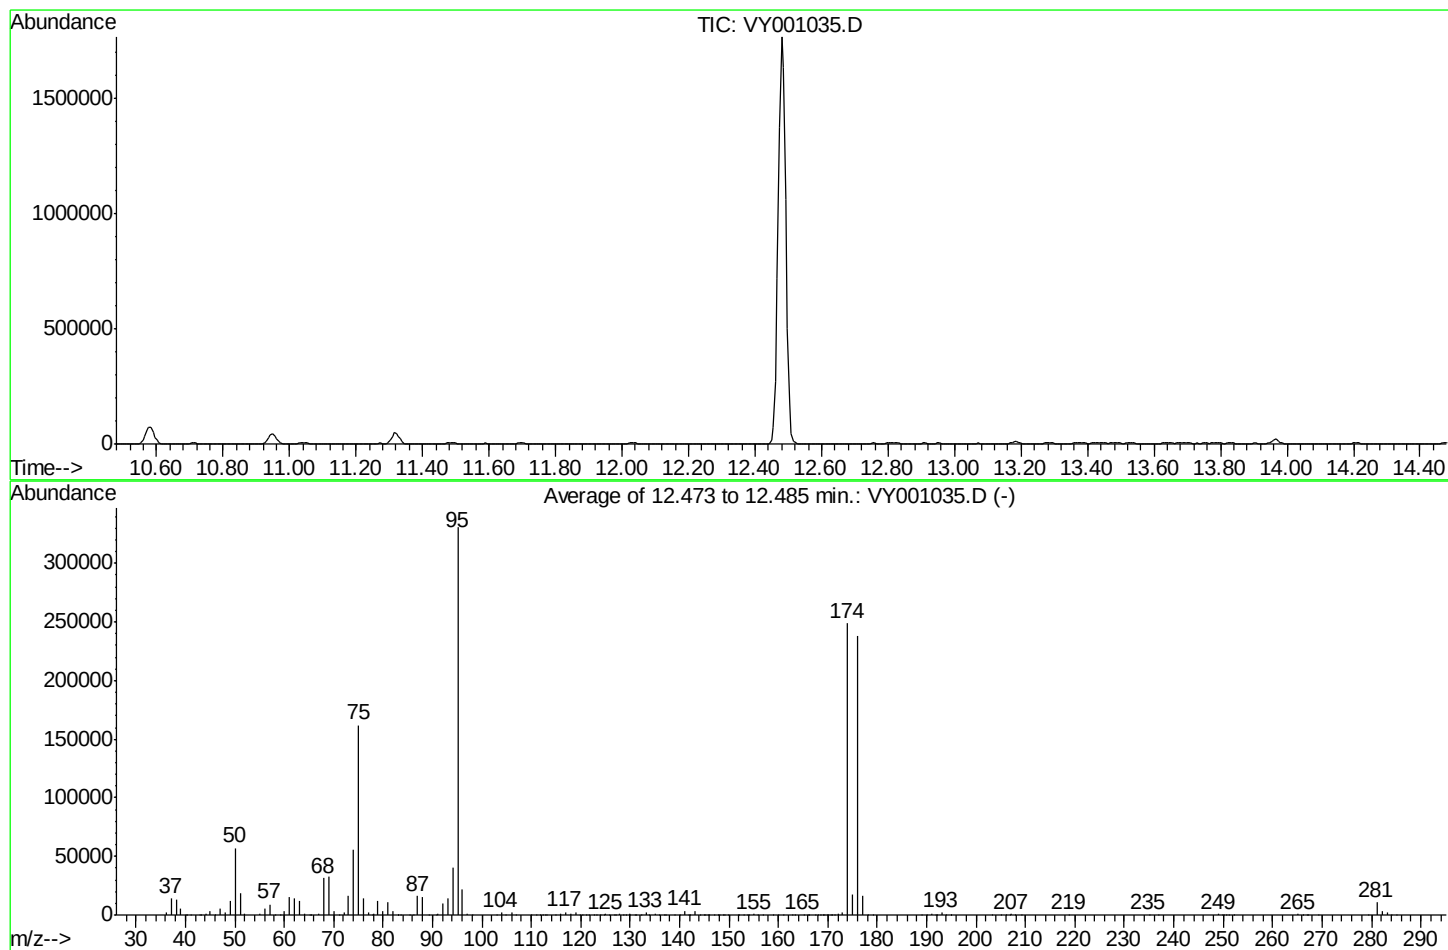

AutoFind: Scans 1761, 1762, 1763; Background Corrected with Scan 1752

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.3	57144	PASS
75	95	30	60	49.0	162112	PASS
95	95	100	100	100.0	330709	PASS
96	95	5	9	6.5	21642	PASS
173	174	0.00	2	0.7	1739	PASS
174	95	50	100	75.2	248597	PASS
175	174	5	9	7.2	17827	PASS
176	174	95	101	95.8	238037	PASS
177	176	5	9	6.7	15963	PASS