


Data Path : Z:\voasrv\HPCHEM1\MSVOA Y\Data\vv122619\
Data File : VY001061.D
Acq On : 26 Dec 2019 09:20
Operator : SY/MD
Sample : BFB
Misc : 5.00G/5ML/MSVOA Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y122319S.M
Title : SW846 8260
Last Update : Mon Dec 23 12:07:44 2019

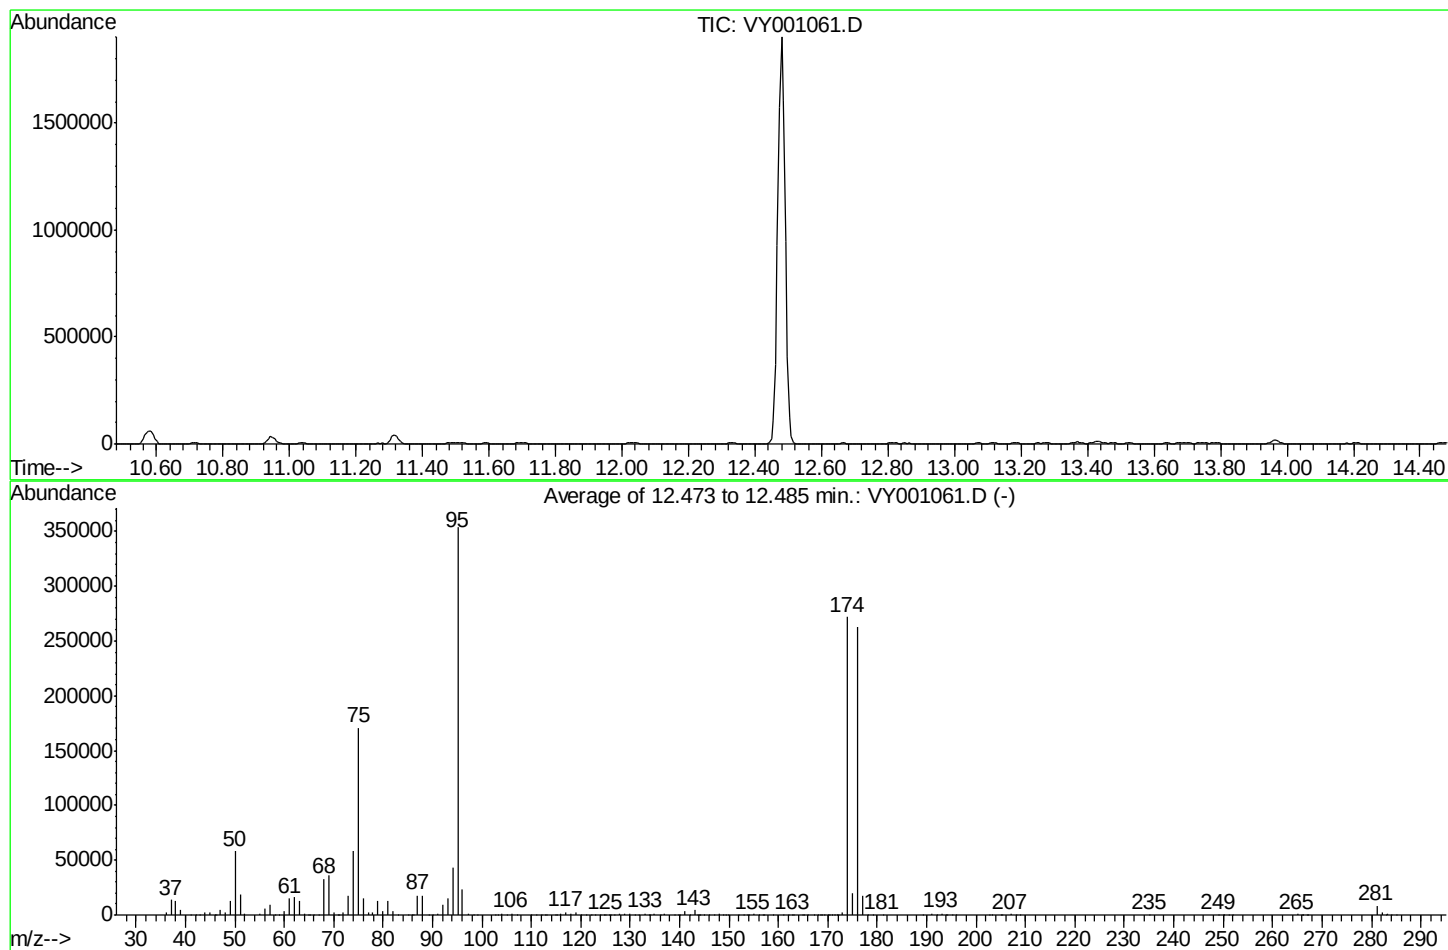

AutoFind: Scans 1761, 1762, 1763; Background Corrected with Scan 1753

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.4	57992	PASS
75	95	30	60	48.3	170944	PASS
95	95	100	100	100.0	353770	PASS
96	95	5	9	6.6	23266	PASS
173	174	0.00	2	0.7	2030	PASS
174	95	50	100	76.8	271872	PASS
175	174	5	9	7.1	19338	PASS
176	174	95	101	96.6	262570	PASS
177	176	5	9	6.6	17377	PASS