

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY122624\
 Data File : VY020714.D
 Acq On : 26 Dec 2024 13:56
 Operator : SY/MD
 Sample : VY1226SBL01
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VY1226SBL01

Quant Time: Dec 26 16:15:26 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y122624S.M
 Quant Title : SW846 8260
 QLast Update : Thu Dec 26 16:12:28 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.719	168	99549	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.622	114	157271	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.420	117	133794	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.352	152	56315	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.067	65	52717	64.652	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	129.300%
35) Dibromofluoromethane	7.640	113	49885	57.586	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	115.180%
50) Toluene-d8	10.109	98	181408	52.569	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	105.140%
62) 4-Bromofluorobenzene	12.407	95	58692	50.981	ug/l	0.00
Spiked Amount	50.000	Range	29 - 146	Recovery	=	101.960%


Target Compounds Qvalue


 (#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY122624\
Data File : VY020714.D
Acq On : 26 Dec 2024 13:56
Operator : SY/MD
Sample : VY1226SBL01
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VY1226SBL01


Quant Time: Dec 26 16:15:26 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y122624S.M
Quant Title : SW846 8260
QLast Update : Thu Dec 26 16:12:28 2024
Response via : Initial Calibration

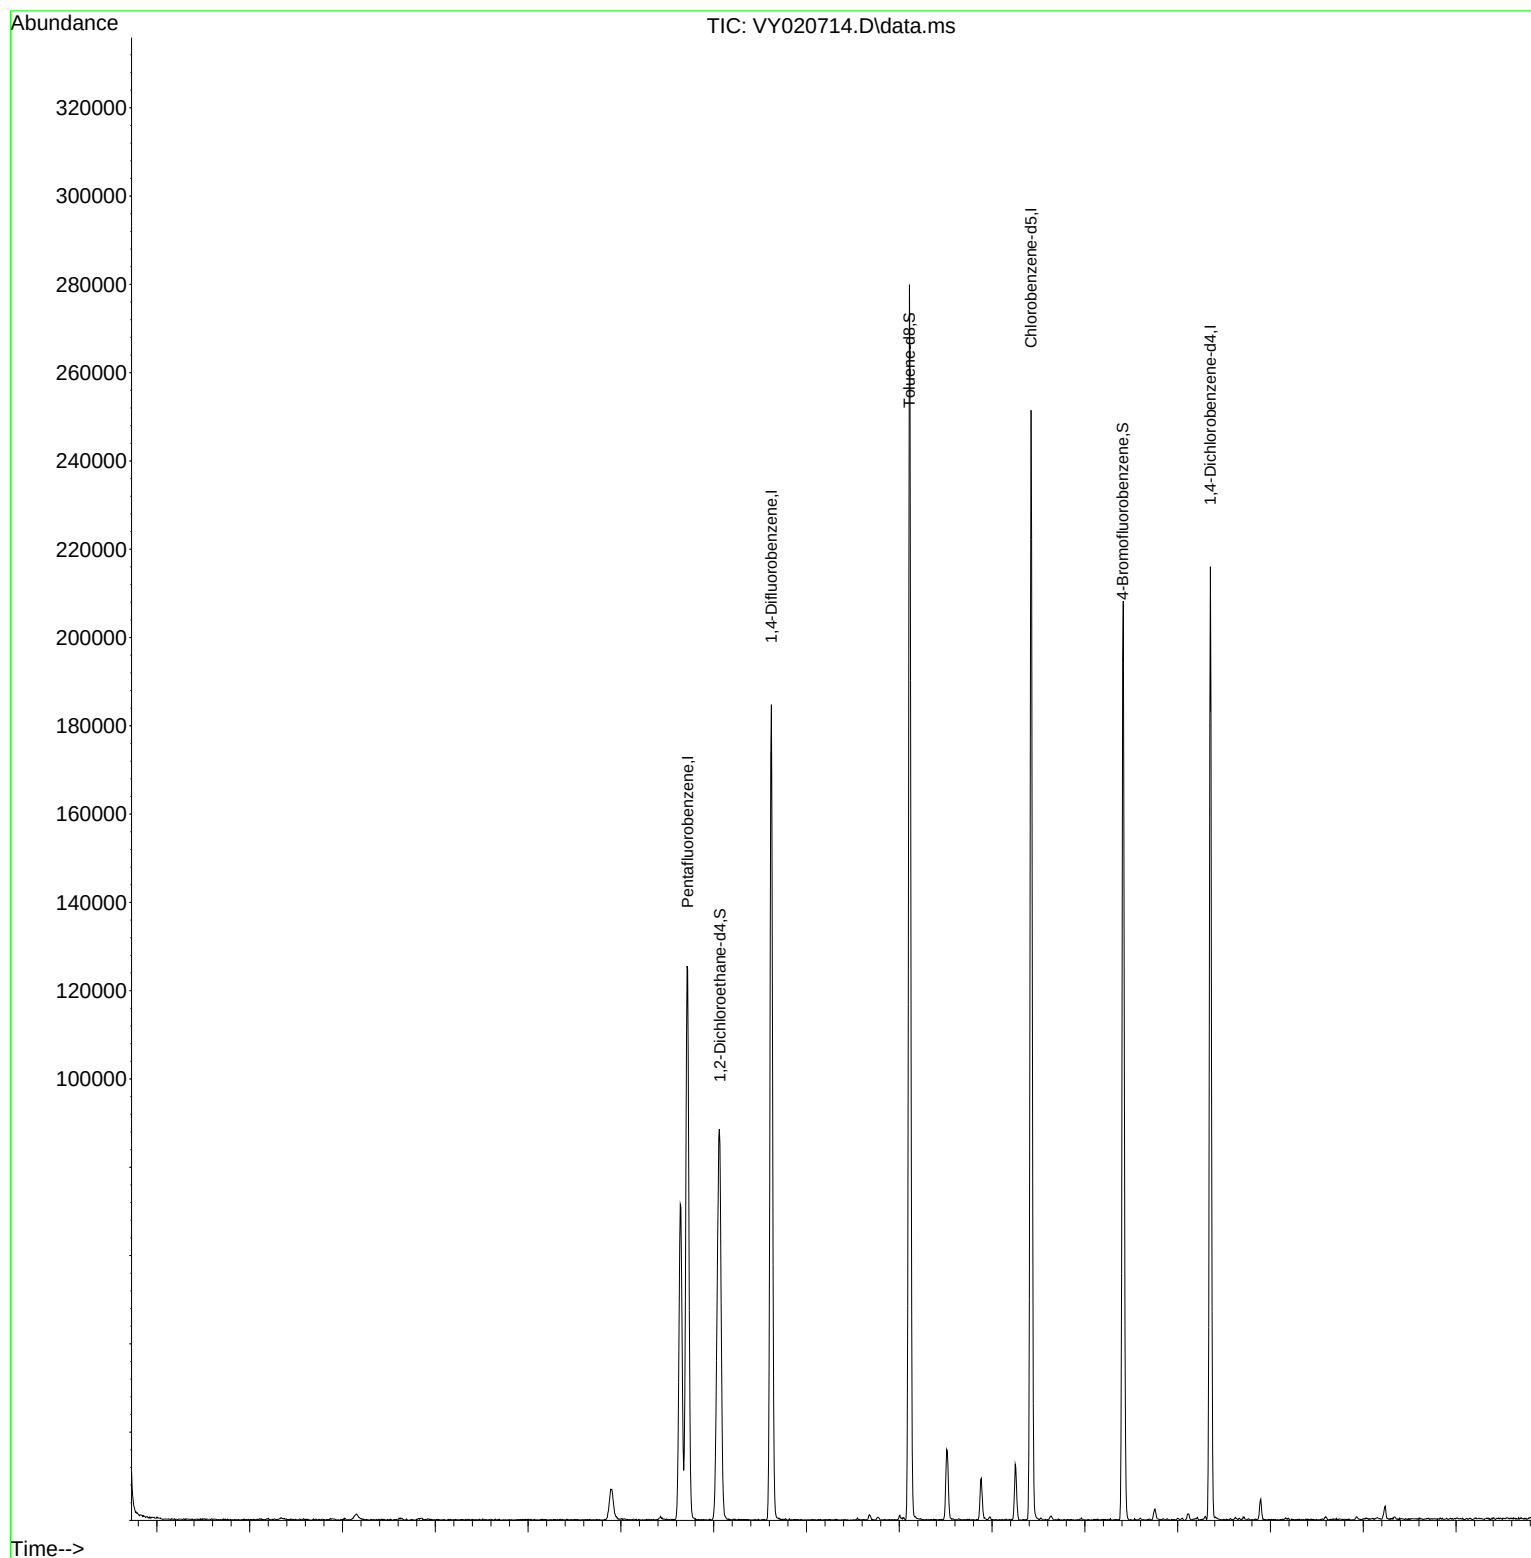



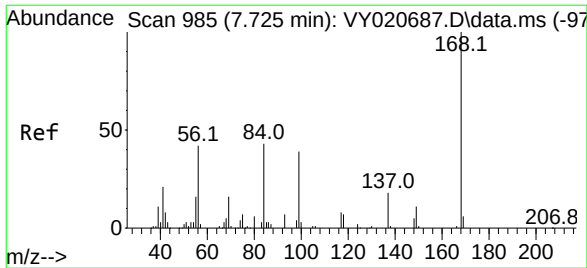


#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.719 min Scan# 98
Delta R.T. -0.006 min
Lab File: VY020714.D
Acq: 26 Dec 2024 13:56

Instrument :
MSVOA_Y
ClientSampleId :
VY1226SBL01



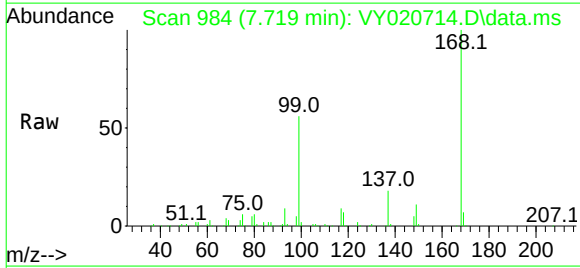



Tgt Ion:168 Resp: 99549
Ion Ratio Lower Upper
168 100
99 56.4 43.8 65.6

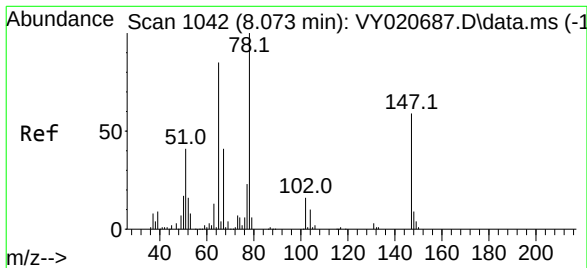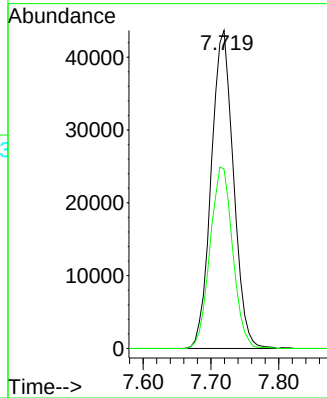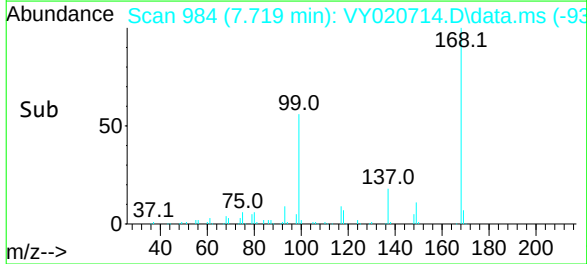

#33
1,2-Dichloroethane-d4
Concen: 64.652 ug/l
RT: 8.067 min Scan# 1041
Delta R.T. -0.006 min
Lab File: VY020714.D
Acq: 26 Dec 2024 13:56

Tgt Ion: 65 Resp: 52717
Ion Ratio Lower Upper
65 100
67 48.8 0.0 98.0

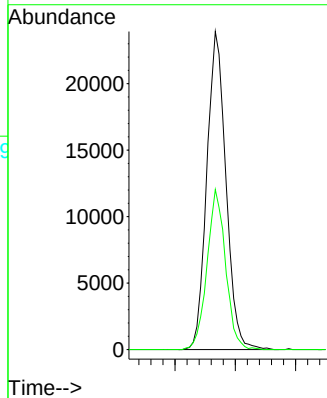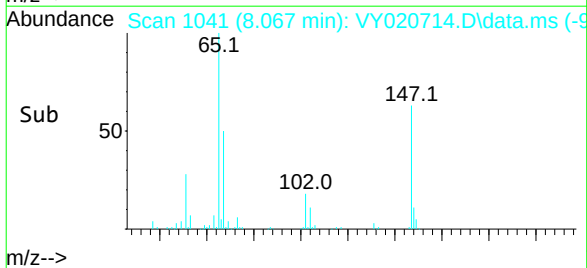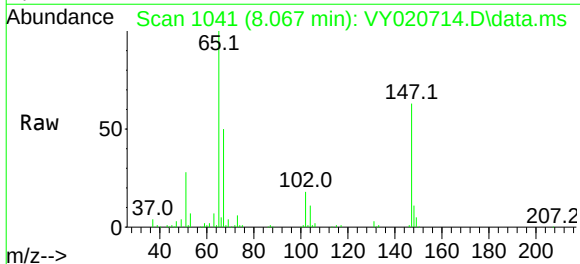

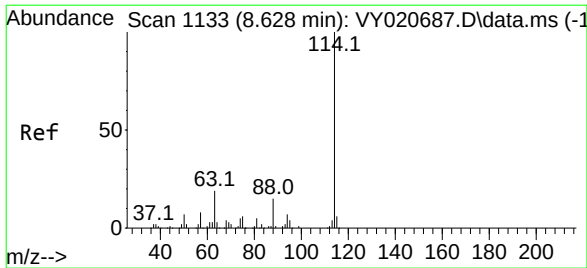

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.622 min Scan# 11

Delta R.T. -0.006 min

Lab File: VY020714.D

Acq: 26 Dec 2024 13:56

Instrument :

MSVOA_Y

ClientSampleId :

VY1226SBL01





Tgt Ion:114 Resp: 157271

Ion Ratio Lower Upper

114 100

63 18.5 0.0 38.4

88 15.5 0.0 30.4

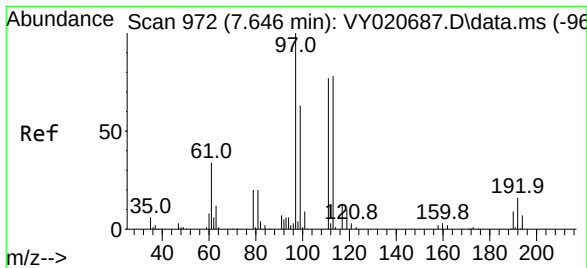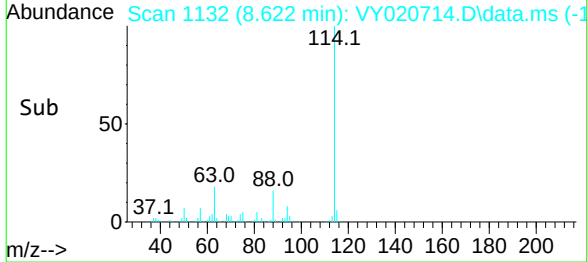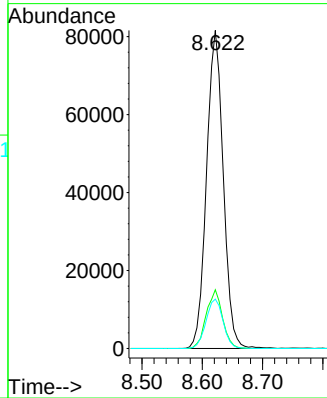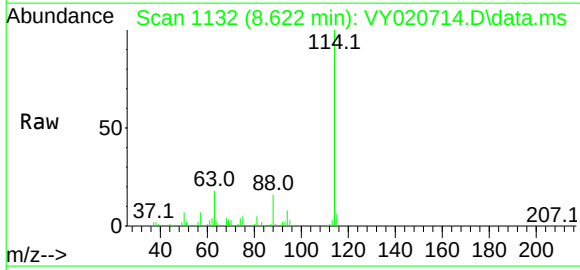

#35

Dibromofluoromethane

Concen: 57.586 ug/l

RT: 7.640 min Scan# 971

Delta R.T. -0.006 min

Lab File: VY020714.D

Acq: 26 Dec 2024 13:56




Tgt Ion:113 Resp: 49885


Ion Ratio Lower Upper

113 100

111 101.3 79.8 119.8

192 21.7 17.0 25.6

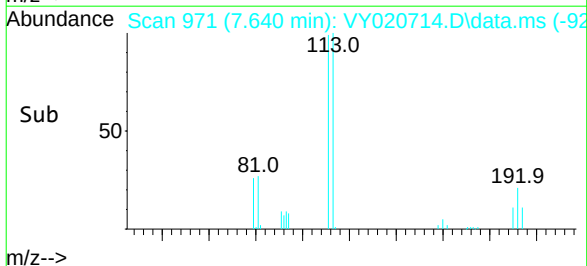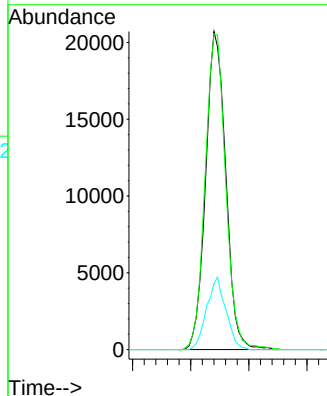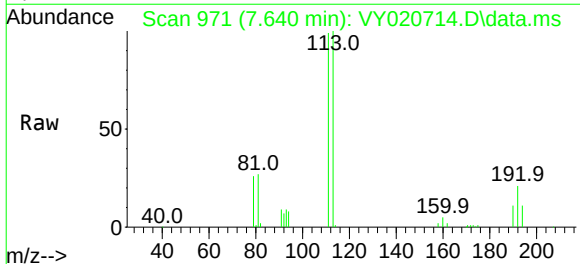

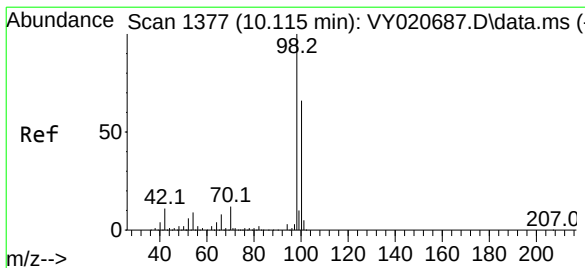

#50

Toluene-d8

Concen: 52.569 ug/l

RT: 10.109 min Scan# 1376

Delta R.T. -0.006 min

Lab File: VY020714.D

Acq: 26 Dec 2024 13:56

Instrument :

MSVOA_Y

ClientSampleId :





VY1226SBL01

Tgt Ion: 98 Resp: 181408

Ion Ratio Lower Upper

98 100

100 65.6 52.2 78.4

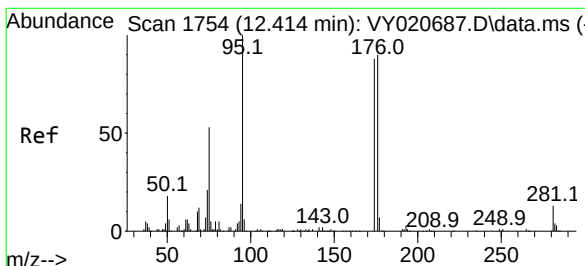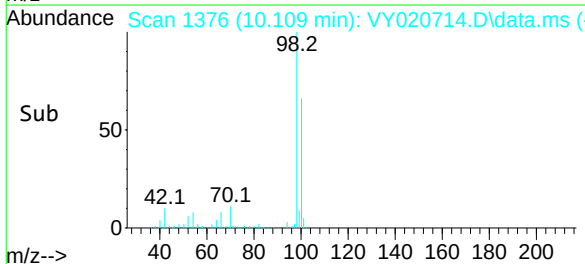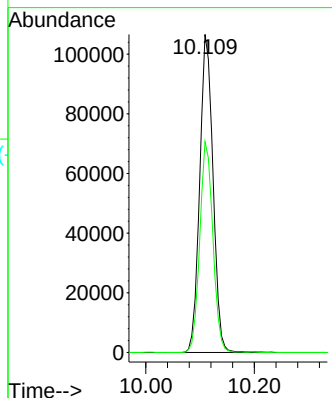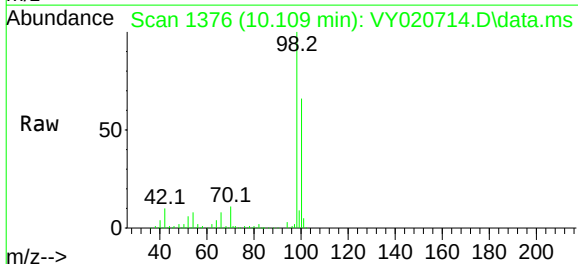

#62

4-Bromofluorobenzene

Concen: 50.981 ug/l

RT: 12.407 min Scan# 1753

Delta R.T. -0.007 min

Lab File: VY020714.D

Acq: 26 Dec 2024 13:56




Tgt Ion: 95 Resp: 58692


Ion Ratio Lower Upper

95 100

174 90.7 0.0 179.2

176 87.5 0.0 179.8

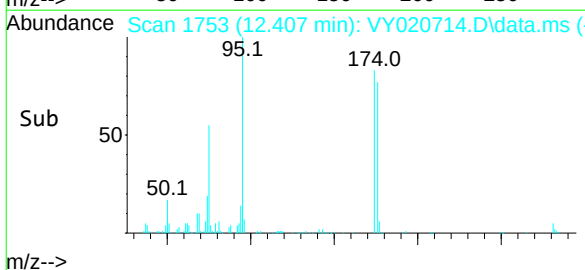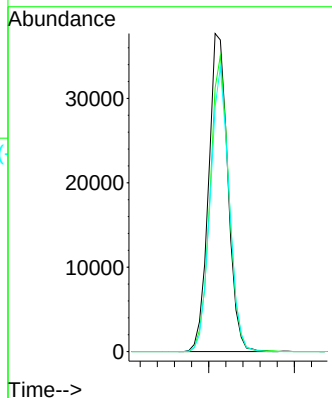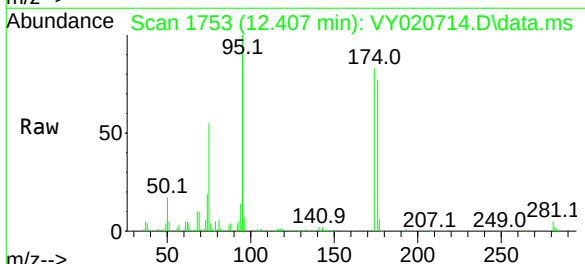

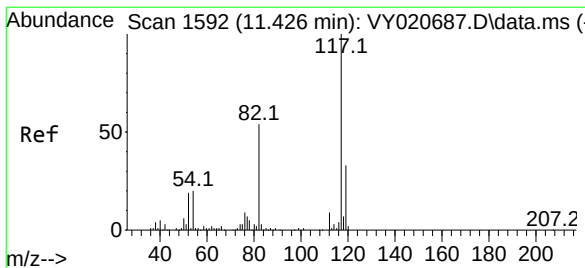

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.420 min Scan# 1591

Delta R.T. -0.006 min

Lab File: VY020714.D

Acq: 26 Dec 2024 13:56

Instrument :

MSVOA_Y

ClientSampleId :

VY1226SBL01





Tgt Ion:117 Resp: 133794

Ion Ratio Lower Upper

117 100

82 52.2 43.4 65.2

119 32.1 26.6 39.8

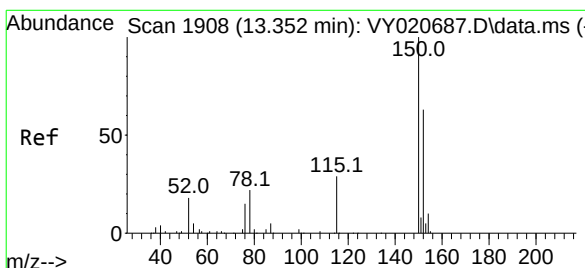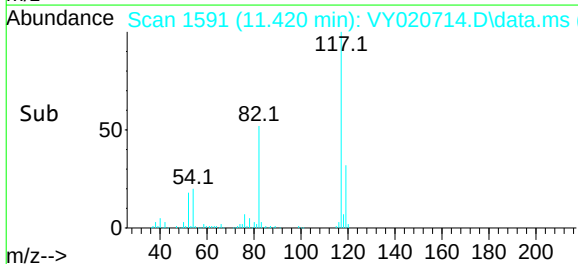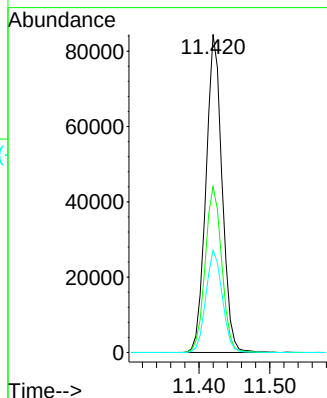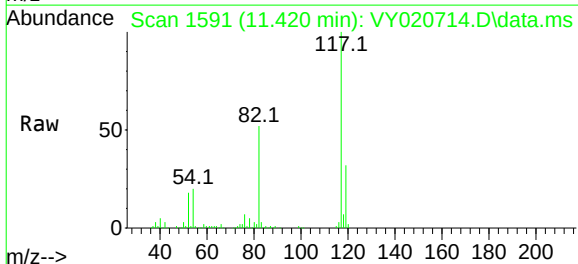

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.352 min Scan# 1908

Delta R.T. 0.000 min

Lab File: VY020714.D

Acq: 26 Dec 2024 13:56

Tgt Ion:152 Resp: 56315

Ion Ratio Lower Upper

152 100

115 57.9 30.3 90.9

150 156.9 0.0 349.0

