
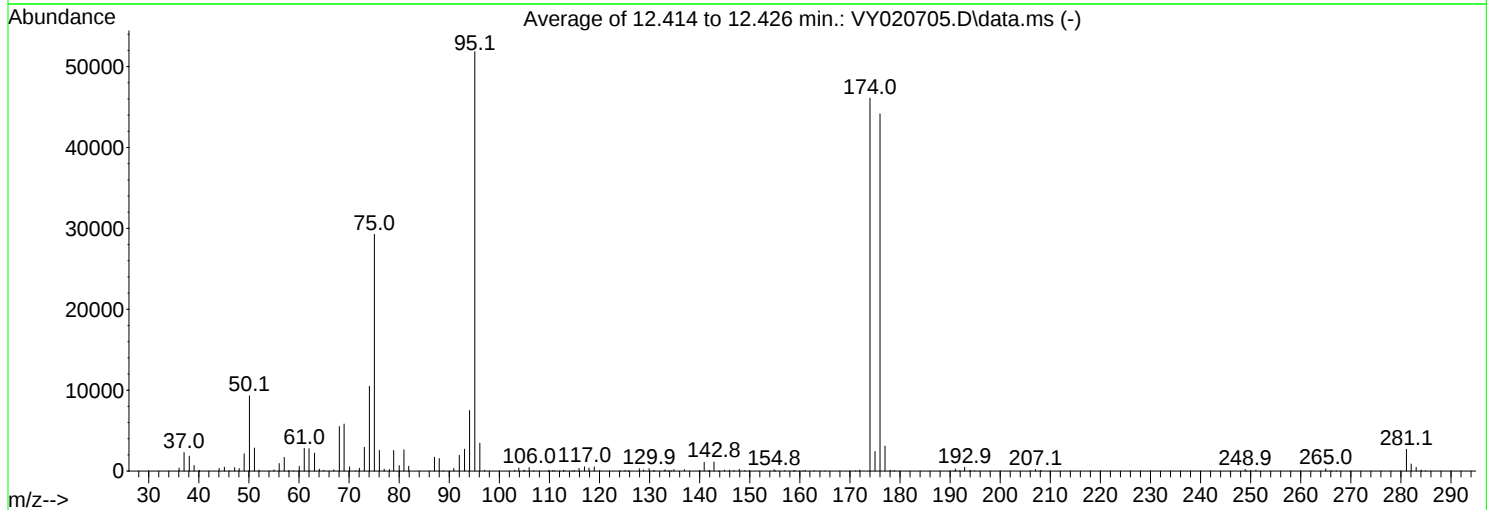


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY122624\
Data File : VY020705.D
Acq On : 26 Dec 2024 08:29
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y122624S.M
Title : SW846 8260
Last Update : Thu Dec 26 16:12:28 2024

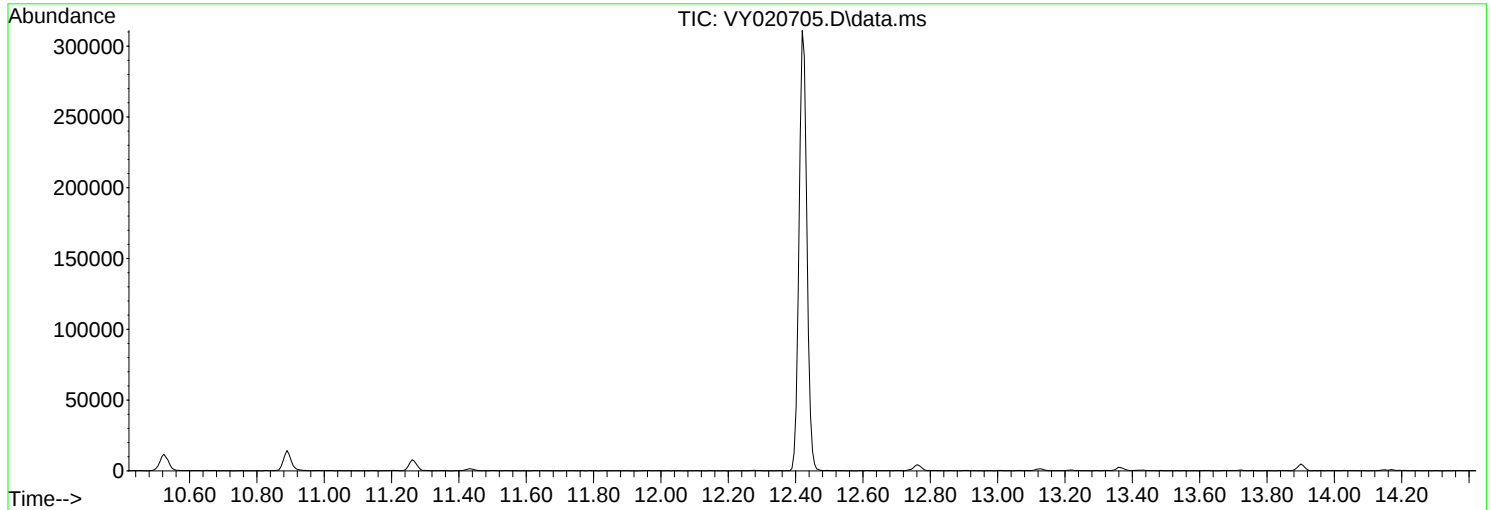

AutoFind: Scans 1754, 1755, 1756; Background Corrected with Scan 1747

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.9	9300	PASS
75	95	30	60	56.5	29264	PASS
95	95	100	100	100.0	51840	PASS
96	95	5	9	6.7	3450	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	88.9	46104	PASS
175	174	5	9	5.3	2423	PASS
176	174	95	101	95.8	44160	PASS
177	176	5	9	7.0	3092	PASS