

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY122722\
 Data File : VY012015.D
 Acq On : 27 Dec 2022 14:12
 Operator : KP/MD
 Sample : N6190-01RE
 Misc : 6.16g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :

Quant Time: Dec 28 00:38:38 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y122022S.M
 Quant Title : SW846 8260
 QLast Update : Tue Dec 20 12:37:37 2022
 Response via : Initial Calibration


Compound	R.T. QIon		Response	Conc	Units	Dev(Min)
Internal Standards						
1) Pentafluorobenzene	7.795	168	1020	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.697	114	2301	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.495	117	2720	50.000	ug/l	# 0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	991	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.149	65	1628	158.423	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	= 316.840%#	
35) Dibromofluoromethane	7.710	113	474	34.217	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	= 68.440%	
50) Toluene-d8	10.185	98	3007	53.502	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	= 107.000%	
62) 4-Bromofluorobenzene	12.483	95	1113	58.881	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	= 117.760%	
Target Compounds						Qvalue
3) Chloromethane	2.125	50	128	14.100	ug/l #	41
4) Vinyl Chloride	2.326	62	24	2.397	ug/l #	43
5) Bromomethane	2.674	94	273	38.329	ug/l	84
10) Methyl Iodide	4.094	142	733	54.914	ug/l #	80
16) Acetone	3.948	43	324	108.420	ug/l #	40
17) Carbon Disulfide	4.204	76	170	5.522	ug/l #	75
20) Methylene Chloride	4.716	84	178	10.265	ug/l #	42
44) Trichloroethene	8.929	130	27	1.506	ug/l	2
60) Dibromochloromethane	10.721	129	70	4.627	ug/l #	11
64) Tetrachloroethene	10.715	164	50	2.100	ug/l #	42
65) Chlorobenzene	11.520	112	215	3.807	ug/l #	43
67) Ethyl Benzene	11.593	91	204	1.998	ug/l #	81
68) m/p-Xylenes	11.703	106	76	1.914	ug/l #	1
70) Styrene	12.044	104	148	2.386	ug/l #	26
73) Isopropylbenzene	12.331	105	154	2.094	ug/l #	49
76) 1,2,3-Trichloropropane	12.477	75	523	42.412	ug/l #	100
78) n-propylbenzene	12.672	91	261	2.953	ug/l #	52
79) 2-Chlorotoluene	12.751	91	176	3.542	ug/l #	40
80) 1,3,5-Trimethylbenzene	12.812	105	154	2.446	ug/l #	29
81) trans-1,4-Dichloro-2-b...	12.477	75	523	116.146	ug/l #	13
82) 4-Chlorotoluene	12.861	91	305	5.933	ug/l #	53
83) tert-Butylbenzene	13.074	119	119	2.230	ug/l #	62
84) 1,2,4-Trimethylbenzene	13.117	105	116	1.873	ug/l #	31
85) sec-Butylbenzene	13.251	105	270	3.389	ug/l	80
86) p-Isopropyltoluene	13.379	119	101	1.502	ug/l #	50
87) 1,3-Dichlorobenzene	13.373	146	208	6.079	ug/l	87
88) 1,4-Dichlorobenzene	13.373	146	208	6.115	ug/l	87
89) n-Butylbenzene	13.696	91	96	1.577	ug/l #	33
91) 1,2-Dichlorobenzene	13.739	146	177	5.934	ug/l #	58
95) Naphthalene	15.239	128	210	8.212	ug/l #	69
96) 1,2,3-Trichlorobenzene	15.416	180	20	1.348	ug/l #	12


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY122722\
Data File : VY012015.D
Acq On : 27 Dec 2022 14:12
Operator : KP/MD
Sample : N6190-01RE
Misc : 6.16g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :


Quant Time: Dec 28 00:38:38 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y122022S.M
Quant Title : SW846 8260
QLast Update : Tue Dec 20 12:37:37 2022
Response via : Initial Calibration

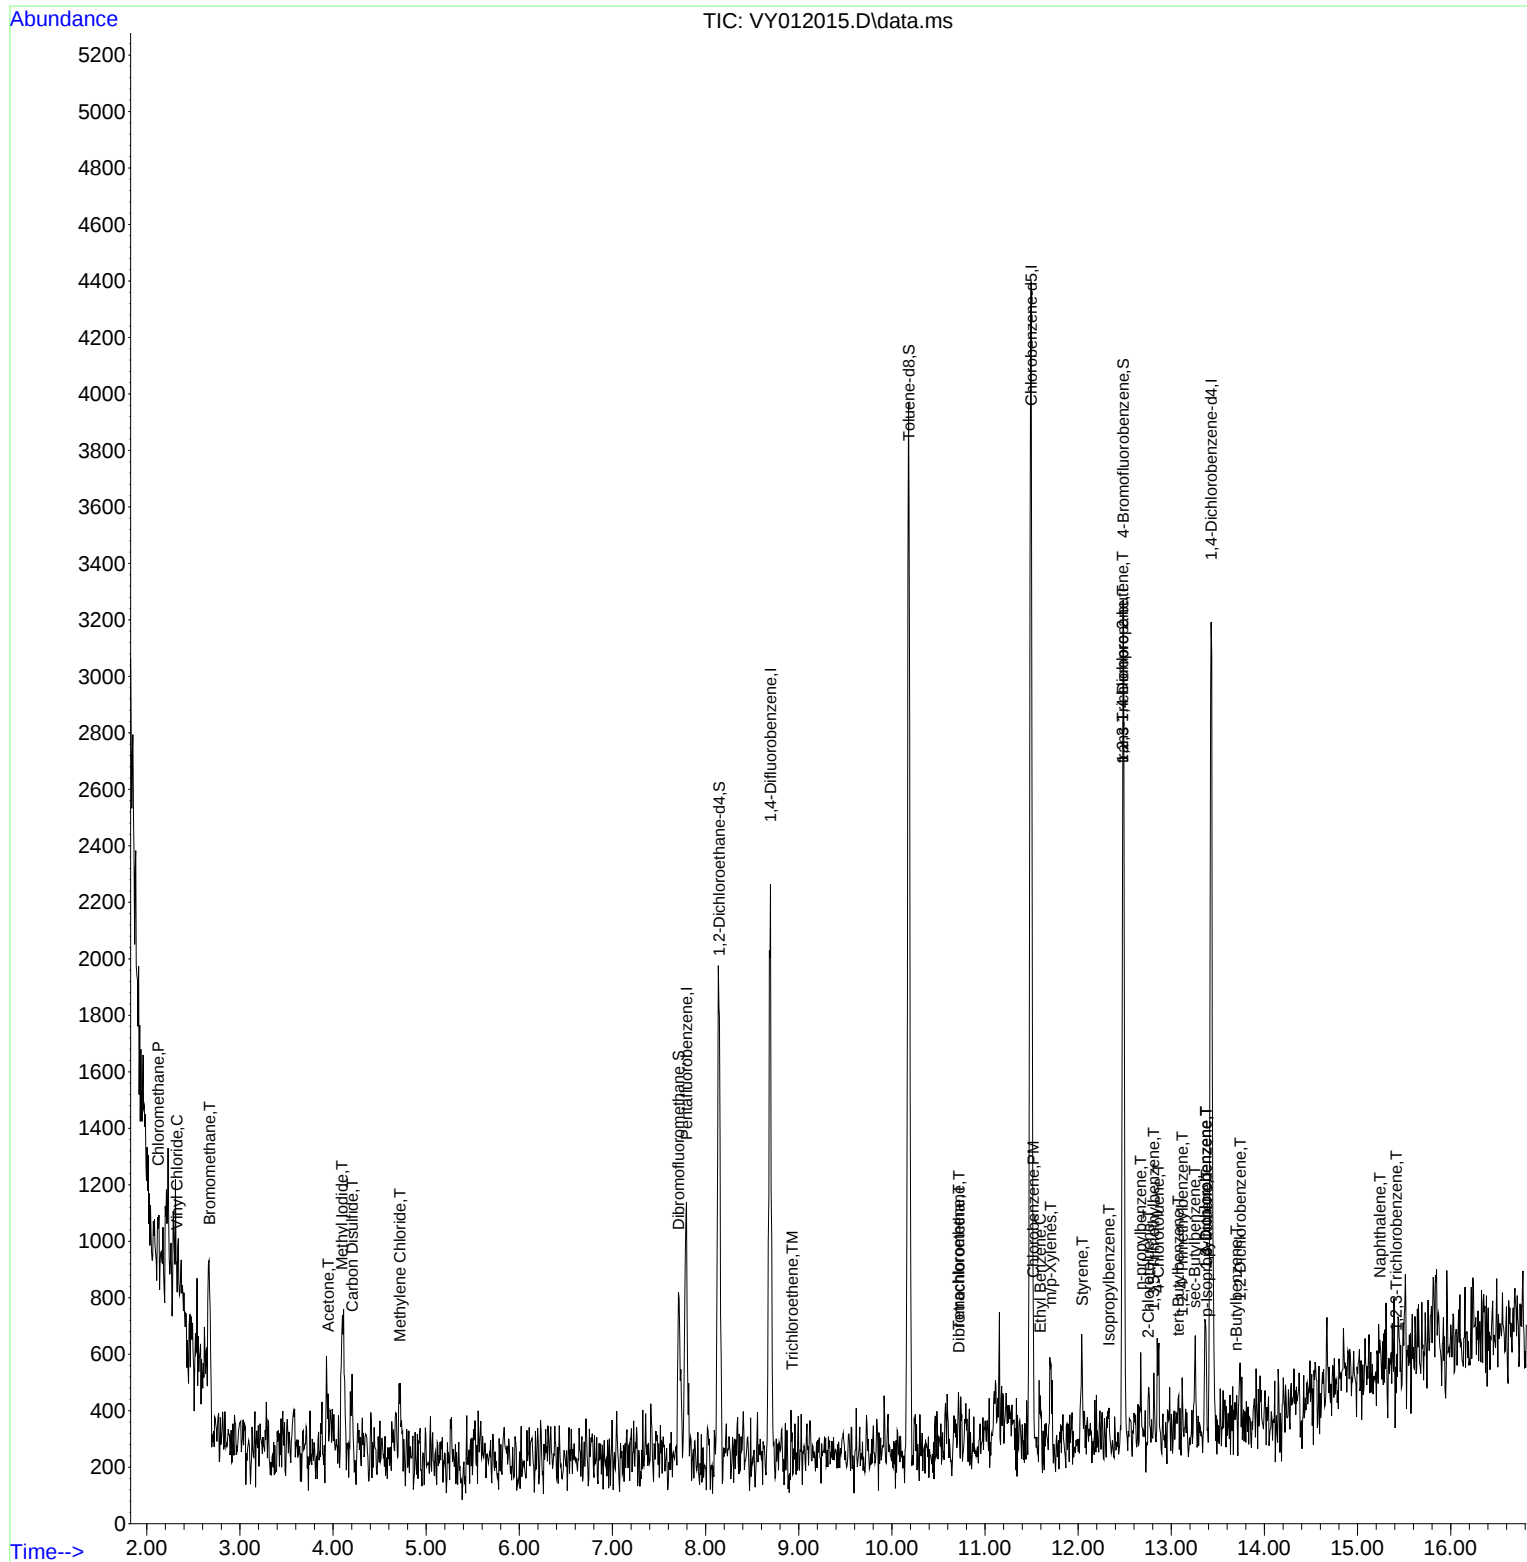






#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.795 min Scan# 91
Delta R.T. 0.006 min
Lab File: VY012015.D
Acq: 27 Dec 2022 14:12

Instrument :
MSVOA_Y
ClientSampleId :






Tgt Ion:168 Resp: 1020
Ion Ratio Lower Upper
168 100
99 55.0 44.0 66.0

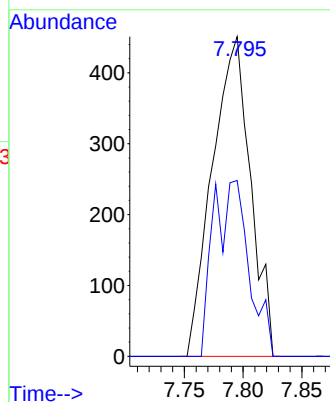


#3
Chloromethane
Concen: 14.100 ug/l
RT: 2.125 min Scan# 50
Delta R.T. 0.012 min
Lab File: VY012015.D
Acq: 27 Dec 2022 14:12

Tgt Ion: 50 Resp: 128
Ion Ratio Lower Upper
50 100
52 0.0 26.8 40.2#

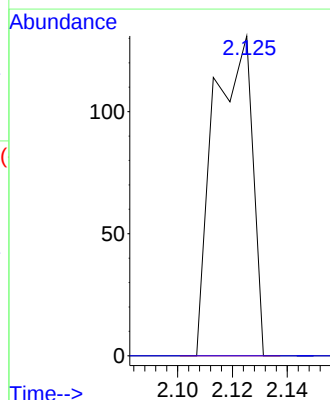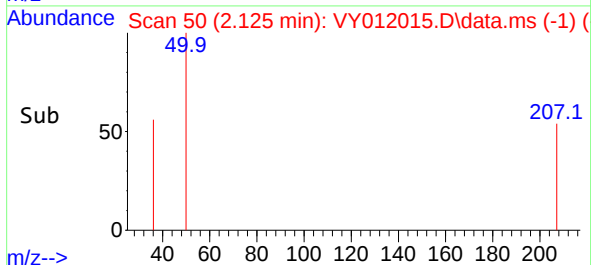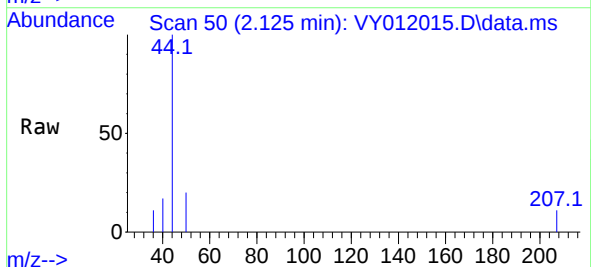

Abundance Scan 71 (2.253 min): VY011739.D\data.ms (-63)

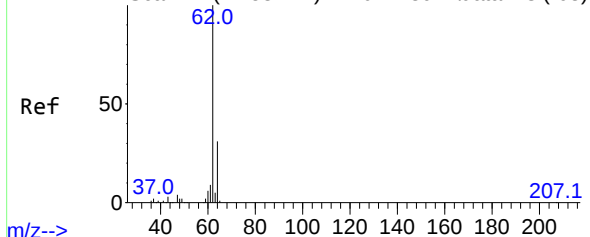

#4

Vinyl Chloride

Concen: 2.397 ug/l

RT: 2.326 min Scan# 81

Delta R.T. 0.073 min

Lab File: VY012015.D

Acq: 27 Dec 2022 14:12

Instrument :

MSVOA_Y

ClientSampleId :



Tgt Ion: 62 Resp: 24

Ion Ratio Lower Upper


62 100

64 0.0 25.0 37.6#


Abundance Scan 83 (2.326 min): VY012015.D\data.ms

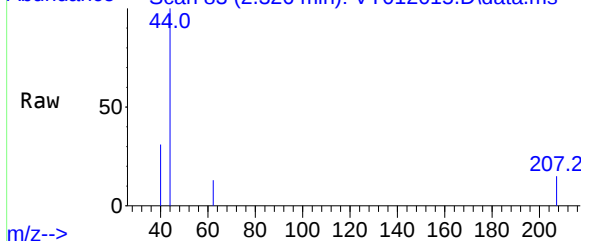

Abundance Scan 83 (2.326 min): VY012015.D\data.ms (-22)

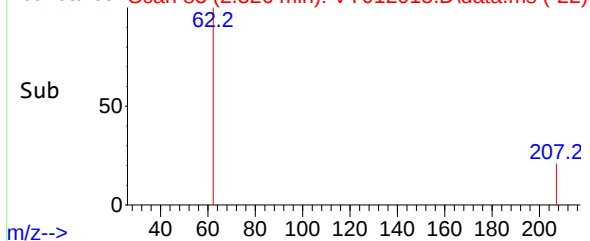

Abundance Scan 136 (2.650 min): VY011739.D\data.ms (-12)

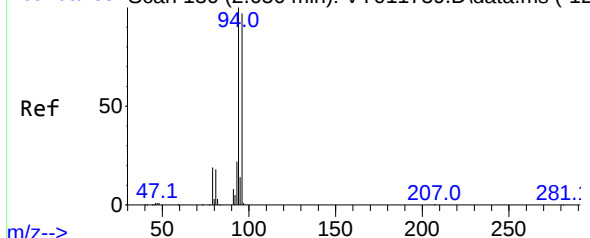

#5

Bromomethane

Concen: 38.329 ug/l

RT: 2.674 min Scan# 140

Delta R.T. 0.024 min

Lab File: VY012015.D

Acq: 27 Dec 2022 14:12



Tgt Ion: 94 Resp: 273

Ion Ratio Lower Upper


94 100


96 80.7 77.4 116.2

Abundance Scan 140 (2.674 min): VY012015.D\data.ms

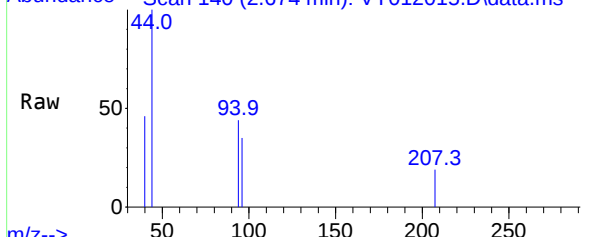


Abundance Scan 140 (2.674 min): VY012015.D\data.ms (-87)

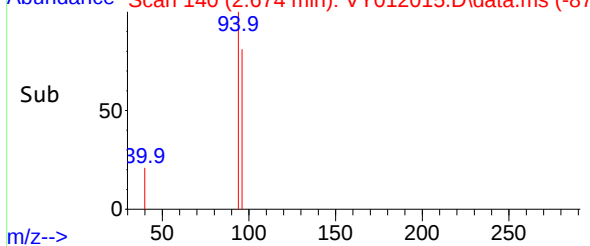



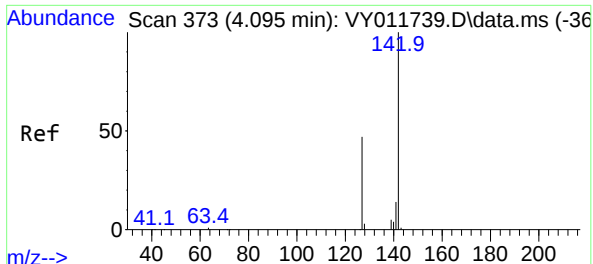


#10
Methyl Iodide
Concen: 54.914 ug/l
RT: 4.094 min Scan# 31
Delta R.T. -0.001 min
Lab File: VY012015.D
Acq: 27 Dec 2022 14:12

Instrument :
MSVOA_Y
ClientSampleId :



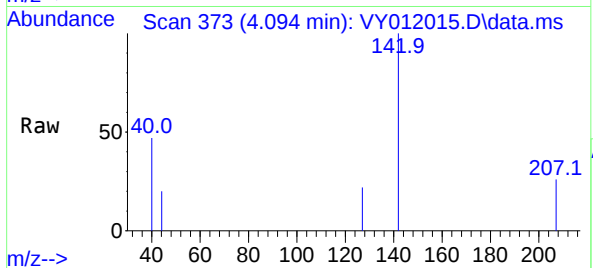



Tgt Ion:142 Resp: 733
Ion Ratio Lower Upper
142 100
127 35.7 37.0 55.4#
141 0.0 11.4 17.0#

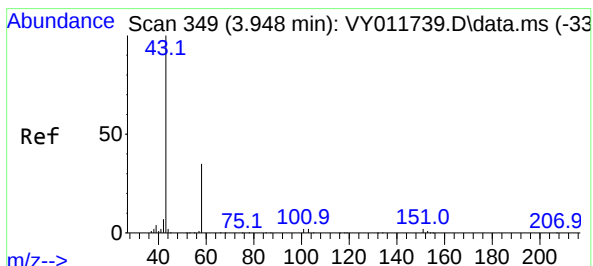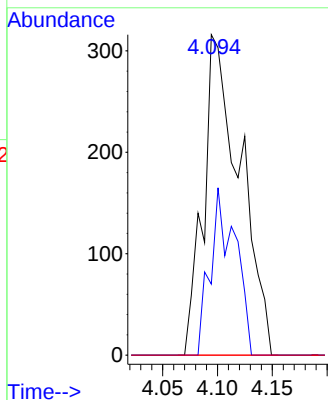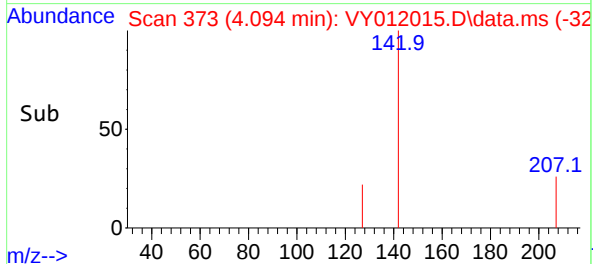

#16
Acetone
Concen: 108.420 ug/l
RT: 3.948 min Scan# 349
Delta R.T. 0.000 min
Lab File: VY012015.D
Acq: 27 Dec 2022 14:12


Tgt Ion: 43 Resp: 324
Ion Ratio Lower Upper
43 100
58 0.0 27.9 41.9#

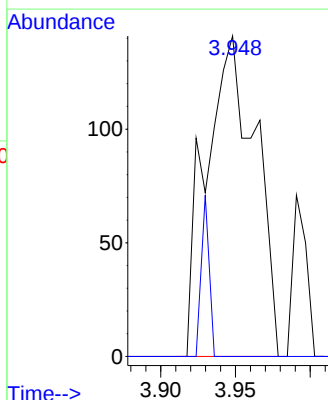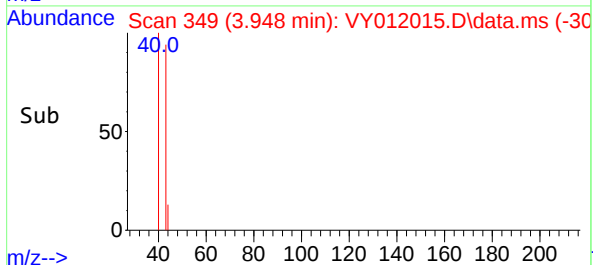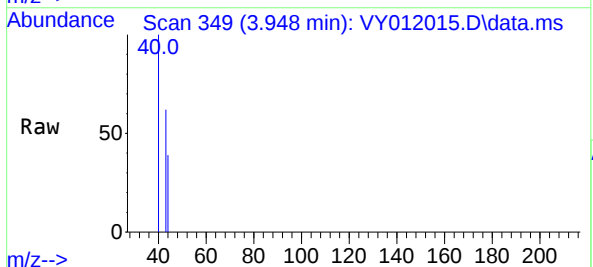






#17
Carbon Disulfide
Concen: 5.522 ug/l
RT: 4.204 min Scan# 391
Delta R.T. 0.006 min
Lab File: VY012015.D
Acq: 27 Dec 2022 14:12


Instrument :
MSVOA_Y
ClientSampleId :





Tgt Ion: 76 Resp: 170
Ion Ratio Lower Upper
76 100
78 0.0 7.2 10.8#

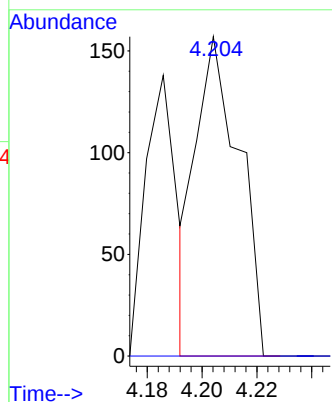


#20
Methylene Chloride
Concen: 10.265 ug/l
RT: 4.716 min Scan# 475
Delta R.T. 0.000 min
Lab File: VY012015.D
Acq: 27 Dec 2022 14:12

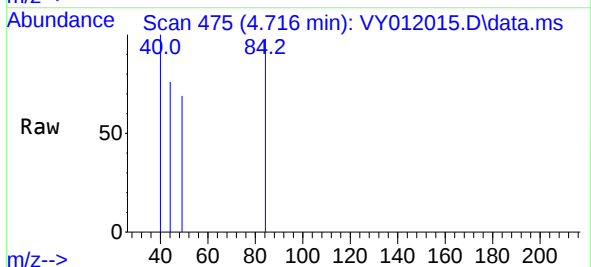

Tgt Ion: 84 Resp: 178
Ion Ratio Lower Upper
84 100
49 69.7 95.4 143.2#
51 0.0 29.9 44.9#
86 0.0 49.6 74.4#



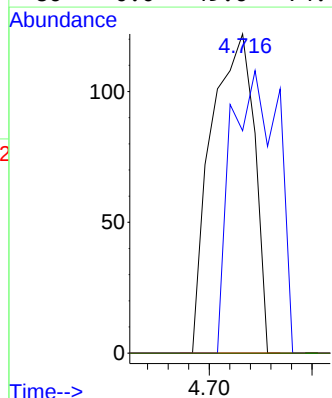
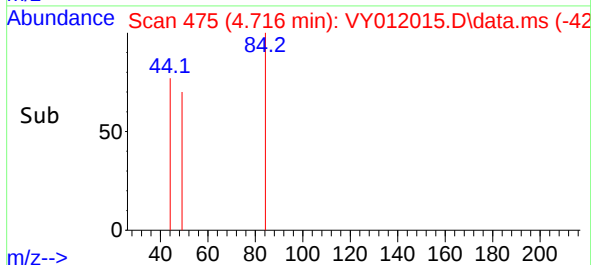


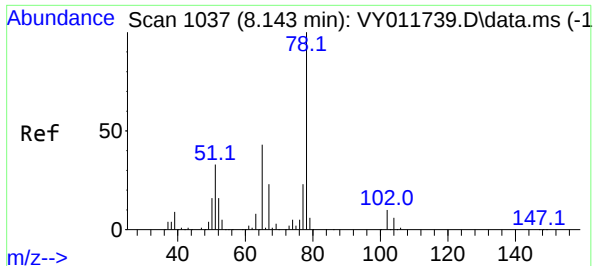

#33
1,2-Dichloroethane-d4
Concen: 158.423 ug/l
RT: 8.149 min Scan# 110
Delta R.T. 0.006 min
Lab File: VY012015.D
Acq: 27 Dec 2022 14:12




Instrument :
MSVOA_Y
ClientSampleId :


Tgt Ion: 65 Resp: 1628
Ion Ratio Lower Upper
65 100
67 48.3 0.0 103.2

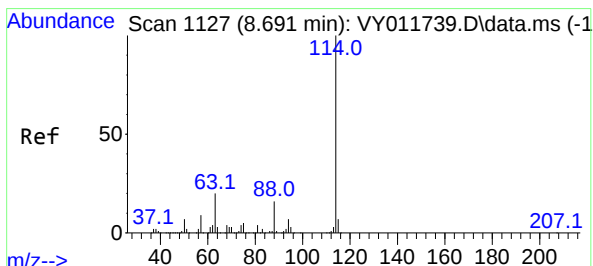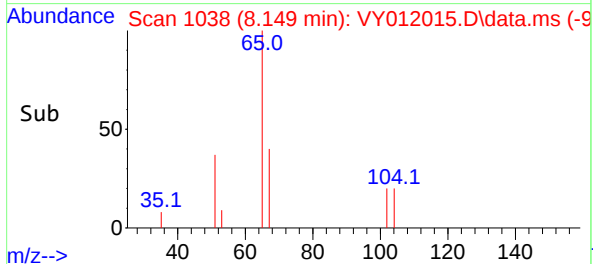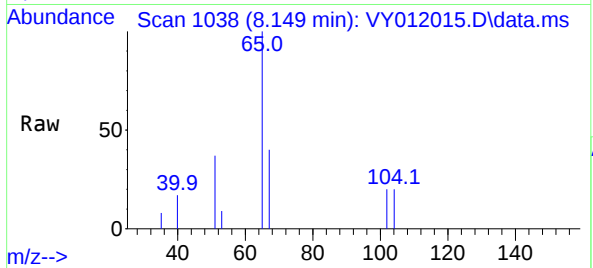

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.697 min Scan# 1128
Delta R.T. 0.006 min
Lab File: VY012015.D
Acq: 27 Dec 2022 14:12


Tgt Ion: 114 Resp: 2301
Ion Ratio Lower Upper
114 100
63 21.2 0.0 39.6
88 15.6 0.0 32.2

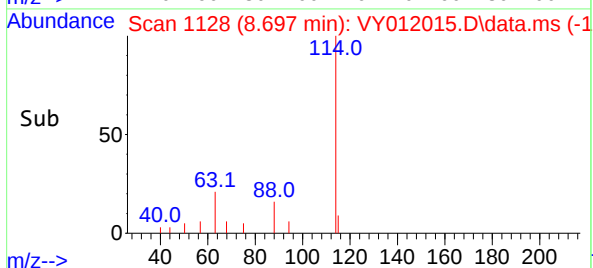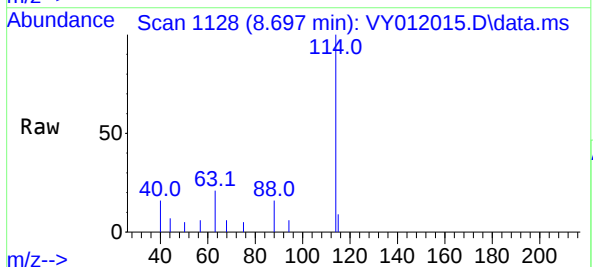






#35
Dibromofluoromethane
Concen: 34.217 ug/l
RT: 7.710 min Scan# 91
Delta R.T. -0.006 min
Lab File: VY012015.D
Acq: 27 Dec 2022 14:12

Instrument :
MSVOA_Y
ClientSampleId :







Tgt Ion:113 Resp: 474
Ion Ratio Lower Upper
113 100
111 117.9 83.0 124.4
192 0.0 16.0 24.0#

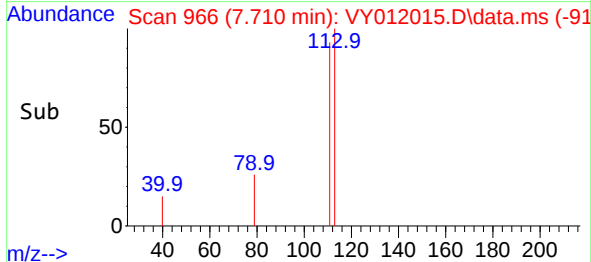

#44
Trichloroethene
Concen: 1.506 ug/l
RT: 8.929 min Scan# 1166
Delta R.T. -0.012 min
Lab File: VY012015.D
Acq: 27 Dec 2022 14:12

Tgt Ion:130 Resp: 27
Ion Ratio Lower Upper
130 100
95 0.0 0.0 190.6


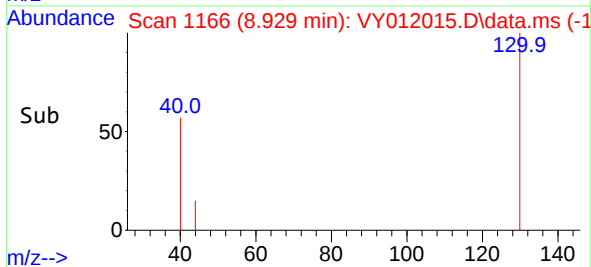

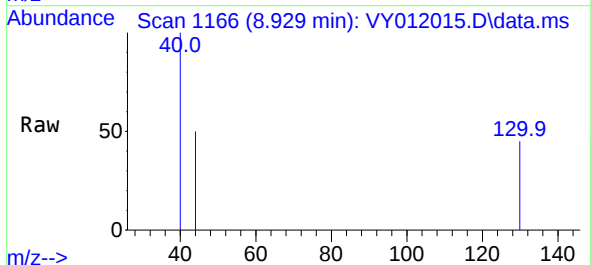




#50
Toluene-d8
Concen: 53.502 ug/l
RT: 10.185 min Scan# 11
Delta R.T. 0.006 min
Lab File: VY012015.D
Acq: 27 Dec 2022 14:12




Instrument :
MSVOA_Y
ClientSampleId :


Tgt Ion: 98 Resp: 3007
Ion Ratio Lower Upper
98 100
100 59.9 51.9 77.9

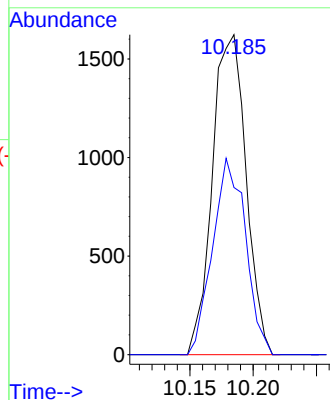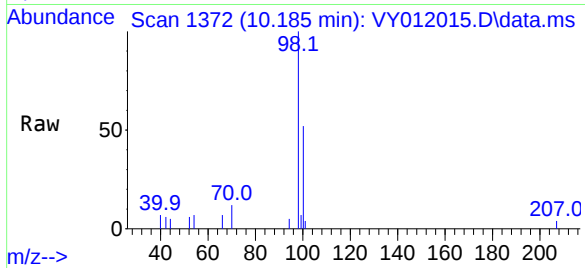

#60
Dibromochloromethane
Concen: 4.627 ug/l
RT: 10.721 min Scan# 1460
Delta R.T. -0.262 min
Lab File: VY012015.D
Acq: 27 Dec 2022 14:12


Tgt Ion: 129 Resp: 70
Ion Ratio Lower Upper
129 100
127 0.0 38.9 116.6#

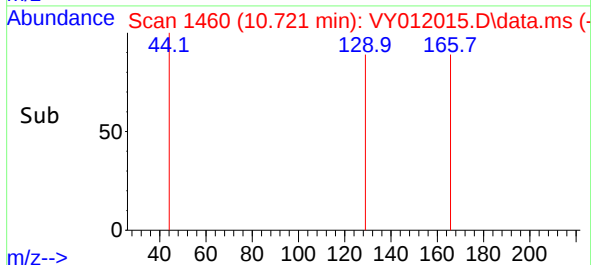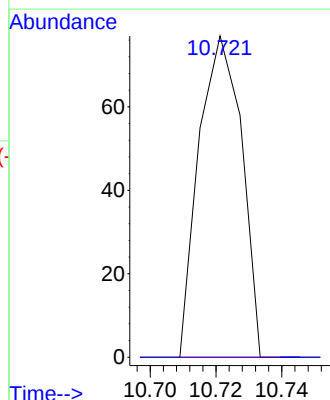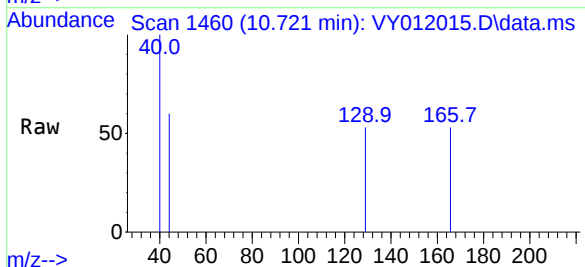






#62
4-Bromofluorobenzene
Concen: 58.881 ug/l
RT: 12.483 min Scan# 1113
Delta R.T. 0.000 min
Lab File: VY012015.D
Acq: 27 Dec 2022 14:12

Instrument :
MSVOA_Y
ClientSampleId :







Tgt Ion: 95 Resp: 1113
Ion Ratio Lower Upper
95 100
174 92.5 0.0 172.0
176 84.6 0.0 167.6

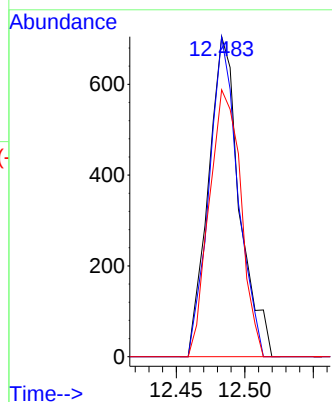

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.495 min Scan# 1587
Delta R.T. 0.006 min
Lab File: VY012015.D
Acq: 27 Dec 2022 14:12


Tgt Ion: 117 Resp: 2720
Ion Ratio Lower Upper
117 100
82 54.3 44.8 67.2
119 42.2 25.4 38.2#

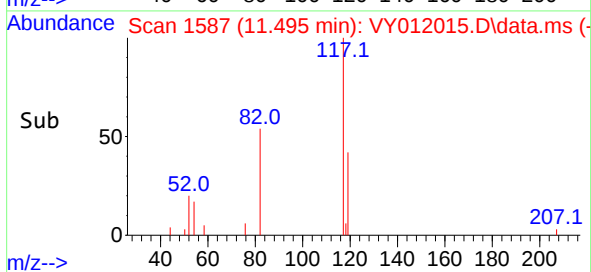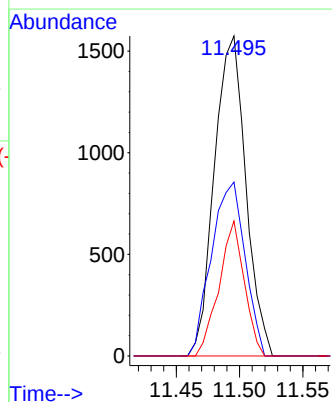



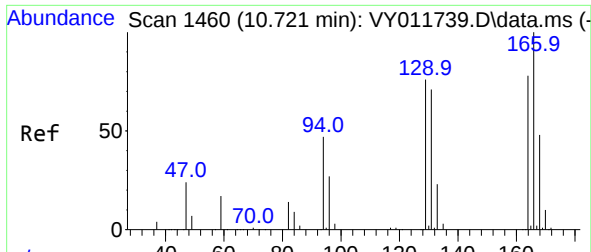


#64
Tetrachloroethene
Concen: 2.100 ug/l
RT: 10.715 min Scan# 1460
Delta R.T. -0.006 min
Lab File: VY012015.D
Acq: 27 Dec 2022 14:12

Instrument :
MSVOA_Y
ClientSampleId :



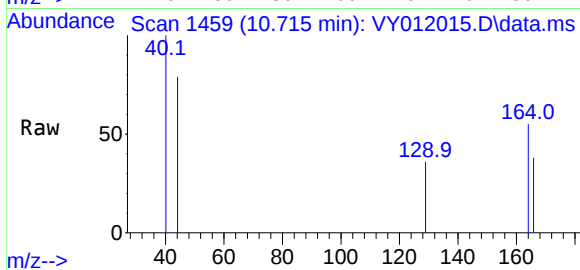



Tgt Ion:164 Resp: 50
Ion Ratio Lower Upper
164 100
166 68.7 102.3 153.5#
129 66.3 77.2 115.8#
131 0.0 72.5 108.7#

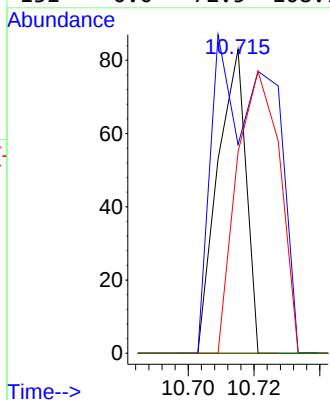

#65
Chlorobenzene
Concen: 3.807 ug/l
RT: 11.520 min Scan# 1591
Delta R.T. 0.006 min
Lab File: VY012015.D
Acq: 27 Dec 2022 14:12

Tgt Ion:112 Resp: 215
Ion Ratio Lower Upper
112 100
114 0.0 25.3 37.9#

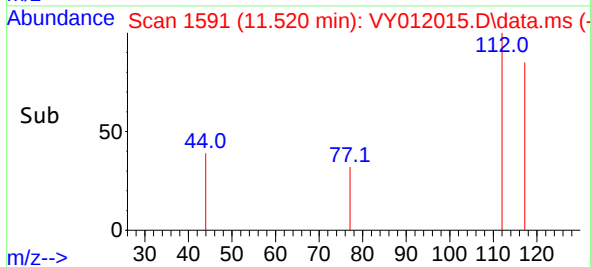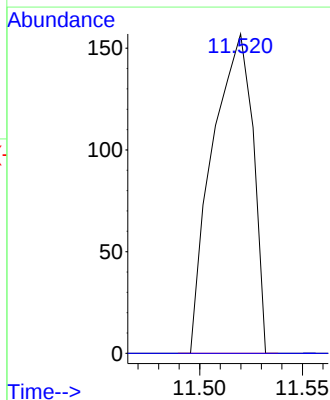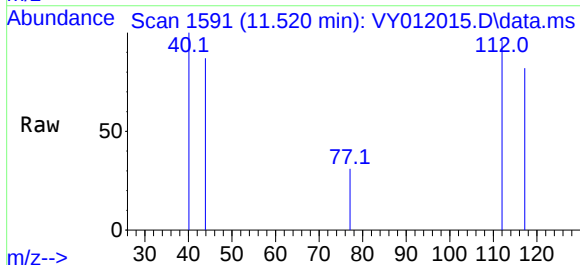



#67

Ethyl Benzene

Concen: 1.998 ug/l

RT: 11.593 min Scan# 1603

Delta R.T. -0.000 min

Lab File: VY012015.D

Acq: 27 Dec 2022 14:12

Instrument :

MSVOA_Y





ClientSampleId :

Tgt Ion: 91 Resp: 204

Ion Ratio Lower Upper

91 100

106 41.6 25.0 37.4#

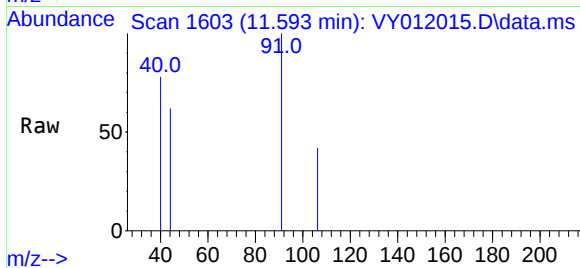

#68

m/p-Xylenes

Concen: 1.914 ug/l

RT: 11.703 min Scan# 1621

Delta R.T. -0.000 min

Lab File: VY012015.D




Acq: 27 Dec 2022 14:12


Tgt Ion: 106 Resp: 76

Ion Ratio Lower Upper

106 100


91 431.6 162.5 243.7#

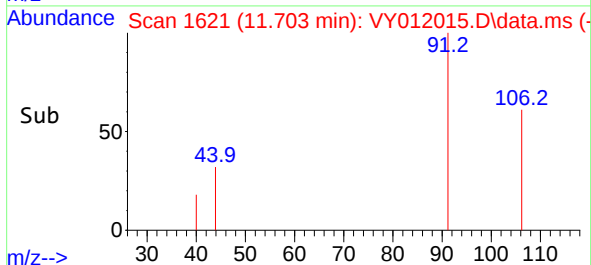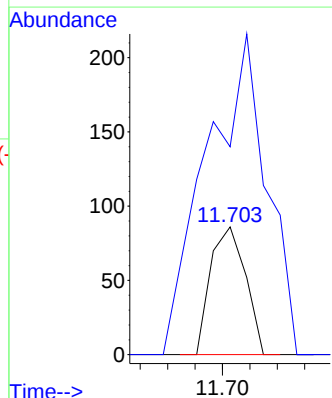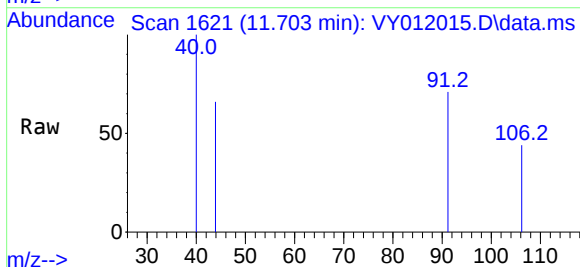






#70
Styrene
Concen: 2.386 ug/l
RT: 12.044 min Scan# 1
Delta R.T. -0.000 min
Lab File: VY012015.D
Acq: 27 Dec 2022 14:12

Instrument :
MSVOA_Y
ClientSampleId :



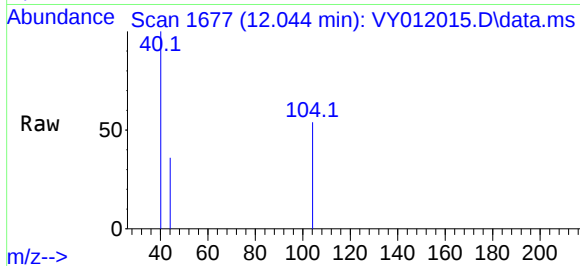



Tgt Ion:104 Resp: 148
Ion Ratio Lower Upper
104 100
78 0.0 39.4 59.0#
103 0.0 43.0 64.4#



#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.428 min Scan# 1904
Delta R.T. -0.000 min
Lab File: VY012015.D
Acq: 27 Dec 2022 14:12

Tgt Ion:152 Resp: 991
Ion Ratio Lower Upper
152 100
115 60.0 29.1 87.3
150 164.9 0.0 342.6


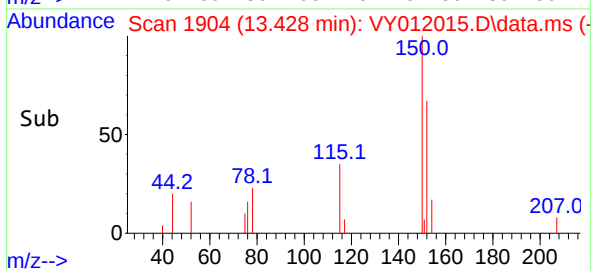

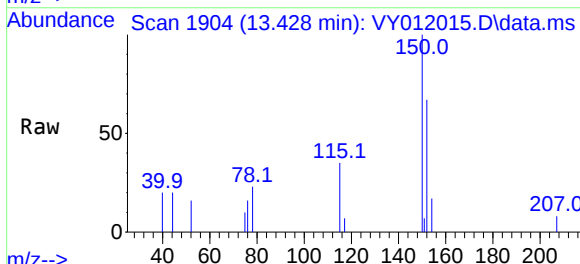


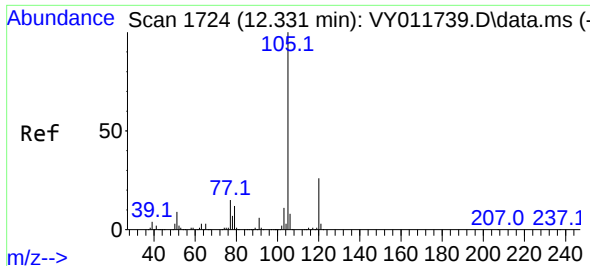

#73
Isopropylbenzene
Concen: 2.094 ug/l
RT: 12.331 min Scan# 11
Delta R.T. -0.000 min
Lab File: VY012015.D
Acq: 27 Dec 2022 14:12




Instrument :
MSVOA_Y
ClientSampleId :


Tgt Ion:105 Resp: 154
Ion Ratio Lower Upper
105 100
120 0.0 13.2 39.6#

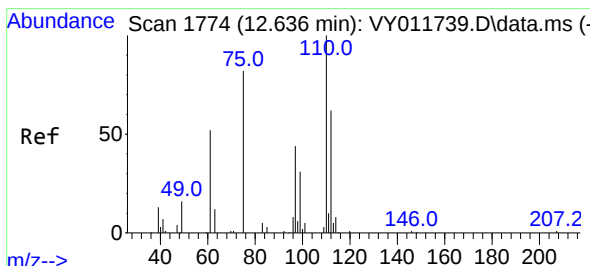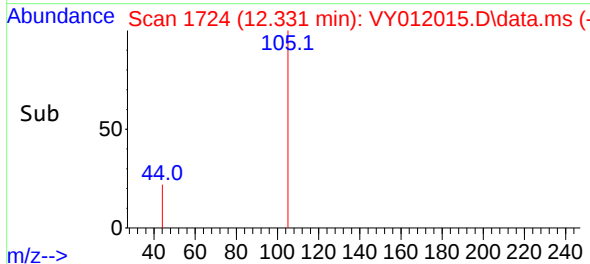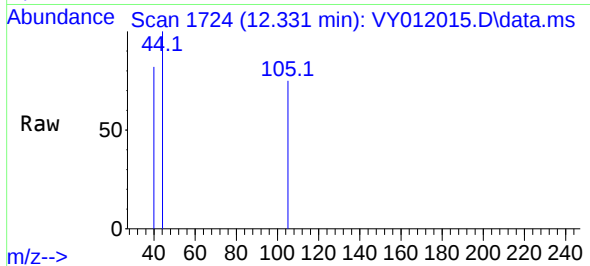

#76
1,2,3-Trichloropropane
Concen: 42.412 ug/l
RT: 12.477 min Scan# 1748
Delta R.T. -0.159 min
Lab File: VY012015.D
Acq: 27 Dec 2022 14:12

Tgt Ion: 75 Resp: 523
Ion Ratio Lower Upper
75 100
77 0.0 0.0 0.0


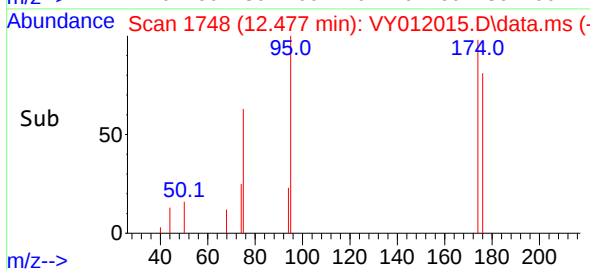

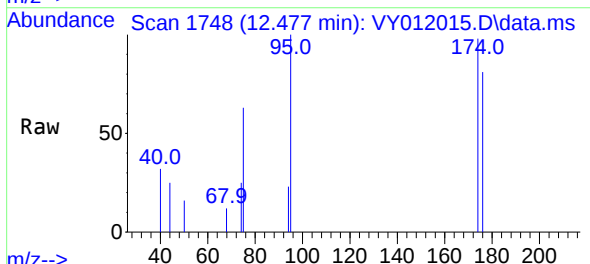




#78
n-propylbenzene
Concen: 2.953 ug/l
RT: 12.672 min Scan# 1780
Delta R.T. -0.000 min
Lab File: VY012015.D
Acq: 27 Dec 2022 14:12




Instrument :
MSVOA_Y
ClientSampleId :


Tgt Ion: 91 Resp: 261
Ion Ratio Lower Upper
91 100
120 0.0 11.8 35.4#

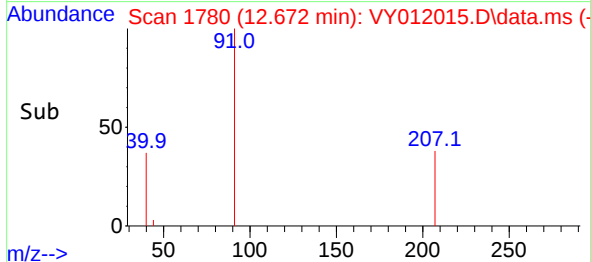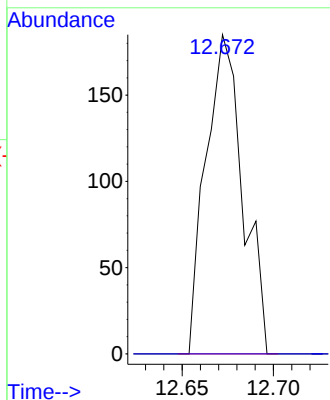

#79
2-Chlorotoluene
Concen: 3.542 ug/l
RT: 12.751 min Scan# 1793
Delta R.T. -0.006 min
Lab File: VY012015.D
Acq: 27 Dec 2022 14:12


Tgt Ion: 91 Resp: 176
Ion Ratio Lower Upper
91 100
126 0.0 17.2 51.5#

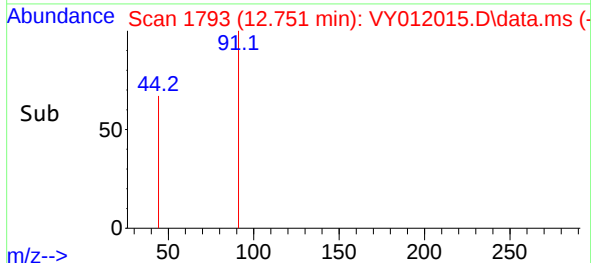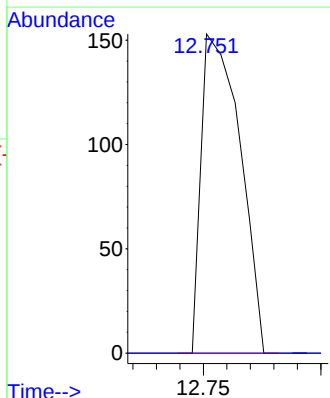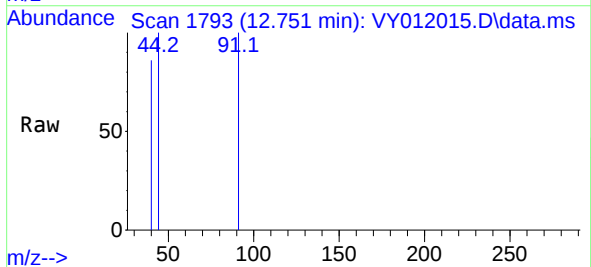






#80
1,3,5-Trimethylbenzene
Concen: 2.446 ug/l
RT: 12.812 min Scan# 11
Delta R.T. -0.000 min
Lab File: VY012015.D
Acq: 27 Dec 2022 14:12

Instrument :
MSVOA_Y
ClientSampleId :



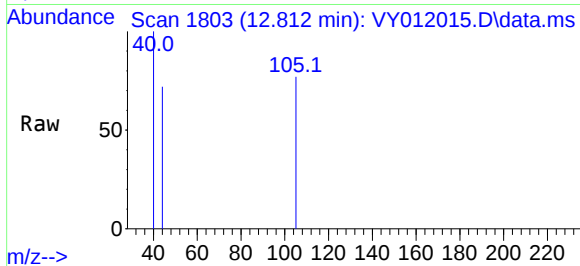



Tgt Ion:105 Resp: 154
Ion Ratio Lower Upper
105 100
120 0.0 24.2 72.6#



#81
trans-1,4-Dichloro-2-butene
Concen: 116.146 ug/l
RT: 12.477 min Scan# 1748
Delta R.T. 0.097 min
Lab File: VY012015.D
Acq: 27 Dec 2022 14:12

Tgt Ion: 75 Resp: 523
Ion Ratio Lower Upper
75 100
53 0.0 72.5 108.7#
89 0.0 37.0 55.4#


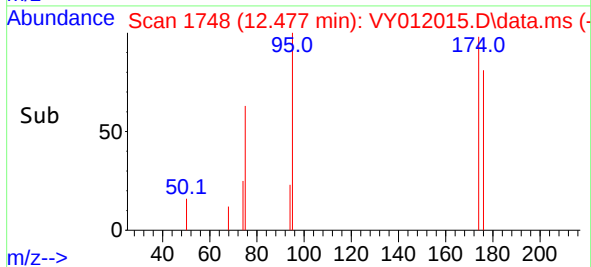

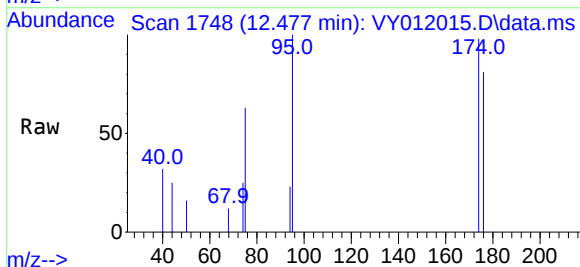




#82
4-Chlorotoluene
Concen: 5.933 ug/l
RT: 12.861 min Scan# 1810
Delta R.T. 0.006 min
Lab File: VY012015.D
Acq: 27 Dec 2022 14:12




Instrument :
MSVOA_Y
ClientSampleId :


Tgt Ion: 91 Resp: 305
Ion Ratio Lower Upper
91 100
126 6.9 17.1 51.2#

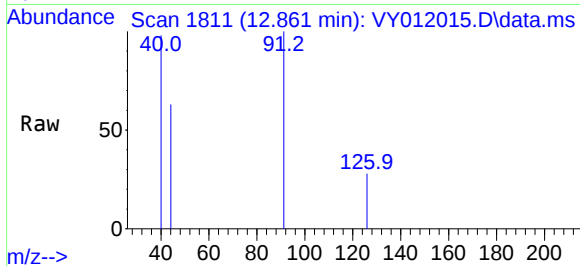

#83
tert-Butylbenzene
Concen: 2.230 ug/l
RT: 13.074 min Scan# 1846
Delta R.T. -0.000 min
Lab File: VY012015.D
Acq: 27 Dec 2022 14:12

Tgt Ion: 119 Resp: 119
Ion Ratio Lower Upper
119 100
91 89.9 32.3 96.8
134 0.0 13.0 39.0#


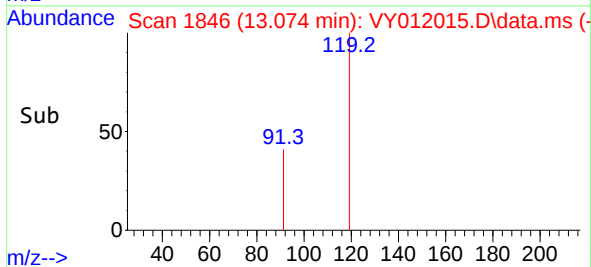

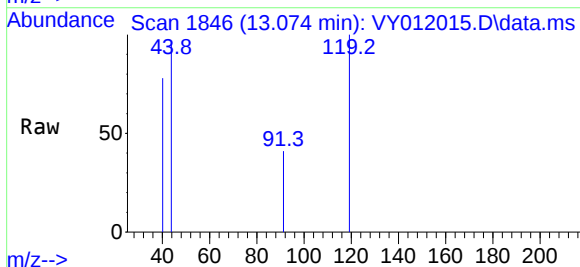




#84
1,2,4-Trimethylbenzene
Concen: 1.873 ug/l
RT: 13.117 min Scan# 1853
Delta R.T. -0.000 min
Lab File: VY012015.D
Acq: 27 Dec 2022 14:12




Instrument :
MSVOA_Y
ClientSampleId :


Tgt Ion:105 Resp: 116
Ion Ratio Lower Upper
105 100
120 0.0 22.9 68.7#

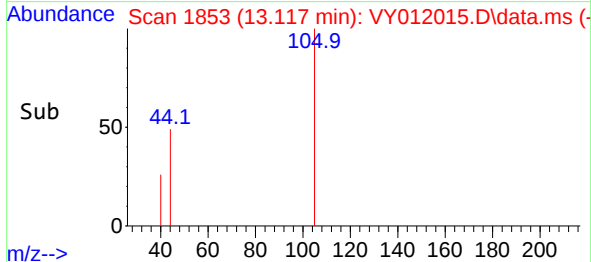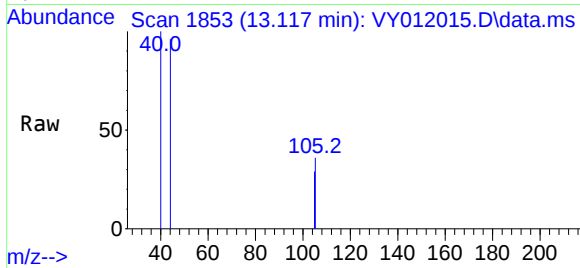

#85
sec-Butylbenzene
Concen: 3.389 ug/l
RT: 13.251 min Scan# 1875
Delta R.T. -0.000 min
Lab File: VY012015.D
Acq: 27 Dec 2022 14:12

Tgt Ion:105 Resp: 270
Ion Ratio Lower Upper
105 100
134 11.1 10.1 30.3


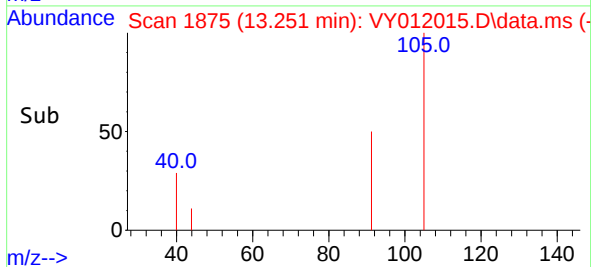

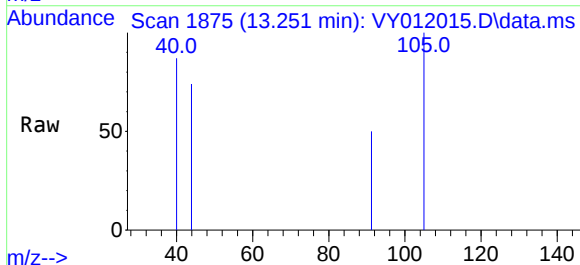




#86
p-Isopropyltoluene
Concen: 1.502 ug/l
RT: 13.379 min Scan# 1896
Delta R.T. 0.012 min
Lab File: VY012015.D
Acq: 27 Dec 2022 14:12




Instrument :
MSVOA_Y
ClientSampleId :


Tgt Ion:119 Resp: 101
Ion Ratio Lower Upper
119 100
134 0.0 13.0 39.0#
91 0.0 11.9 35.9#



#87
1,3-Dichlorobenzene
Concen: 6.079 ug/l
RT: 13.373 min Scan# 1895
Delta R.T. 0.006 min
Lab File: VY012015.D
Acq: 27 Dec 2022 14:12


Tgt Ion:146 Resp: 208
Ion Ratio Lower Upper
146 100
111 23.6 19.7 59.0
148 60.1 32.0 96.0

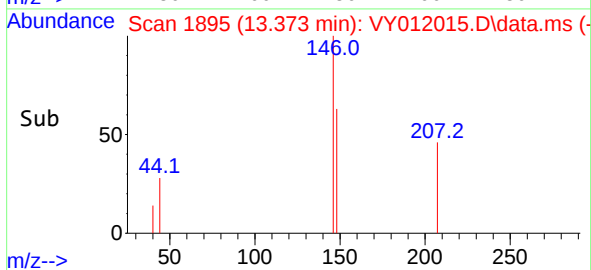






#88
1,4-Dichlorobenzene
Concen: 6.115 ug/l
RT: 13.373 min Scan# 11
Delta R.T. -0.073 min
Lab File: VY012015.D
Acq: 27 Dec 2022 14:12


Instrument :
MSVOA_Y
ClientSampleId :

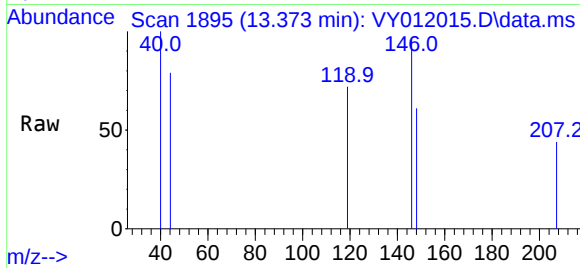



Tgt Ion:146 Resp: 208
Ion Ratio Lower Upper
146 100
111 23.6 19.6 58.7
148 60.1 31.9 95.7

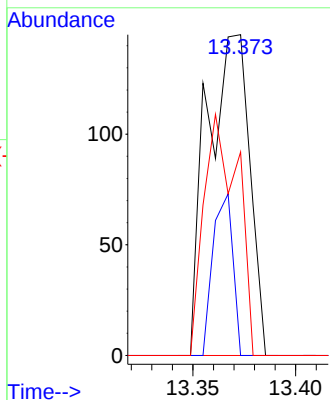


#89
n-Butylbenzene
Concen: 1.577 ug/l
RT: 13.696 min Scan# 1948
Delta R.T. -0.000 min
Lab File: VY012015.D
Acq: 27 Dec 2022 14:12

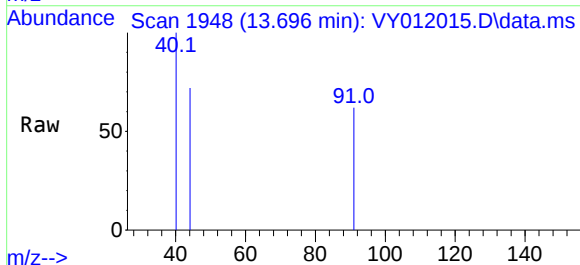


Tgt Ion: 91 Resp: 96
Ion Ratio Lower Upper
91 100
92 0.0 26.8 80.4#
134 0.0 13.3 39.8#

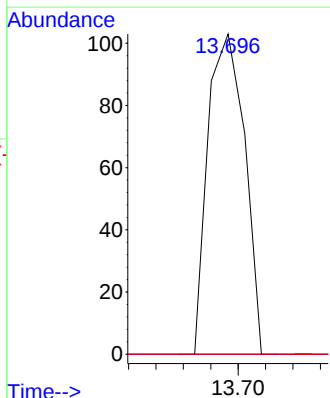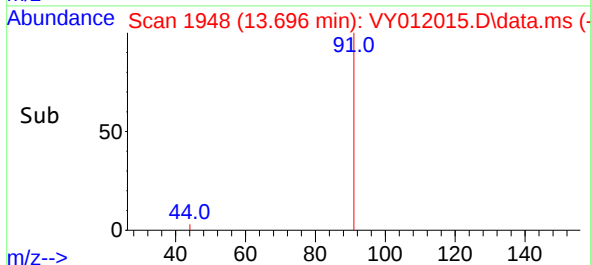






#91
1,2-Dichlorobenzene
Concen: 5.934 ug/l
RT: 13.739 min Scan# 1955
Delta R.T. -0.000 min
Lab File: VY012015.D
Acq: 27 Dec 2022 14:12


Instrument :
MSVOA_Y
ClientSampleId :





Tgt Ion:146 Resp: 177
Ion Ratio Lower Upper
146 100
111 26.6 20.3 60.8
148 21.5 31.8 95.4#

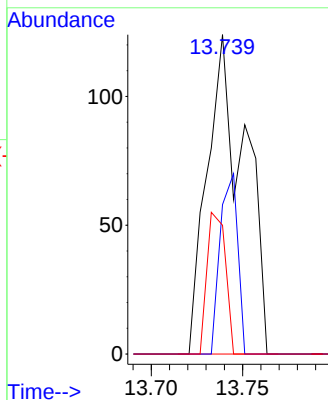


#95
Naphthalene
Concen: 8.212 ug/l
RT: 15.239 min Scan# 2201
Delta R.T. -0.000 min
Lab File: VY012015.D
Acq: 27 Dec 2022 14:12




Tgt Ion:128 Resp: 210
Ion Ratio Lower Upper
128 100
127 0.0 10.2 15.2#
129 0.0 8.8 13.2#

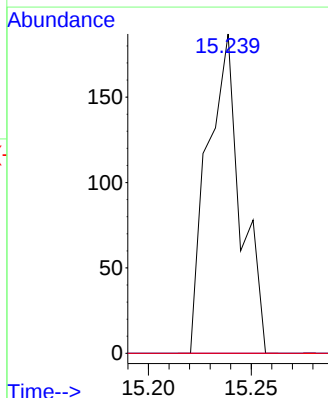



#96
 1,2,3-Trichlorobenzene
 Concen: 1.348 ug/l
 RT: 15.416 min Scan# 21
 Delta R.T. -0.006 min
 Lab File: VY012015.D
 Acq: 27 Dec 2022 14:12

Instrument :
 MSVOA_Y
 ClientSampleId :



Tgt Ion:180 Resp: 20
 Ion Ratio Lower Upper
 180 100
 182 0.0 47.9 143.7#
 145 0.0 16.1 48.2#

