
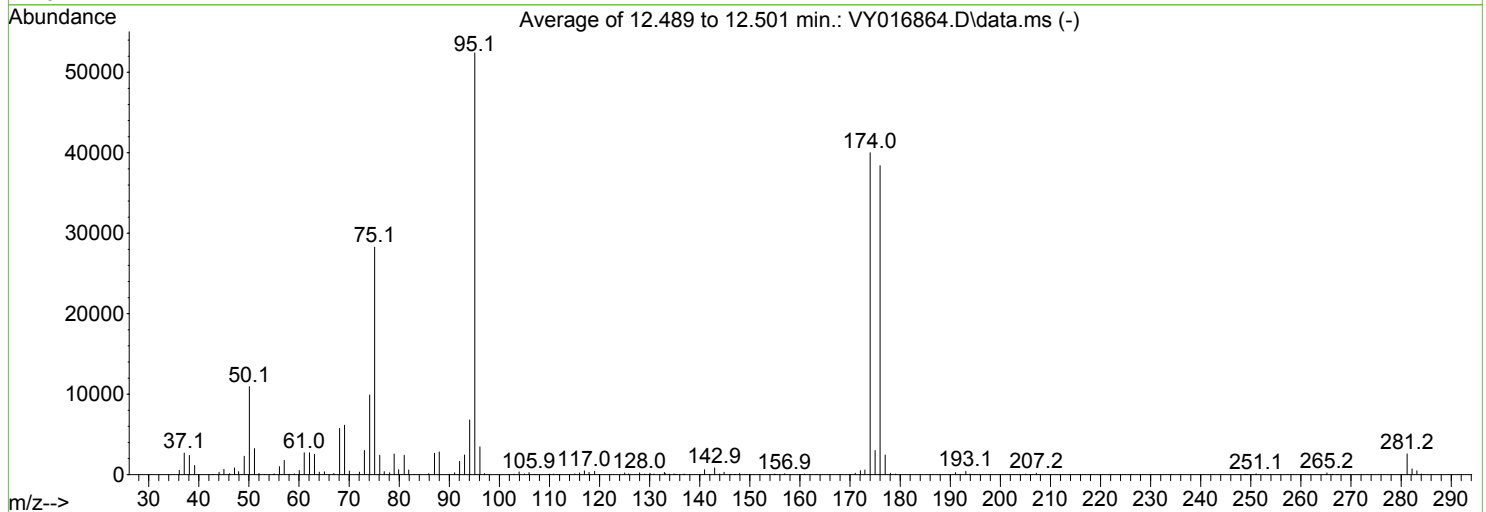


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY122723\
Data File : VY016864.D
Acq On : 27 Dec 2023 08:38
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y122023S.M
Title : SW846 8260
Last Update : Thu Dec 21 01:49:45 2023

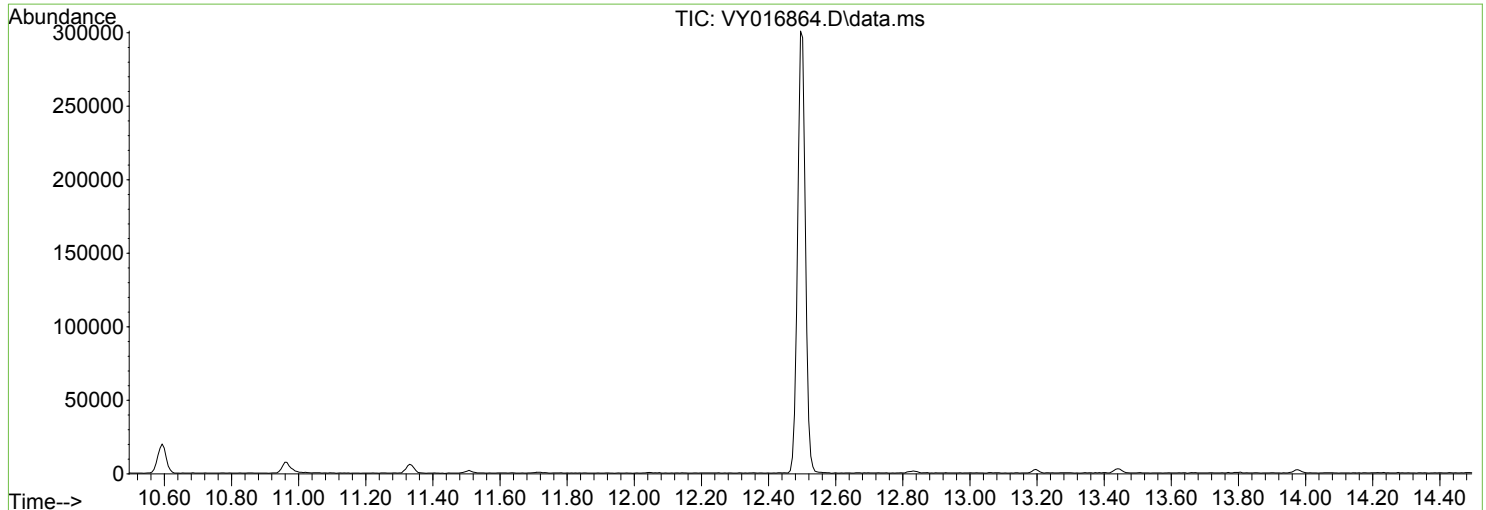

AutoFind: Scans 1750, 1751, 1752; Background Corrected with Scan 1743

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.9	10933	PASS
75	95	30	60	53.9	28272	PASS
95	95	100	100	100.0	52419	PASS
96	95	5	9	6.6	3463	PASS
173	174	0.00	2	1.5	581	PASS
174	95	50	100	76.3	40016	PASS
175	174	5	9	7.5	2998	PASS
176	174	95	101	96.0	38405	PASS
177	176	5	9	6.4	2452	PASS