


Data Path : Z:\voasrv\HPCHEM1\MSVOA Y\Data\vv123019\
Data File : VY001116.D
Acq On : 30 Dec 2019 09:23
Operator : SY/MD
Sample : BFB
Misc : 5.00G/5ML/MSVOA Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y122319S.M
Title : SW846 8260
Last Update : Mon Dec 23 12:07:44 2019

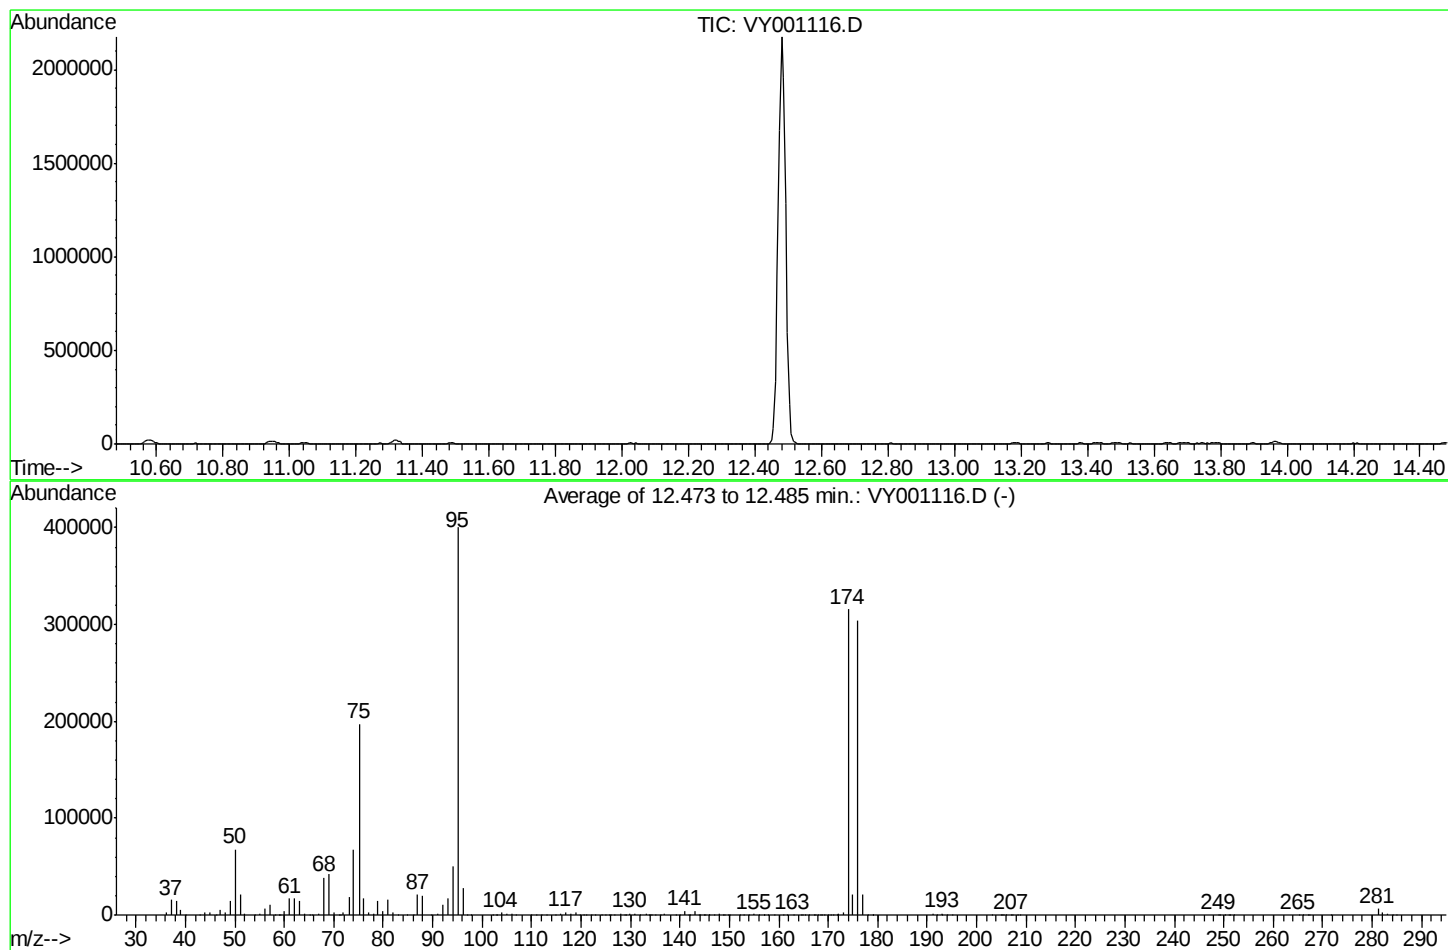

AutoFind: Scans 1761, 1762, 1763; Background Corrected with Scan 1752

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.8	67432	PASS
75	95	30	60	49.2	197077	PASS
95	95	100	100	100.0	400298	PASS
96	95	5	9	6.8	27224	PASS
173	174	0.00	2	0.7	2251	PASS
174	95	50	100	78.9	315669	PASS
175	174	5	9	6.9	21778	PASS
176	174	95	101	96.3	304064	PASS
177	176	5	9	6.9	20973	PASS