


Data Path : Z:\voasrv\HPCHEM1\MSVOA Y\Data\VY011320\
 Data File : VY001167.D
 Acq On : 13 Jan 2020 08:52
 Operator : SY/MD
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y011020S.M
 Title : SW846 8260
 Last Update : Fri Jan 10 16:01:58 2020

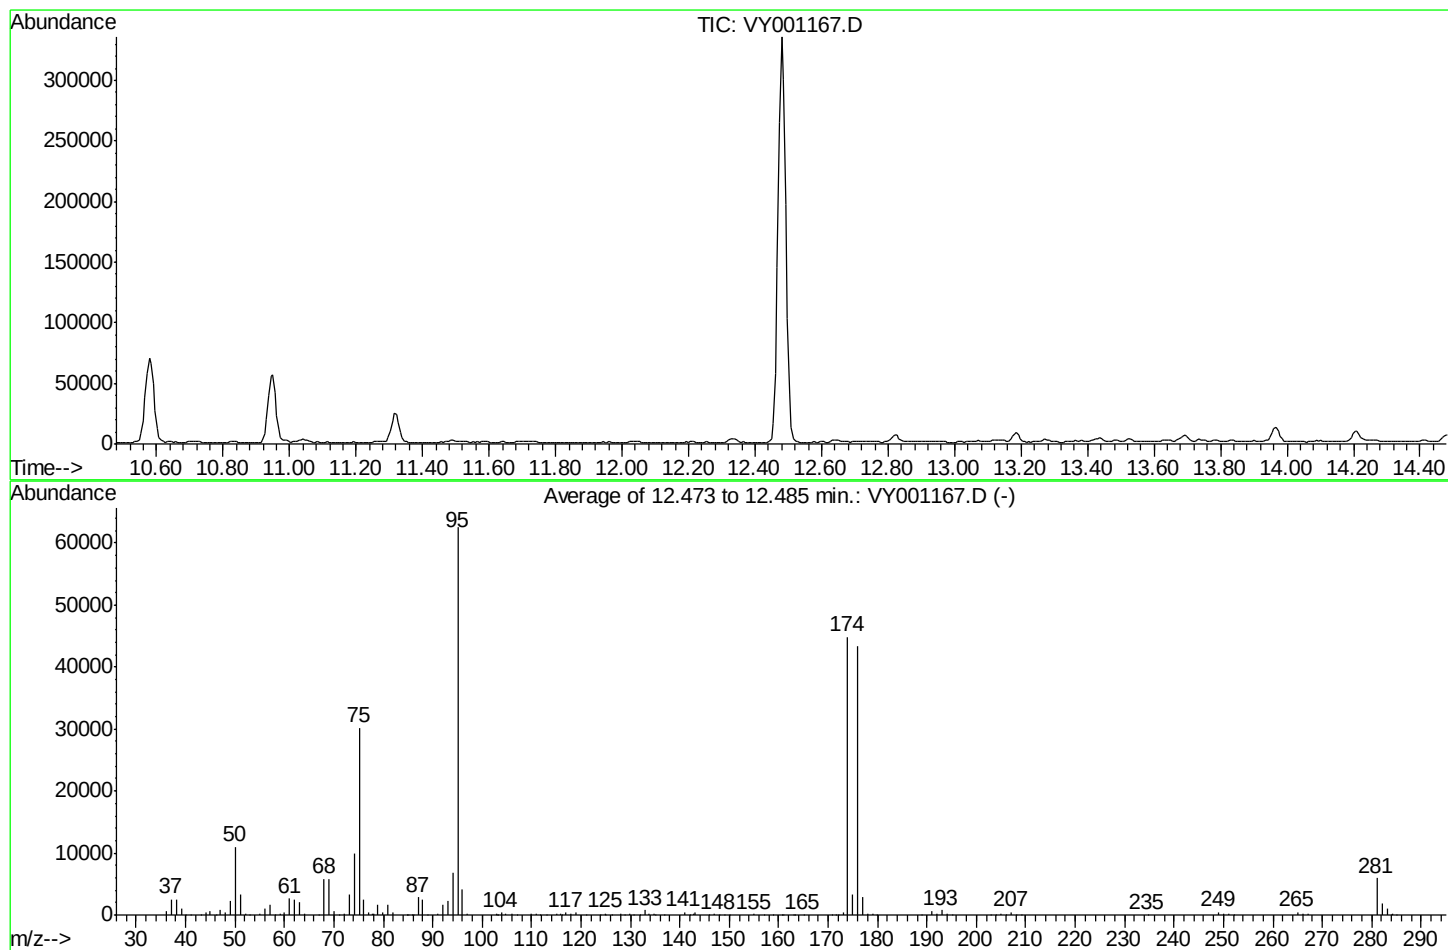

AutoFind: Scans 1761, 1762, 1763; Background Corrected with Scan 1753

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	10962	PASS
75	95	30	60	48.2	30160	PASS
95	95	100	100	100.0	62541	PASS
96	95	5	9	6.6	4122	PASS
173	174	0.00	2	0.9	402	PASS
174	95	50	100	71.7	44837	PASS
175	174	5	9	7.4	3314	PASS
176	174	95	101	96.7	43354	PASS
177	176	5	9	6.7	2891	PASS