
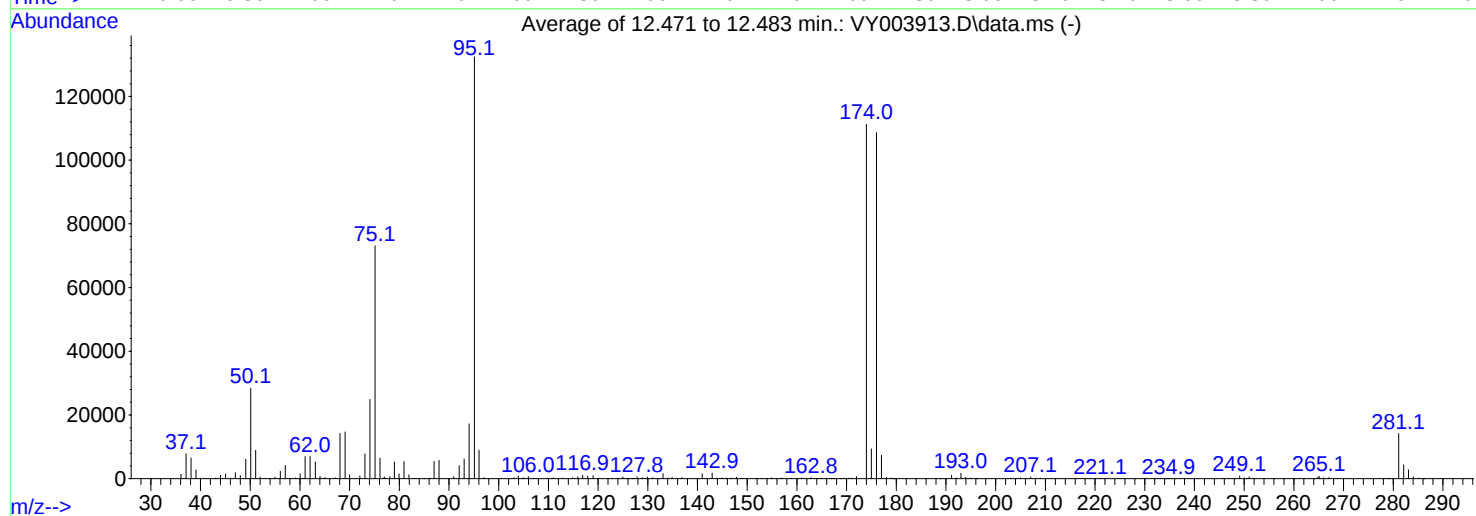


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY011421\
 Data File : VY003913.D
 Acq On : 14 Jan 2021 10:23
 Operator : SY/MD
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA_Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y0112215.M
 Title : SW846 8260
 Last Update : Tue Jan 12 11:47:10 2021

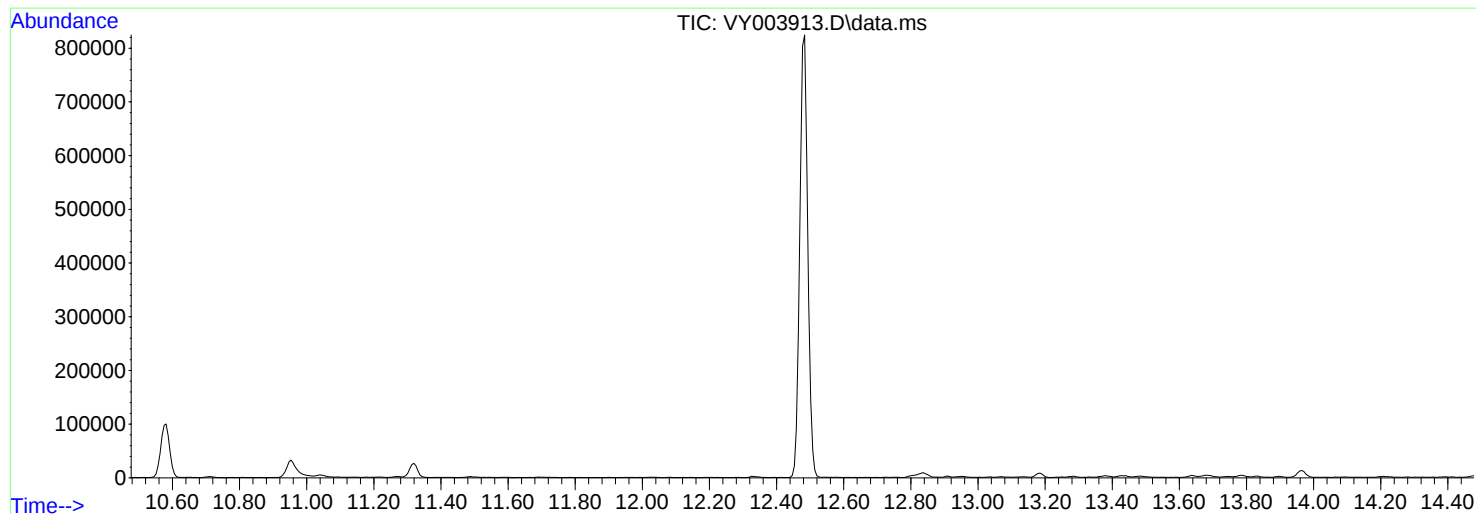

AutoFind: Scans 1747, 1748, 1749; Background Corrected with Scan 1739

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.4	28355	PASS
75	95	30	60	55.2	73124	PASS
95	95	100	100	100.0	132429	PASS
96	95	5	9	6.7	8924	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	84.0	111227	PASS
175	174	5	9	8.4	9355	PASS
176	174	95	101	97.7	108643	PASS
177	176	5	9	6.8	7336	PASS