

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY011723\
 Data File : VY012226.D
 Acq On : 17 Jan 2023 16:26
 Operator : KP/MD
 Sample : 01170-01
 Misc : 5.07g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 CL-2-011623

Quant Time: Jan 18 00:33:26 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y011623S.M
 Quant Title : SW846 8260
 QLast Update : Tue Jan 17 04:31:47 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.789	168	260891	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.691	114	445828	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.489	117	428427	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	197899	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.142	65	148440	70.234	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	140.460%
35) Dibromofluoromethane	7.716	113	138736	58.770	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	117.540%
50) Toluene-d8	10.179	98	526879	65.784	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	131.560%
62) 4-Bromofluorobenzene	12.483	95	186032	55.902	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	111.800%


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY011723\
Data File : VY012226.D
Acq On : 17 Jan 2023 16:26
Operator : KP/MD
Sample : 01170-01
Misc : 5.07g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
CL-2-011623

Quant Time: Jan 18 00:33:26 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y011623S.M
Quant Title : SW846 8260
QLast Update : Tue Jan 17 04:31:47 2023
Response via : Initial Calibration




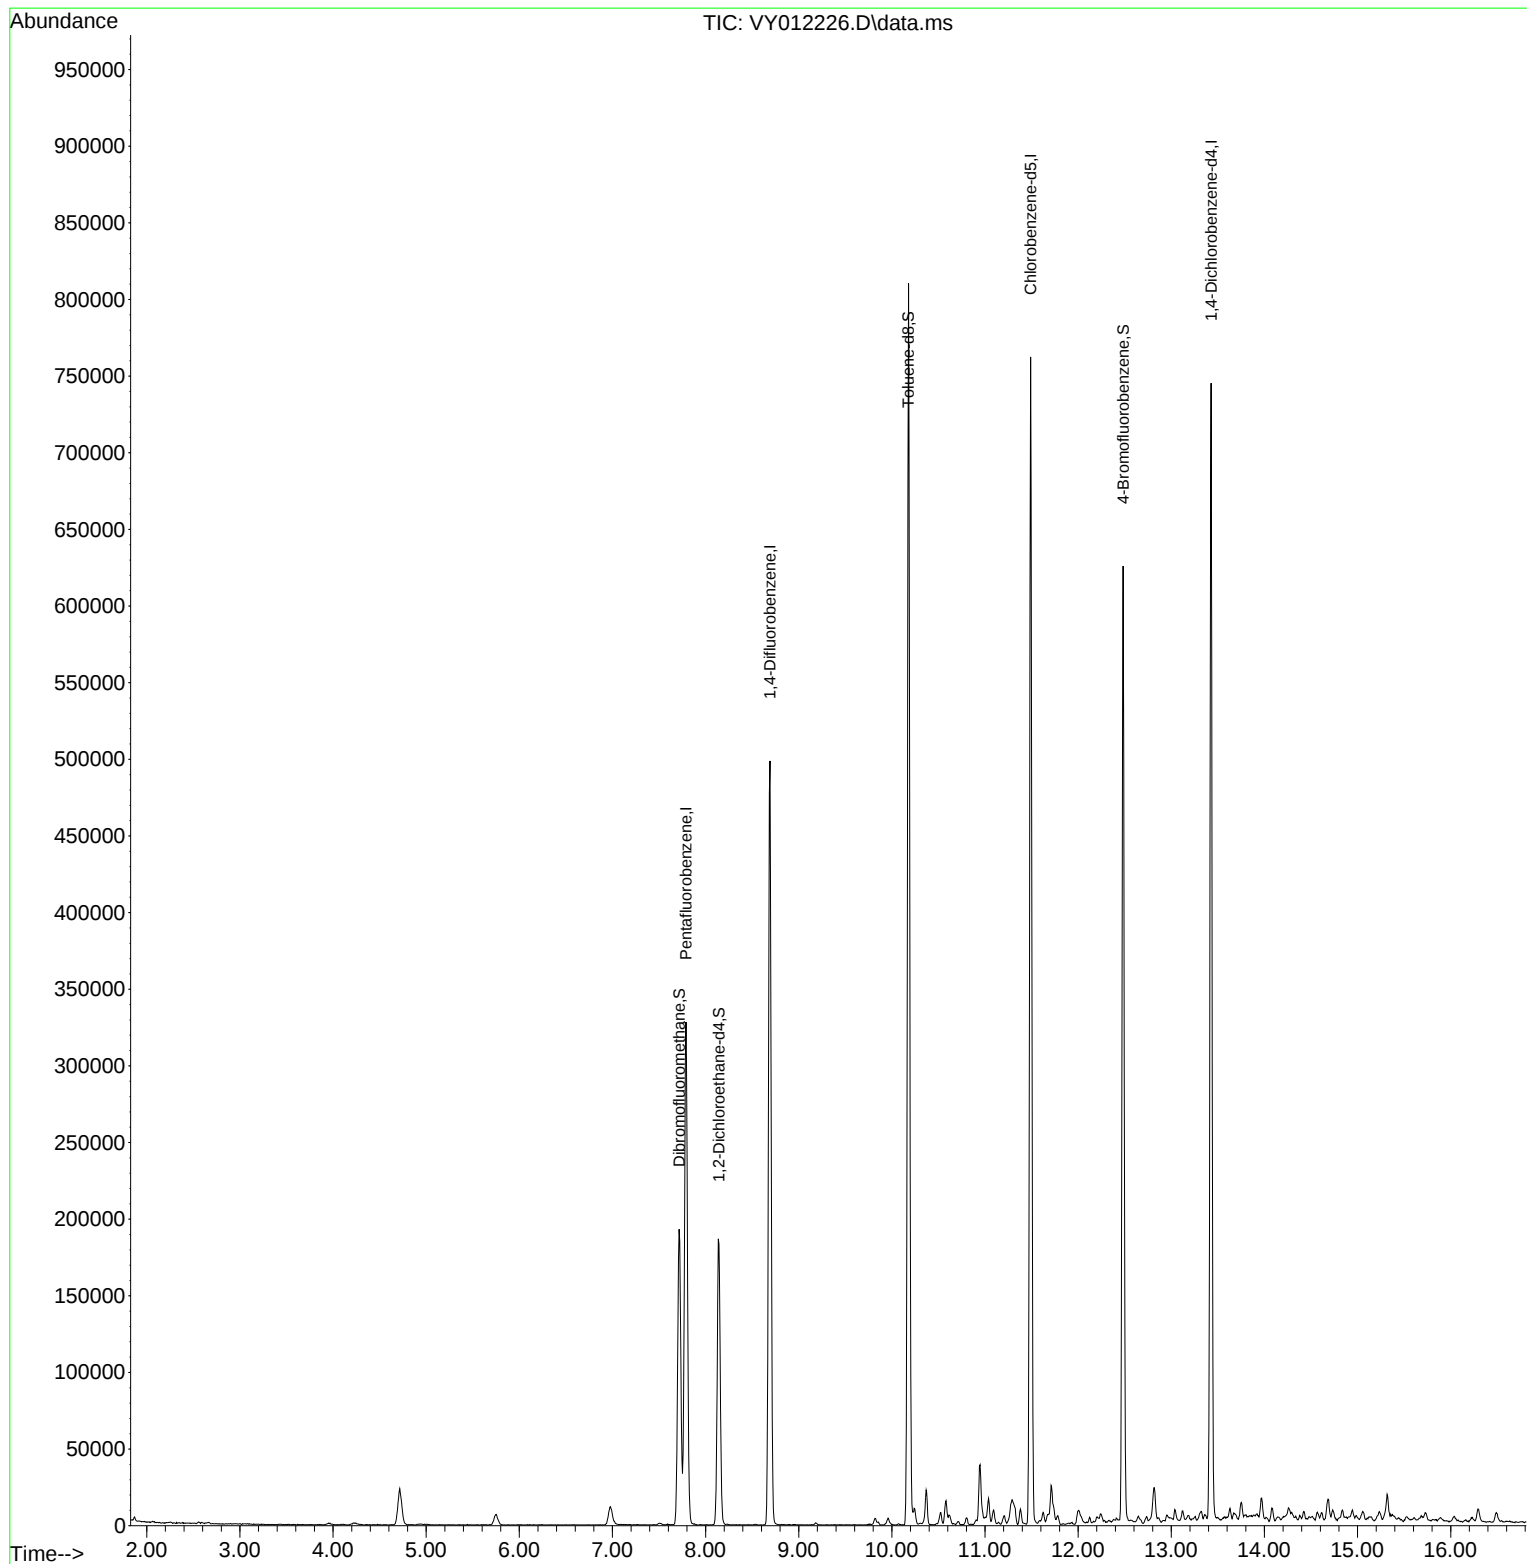




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY012226.D
Acq: 17 Jan 2023 16:26




Instrument :
MSVOA_Y
ClientSampleId :
CL-2-011623


Tgt Ion:168 Resp: 260891
Ion Ratio Lower Upper
168 100
99 53.7 44.0 66.0

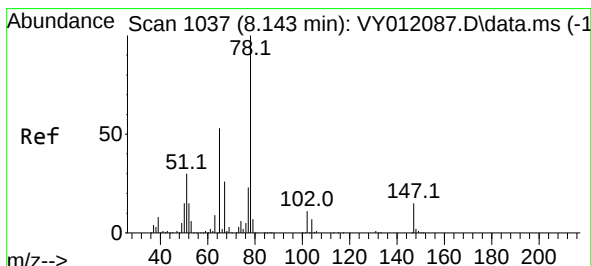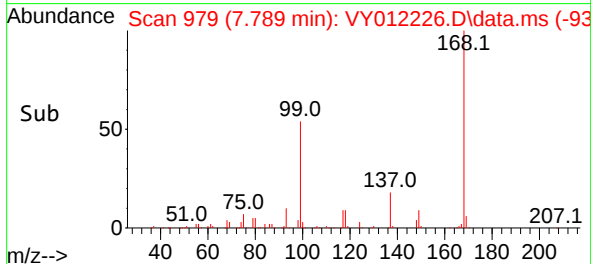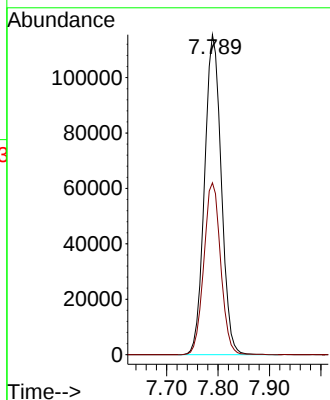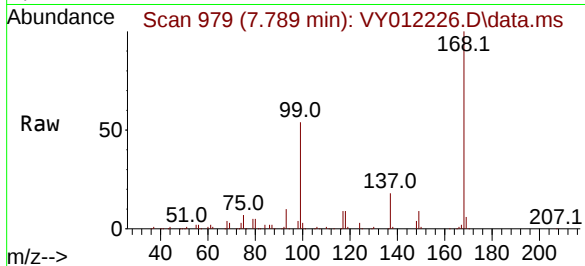

#33
1,2-Dichloroethane-d4
Concen: 70.234 ug/l
RT: 8.142 min Scan# 1037
Delta R.T. -0.001 min
Lab File: VY012226.D
Acq: 17 Jan 2023 16:26

Tgt Ion: 65 Resp: 148440
Ion Ratio Lower Upper
65 100
67 52.6 0.0 103.2

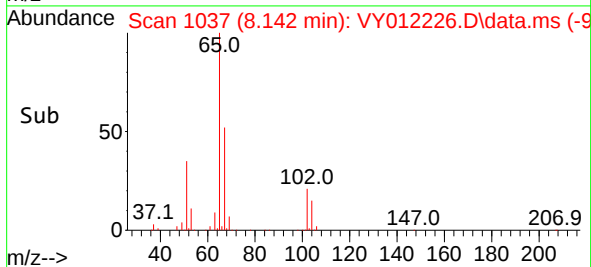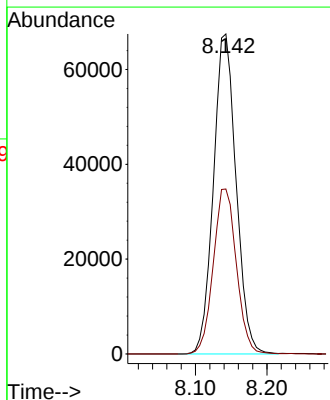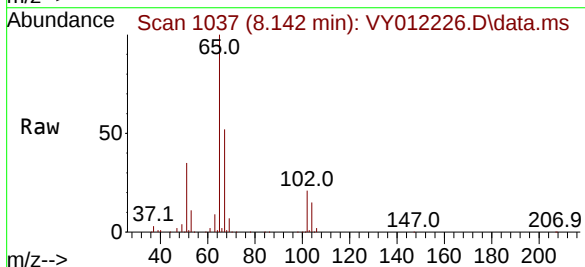

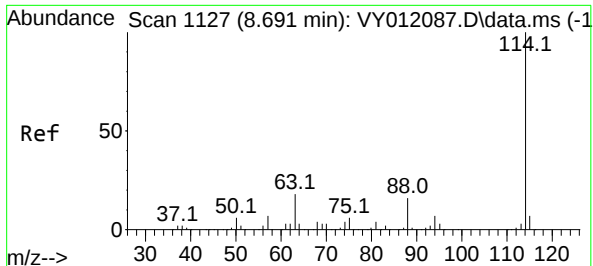

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.691 min Scan# 1127

Delta R.T. 0.000 min

Lab File: VY012226.D

Acq: 17 Jan 2023 16:26

Instrument :

MSVOA_Y

ClientSampleId :

CL-2-011623





Tgt Ion:114 Resp: 445828

Ion Ratio Lower Upper

114 100

63 18.4 0.0 39.6

88 15.3 0.0 32.2

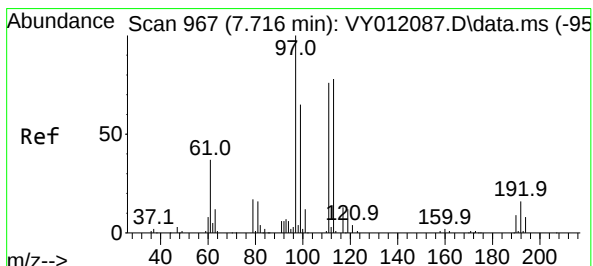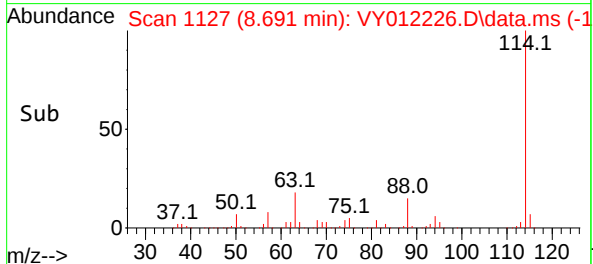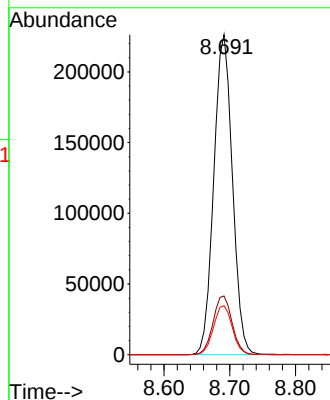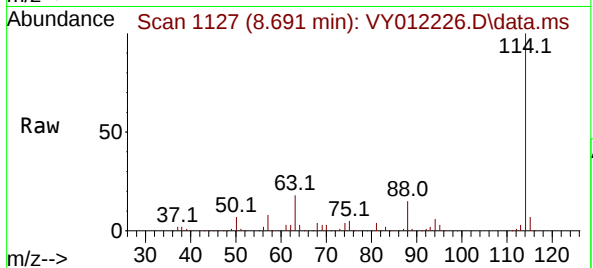

#35

Dibromofluoromethane

Concen: 58.770 ug/l

RT: 7.716 min Scan# 967

Delta R.T. -0.000 min

Lab File: VY012226.D

Acq: 17 Jan 2023 16:26




Tgt Ion:113 Resp: 138736


Ion Ratio Lower Upper

113 100

111 102.2 83.0 124.4

192 20.9 16.0 24.0

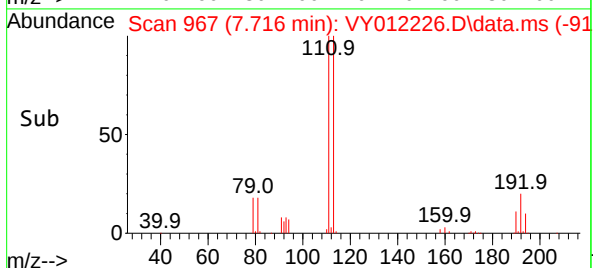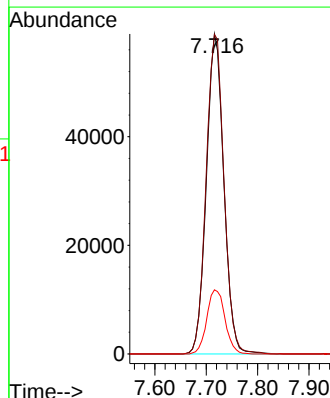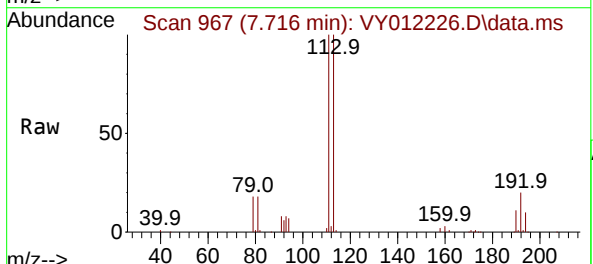

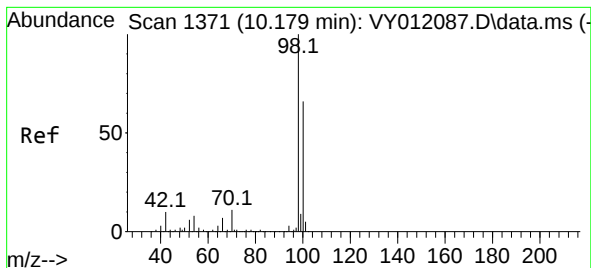

#50

Toluene-d8

Concen: 65.784 ug/l

RT: 10.179 min Scan# 1371

Delta R.T. -0.000 min

Lab File: VY012226.D

Acq: 17 Jan 2023 16:26

Instrument :

MSVOA_Y

ClientSampleId :





CL-2-011623

Tgt Ion: 98 Resp: 526879

Ion Ratio Lower Upper

98 100

100 65.0 51.9 77.9

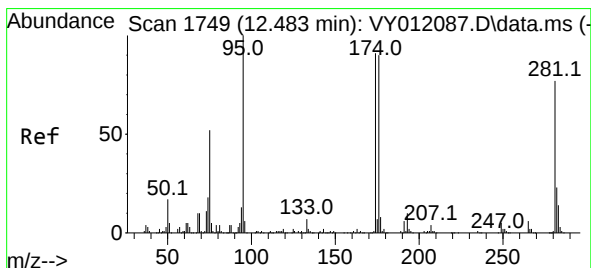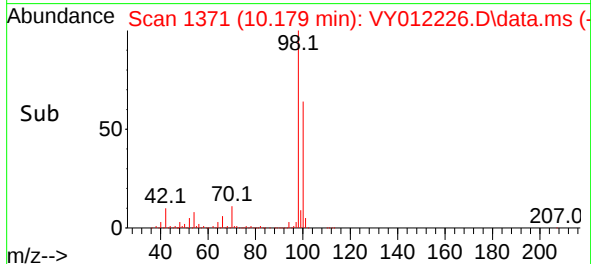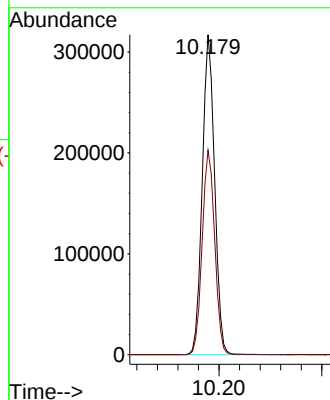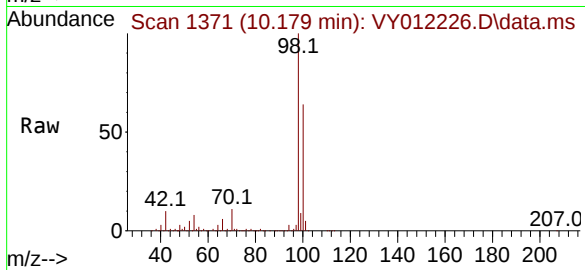

#62

4-Bromofluorobenzene

Concen: 55.902 ug/l

RT: 12.483 min Scan# 1749

Delta R.T. 0.000 min

Lab File: VY012226.D

Acq: 17 Jan 2023 16:26




Tgt Ion: 95 Resp: 186032


Ion Ratio Lower Upper

95 100

174 87.8 0.0 172.0

176 84.7 0.0 167.6

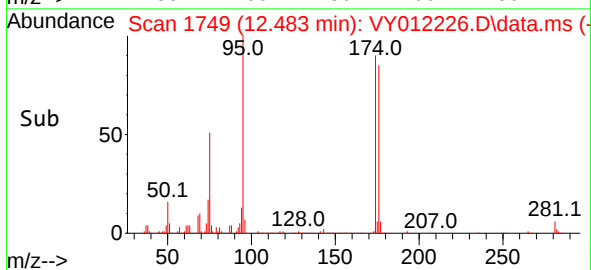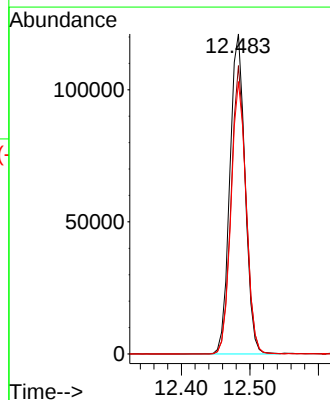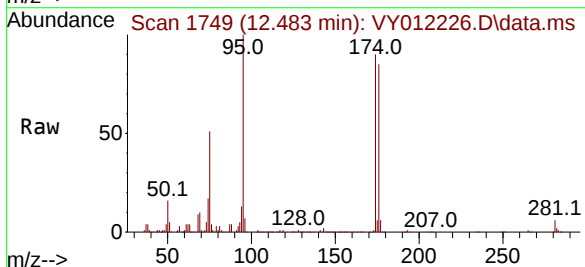

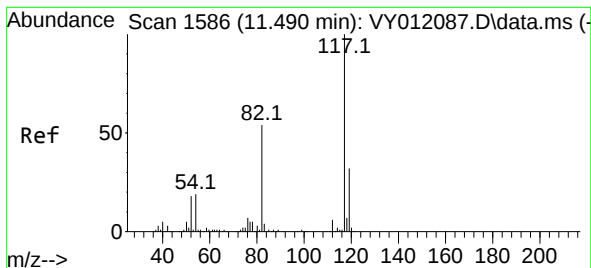

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.489 min Scan# 11

Delta R.T. -0.001 min

Lab File: VY012226.D

Acq: 17 Jan 2023 16:26

Instrument :

MSVOA_Y

ClientSampleId :

CL-2-011623





Tgt Ion:117 Resp: 428427

Ion Ratio Lower Upper

117 100

82 54.8 44.8 67.2

119 32.8 25.4 38.2

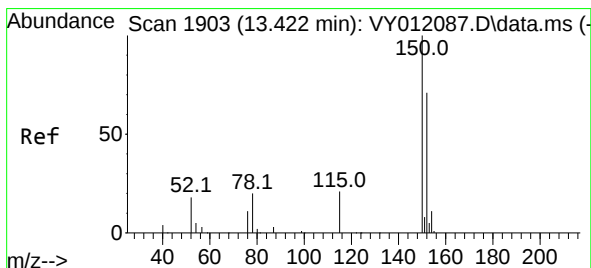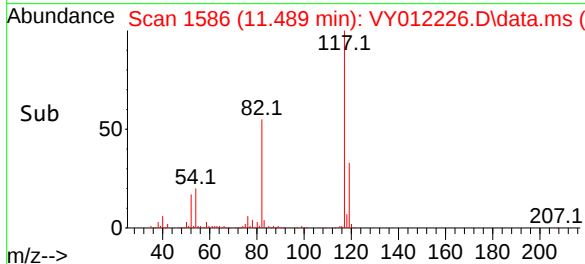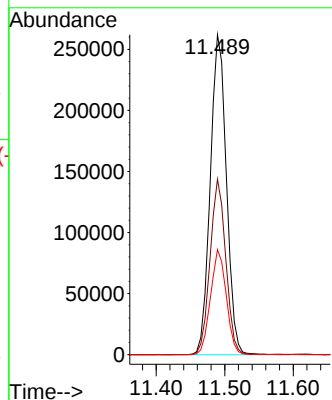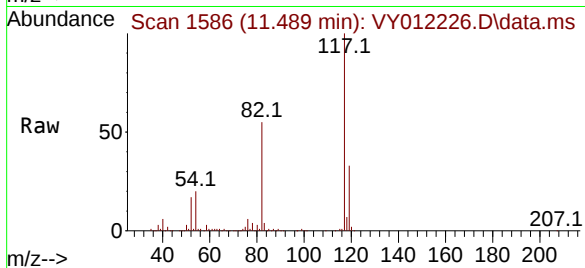

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.428 min Scan# 1904

Delta R.T. 0.006 min

Lab File: VY012226.D

Acq: 17 Jan 2023 16:26

Tgt Ion:152 Resp: 197899

Ion Ratio Lower Upper

152 100

115 57.8 29.1 87.3

150 156.0 0.0 342.6

