

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY011723\
 Data File : VY012228.D
 Acq On : 17 Jan 2023 17:13
 Operator : KP/MD
 Sample : 01180-01
 Misc : 5.30g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 MH-7

Quant Time: Jan 18 00:33:47 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y011623S.M
 Quant Title : SW846 8260
 QLast Update : Tue Jan 17 04:31:47 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.789	168	222990	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.691	114	364178	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.489	117	319865	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	142395	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.136	65	108083	59.199	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	118.400%
35) Dibromofluoromethane	7.716	113	106175	55.061	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	110.120%
50) Toluene-d8	10.179	98	423649	64.680	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	129.360%
62) 4-Bromofluorobenzene	12.483	95	130882	48.148	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	96.300%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY011723\
Data File : VY012228.D
Acq On : 17 Jan 2023 17:13
Operator : KP/MD
Sample : 01180-01
Misc : 5.30g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
MH-7

Quant Time: Jan 18 00:33:47 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y011623S.M
Quant Title : SW846 8260
QLast Update : Tue Jan 17 04:31:47 2023
Response via : Initial Calibration




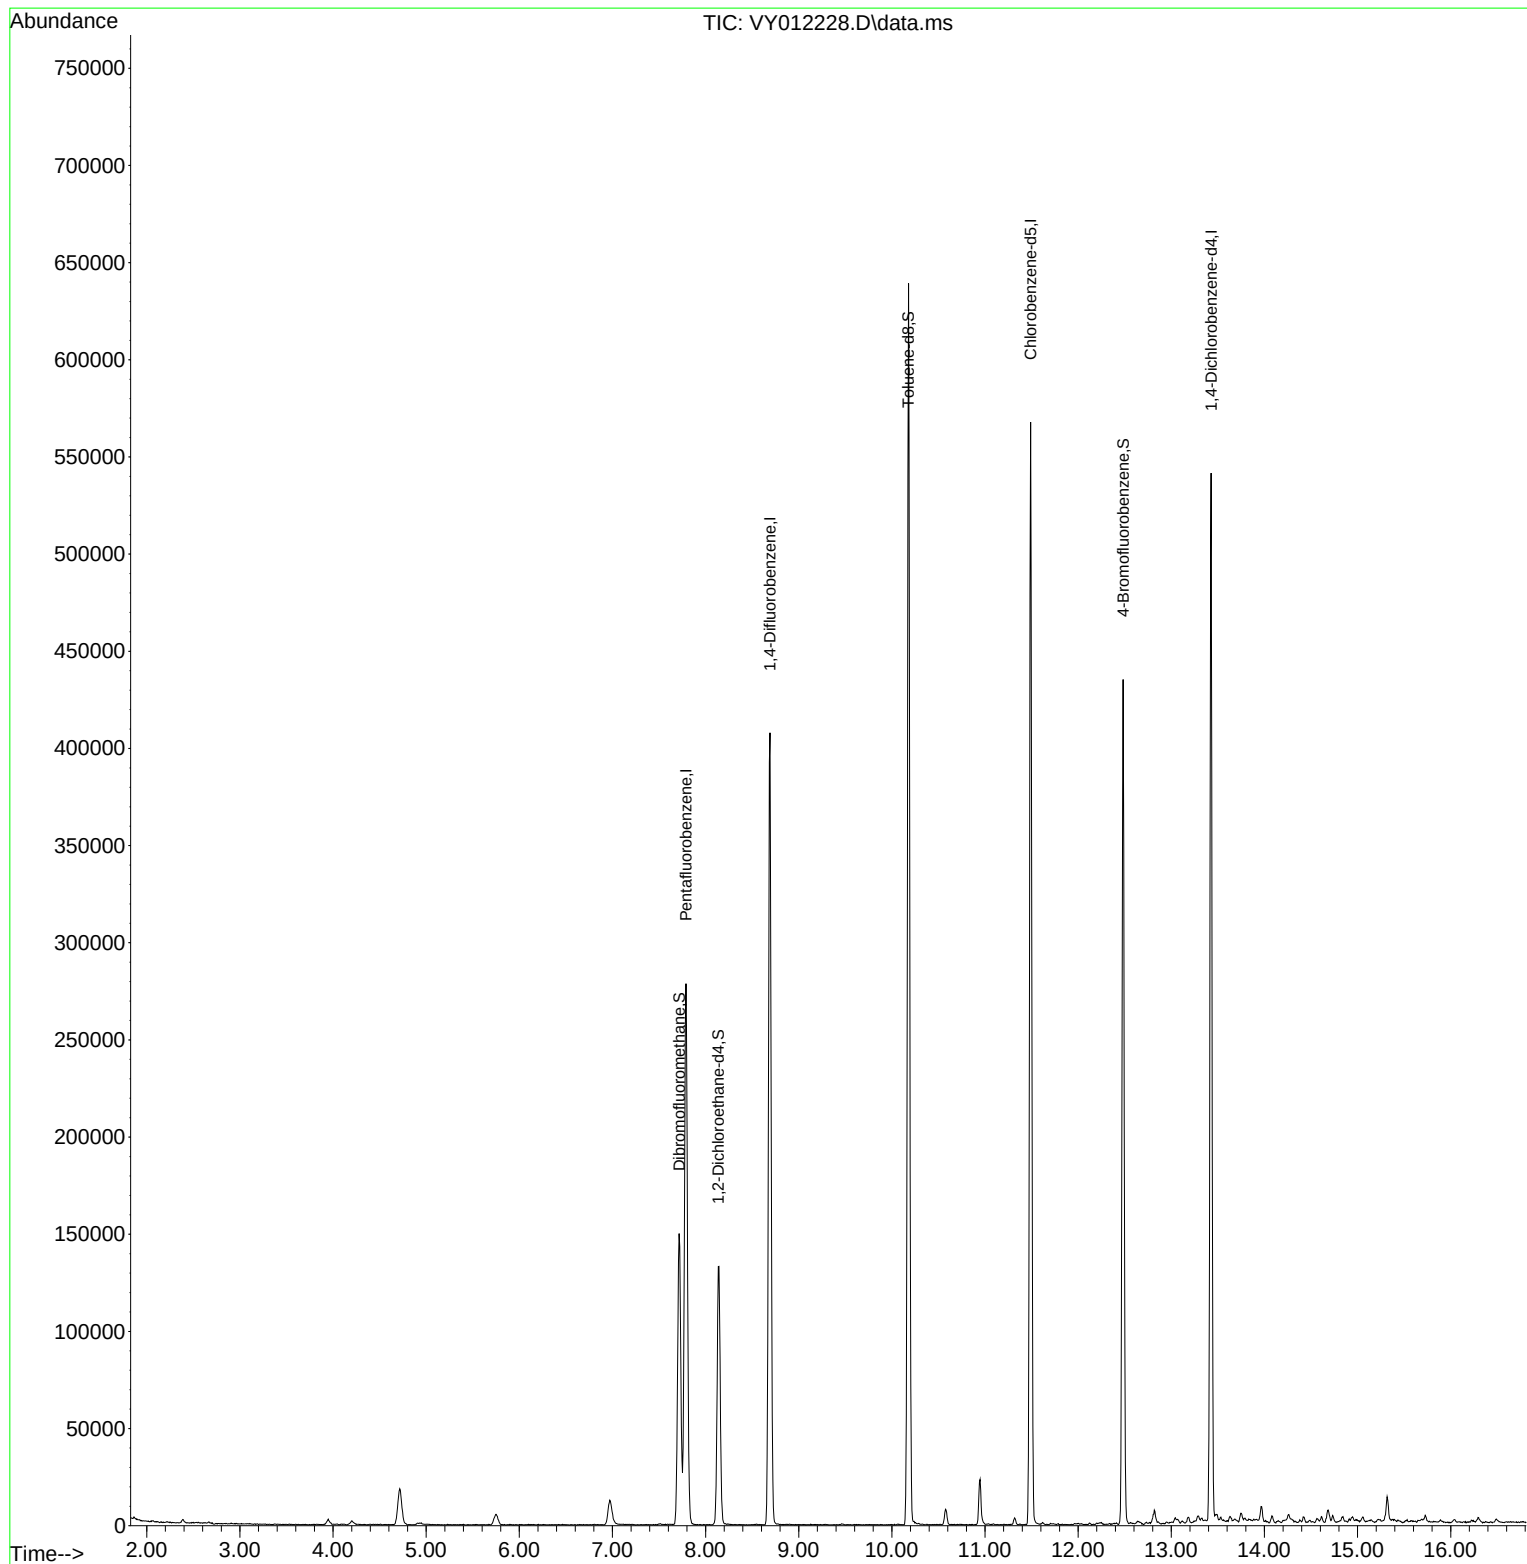


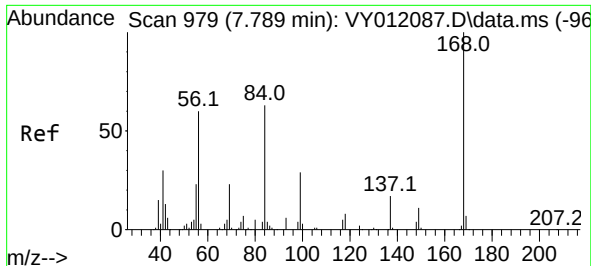

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY012228.D
Acq: 17 Jan 2023 17:13




Instrument :
MSVOA_Y
ClientSampleId :
MH-7


Tgt Ion:168 Resp: 222990
Ion Ratio Lower Upper
168 100
99 53.8 44.0 66.0

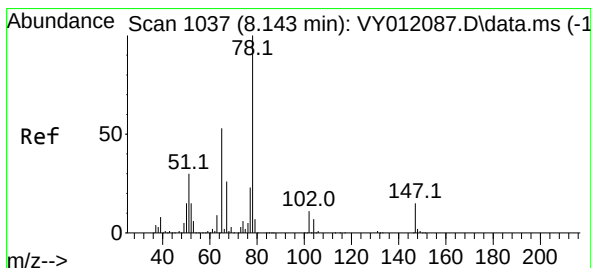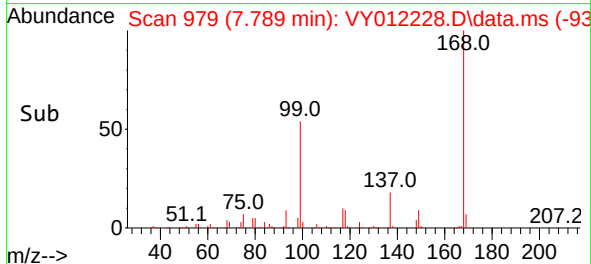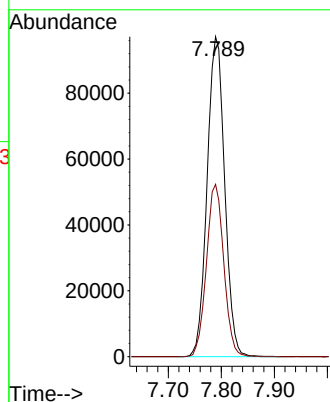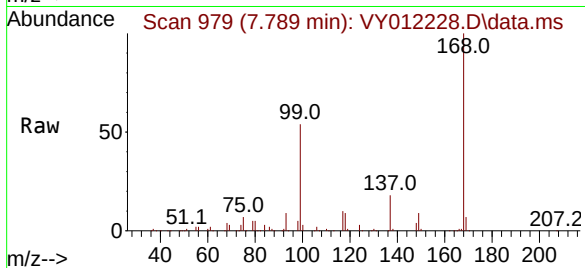

#33
1,2-Dichloroethane-d4
Concen: 59.199 ug/l
RT: 8.136 min Scan# 1036
Delta R.T. -0.007 min
Lab File: VY012228.D
Acq: 17 Jan 2023 17:13

Tgt Ion: 65 Resp: 108083
Ion Ratio Lower Upper
65 100
67 52.4 0.0 103.2

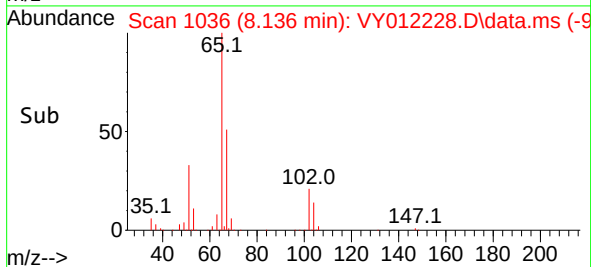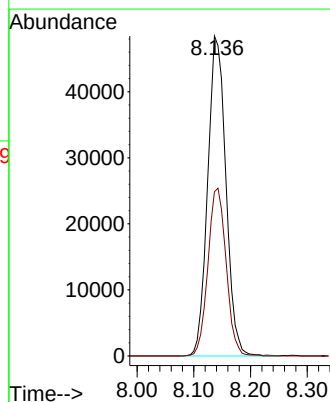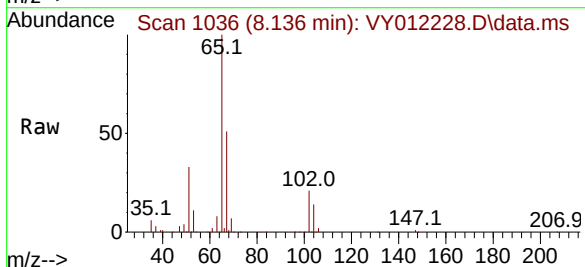

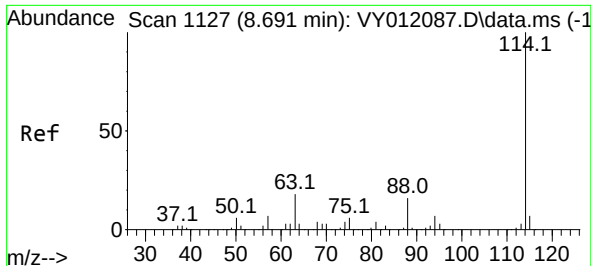

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.691 min Scan# 1127

Delta R.T. 0.000 min

Lab File: VY012228.D

Acq: 17 Jan 2023 17:13

Instrument :

MSVOA_Y

ClientSampleId :

MH-7





Tgt Ion:114 Resp: 364178

Ion Ratio Lower Upper

114 100

63 18.5 0.0 39.6

88 15.3 0.0 32.2

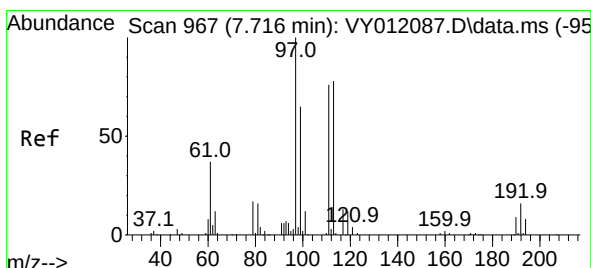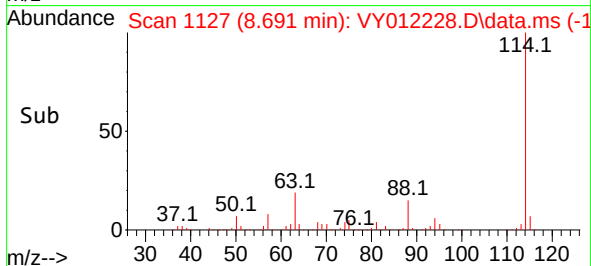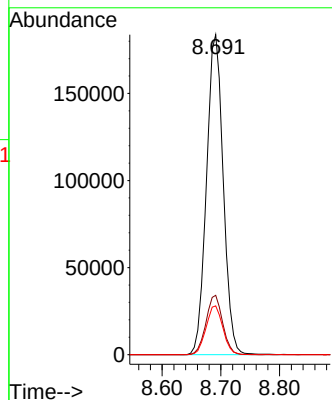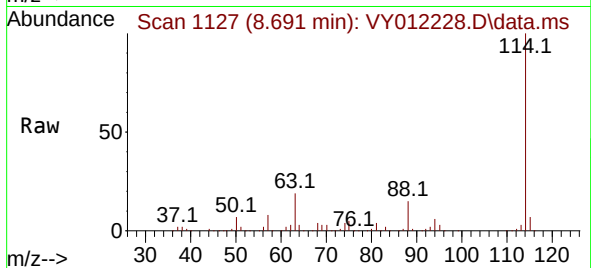

#35

Dibromofluoromethane

Concen: 55.061 ug/l

RT: 7.716 min Scan# 967

Delta R.T. -0.000 min

Lab File: VY012228.D

Acq: 17 Jan 2023 17:13




Tgt Ion:113 Resp: 106175


Ion Ratio Lower Upper

113 100

111 102.2 83.0 124.4

192 21.5 16.0 24.0

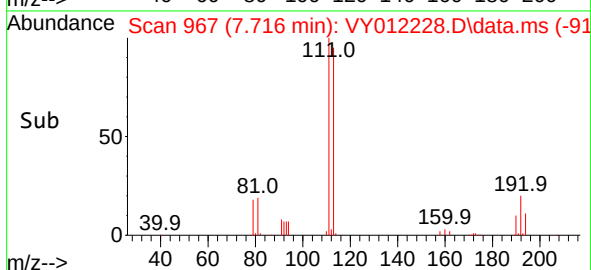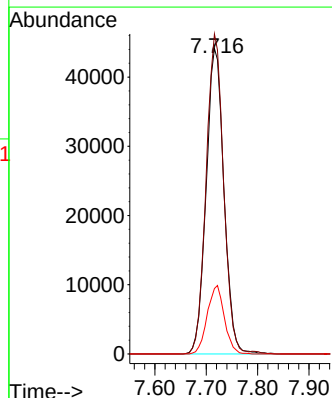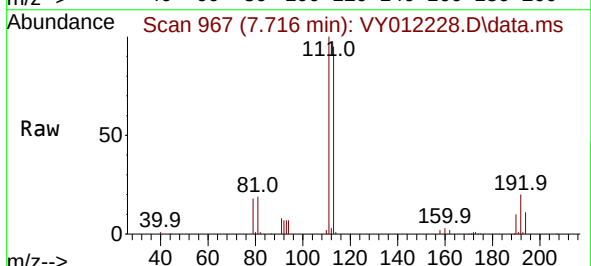

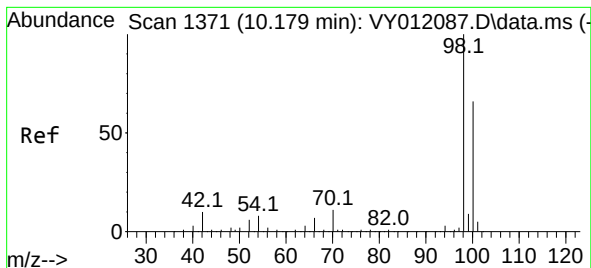

#50

Toluene-d8

Concen: 64.680 ug/l

RT: 10.179 min Scan# 1371

Delta R.T. -0.000 min

Lab File: VY012228.D

Acq: 17 Jan 2023 17:13

Instrument :

MSVOA_Y

ClientSampleId :





MH-7

Tgt Ion: 98 Resp: 423649

Ion Ratio Lower Upper

98 100

100 65.4 51.9 77.9

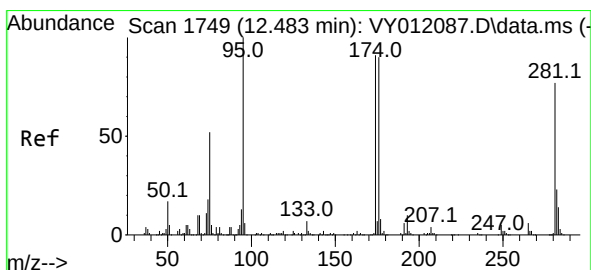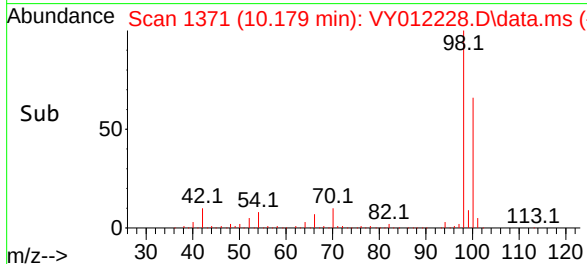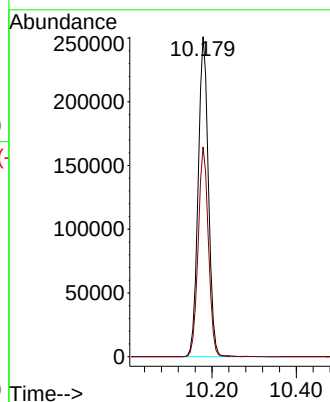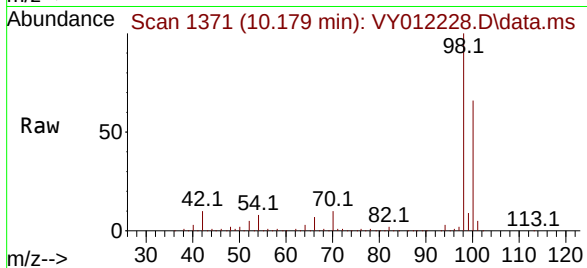

#62

4-Bromofluorobenzene

Concen: 48.148 ug/l

RT: 12.483 min Scan# 1749

Delta R.T. 0.000 min

Lab File: VY012228.D

Acq: 17 Jan 2023 17:13




Tgt Ion: 95 Resp: 130882


Ion Ratio Lower Upper

95 100

174 90.5 0.0 172.0

176 86.5 0.0 167.6


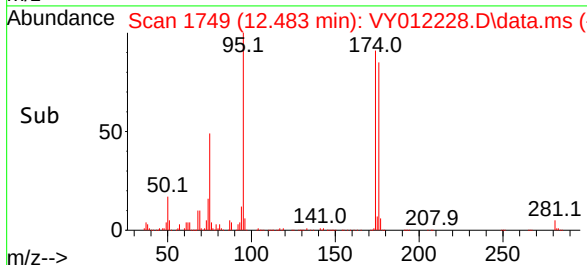
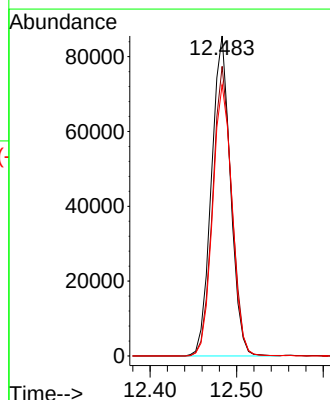
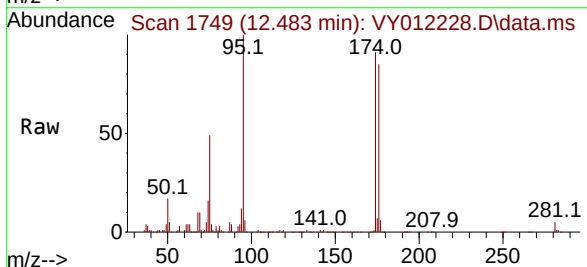


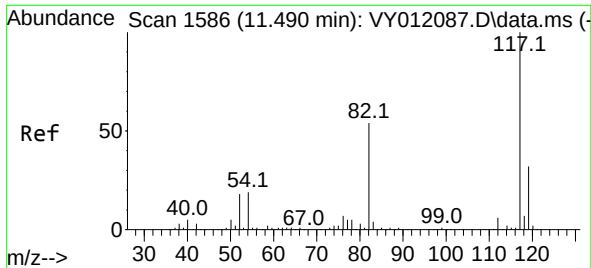

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.489 min Scan# 11
Delta R.T. -0.001 min
Lab File: VY012228.D
Acq: 17 Jan 2023 17:13

Instrument :
MSVOA_Y
ClientSampleId :
MH-7

Tgt Ion:117 Resp: 319865
Ion Ratio Lower Upper
117 100
82 52.4 44.8 67.2
119 31.8 25.4 38.2

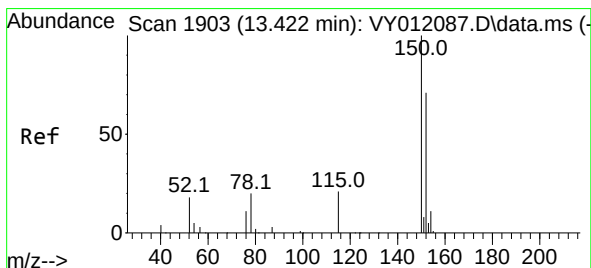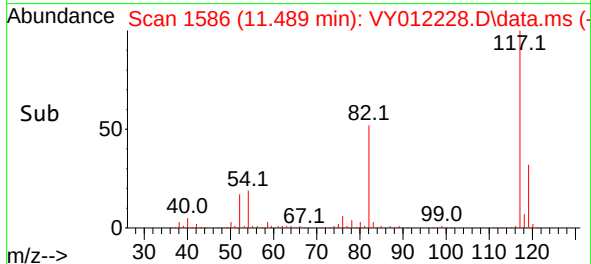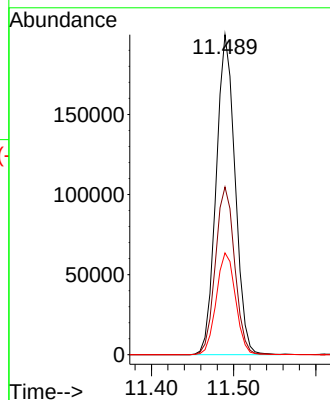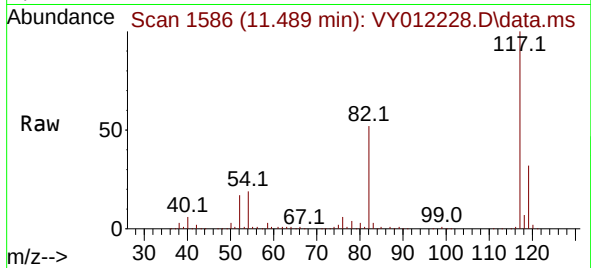

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.428 min Scan# 1904
Delta R.T. 0.006 min
Lab File: VY012228.D
Acq: 17 Jan 2023 17:13

Tgt Ion:152 Resp: 142395
Ion Ratio Lower Upper
152 100
115 57.3 29.1 87.3
150 158.7 0.0 342.6

