
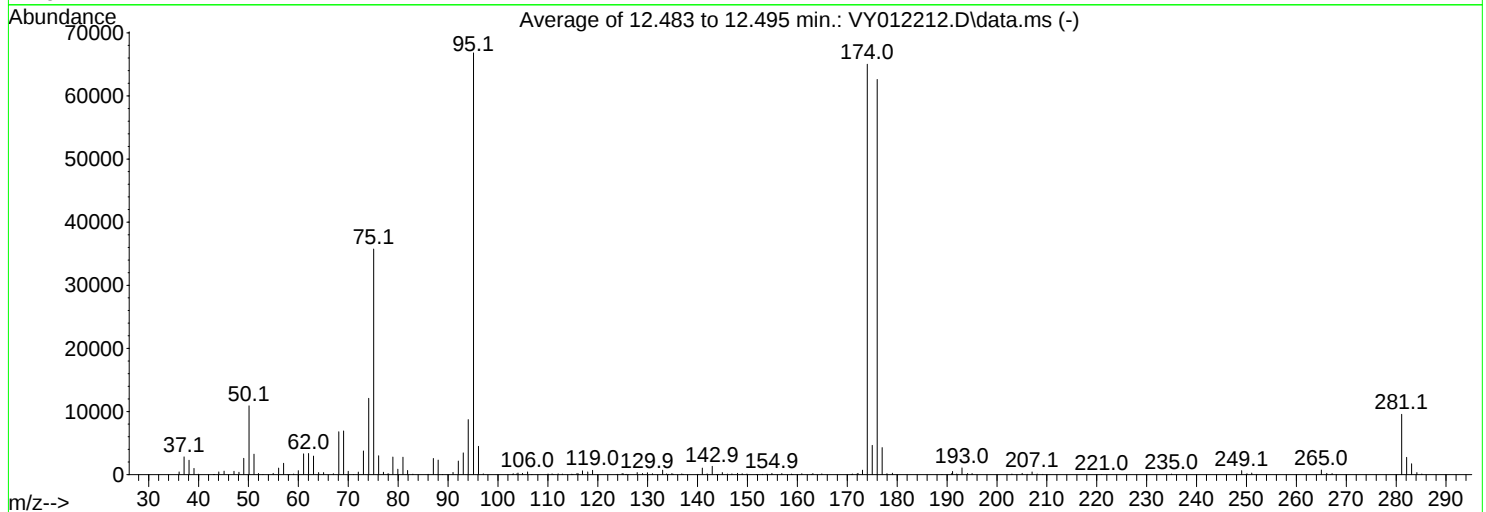


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY011723\
Data File : VY012212.D
Acq On : 17 Jan 2023 09:34
Operator : KP/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y011623S.M
Title : SW846 8260
Last Update : Tue Jan 17 04:31:47 2023

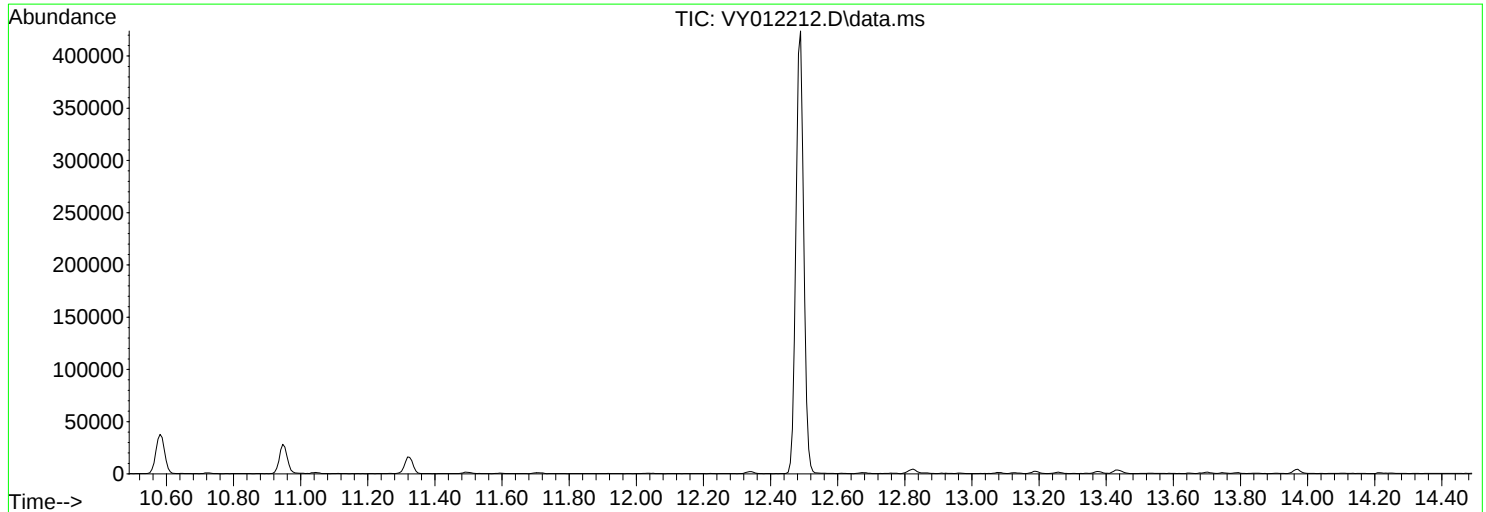

AutoFind: Scans 1749, 1750, 1751; Background Corrected with Scan 1740

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.3	10890	PASS
75	95	30	60	53.5	35733	PASS
95	95	100	100	100.0	66824	PASS
96	95	5	9	6.7	4483	PASS
173	174	0.00	2	1.1	716	PASS
174	95	50	100	97.3	65008	PASS
175	174	5	9	7.2	4653	PASS
176	174	95	101	96.3	62608	PASS
177	176	5	9	6.9	4291	PASS