
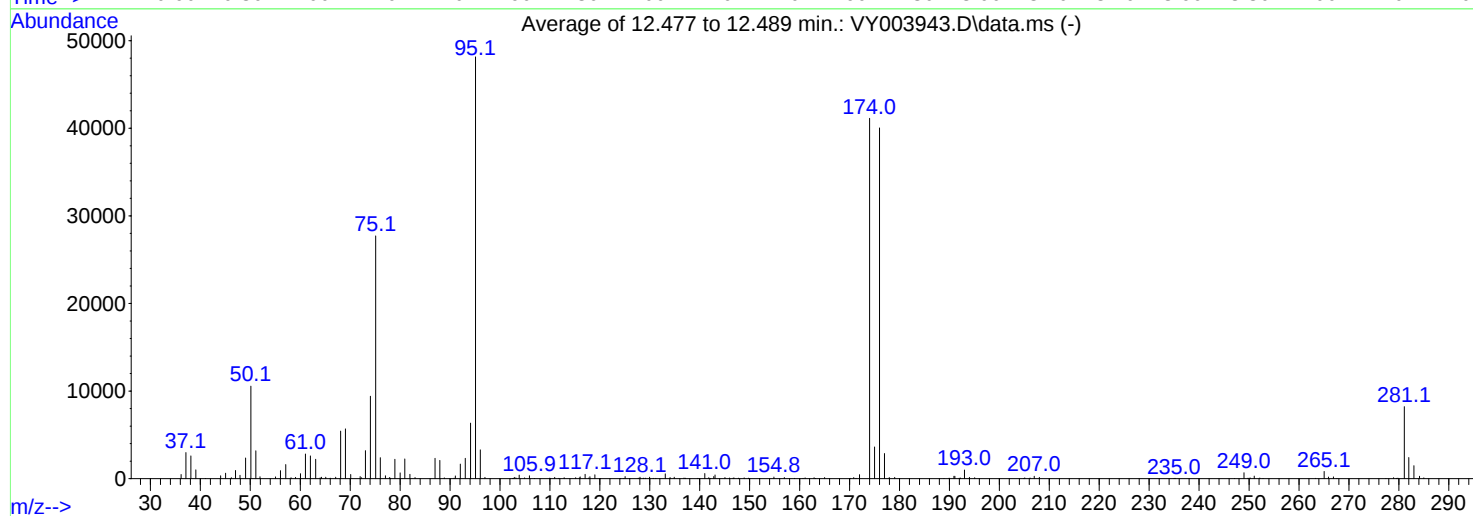


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY012721\
 Data File : VY003943.D
 Acq On : 27 Jan 2021 10:33
 Operator : SY/MD
 Sample : BFB
 Misc : 5.00g/5mL/MSVOA_Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y012721S.M
 Title : SW846 8260
 Last Update : Thu Jan 28 04:46:32 2021

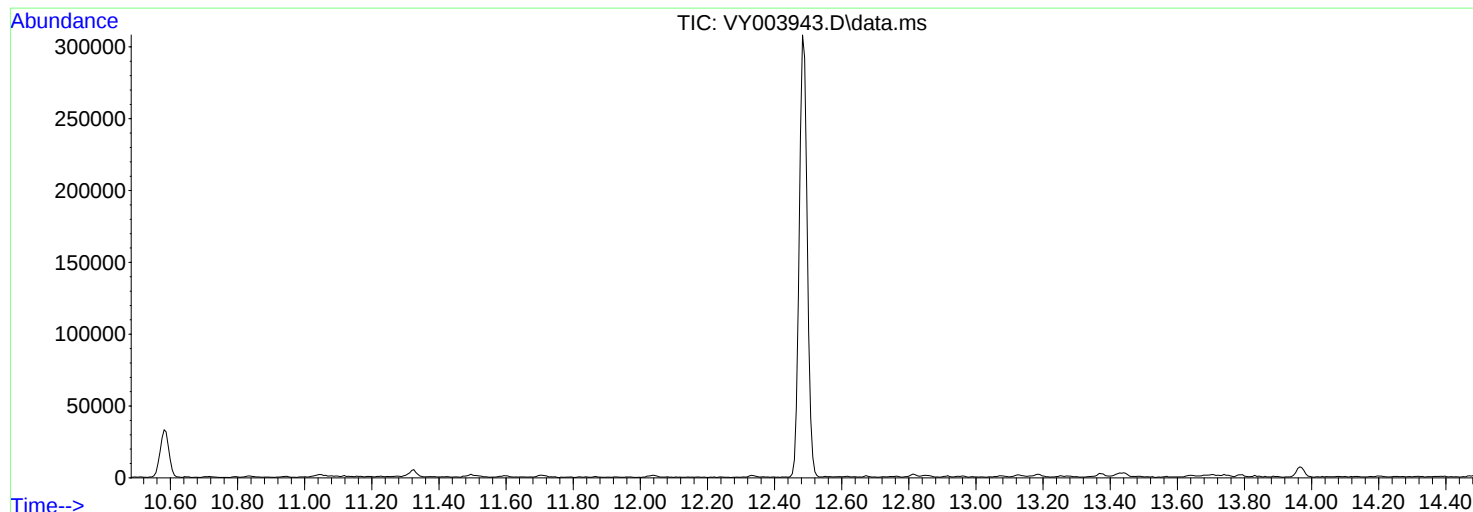

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.9	10555	PASS
75	95	30	60	57.5	27704	PASS
95	95	100	100	100.0	48155	PASS
96	95	5	9	6.8	3289	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	85.4	41136	PASS
175	174	5	9	8.8	3611	PASS
176	174	95	101	97.3	40032	PASS
177	176	5	9	7.2	2868	PASS