

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY012723\
 Data File : VY012377.D
 Acq On : 27 Jan 2023 12:41
 Operator : KP/MD
 Sample : VY0127SBL07
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VY0127SBL07

Quant Time: Jan 30 02:36:37 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y011623S.M
 Quant Title : SW846 8260
 QLast Update : Tue Jan 17 04:31:47 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.789	168	165736	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.691	114	277107	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.490	117	266120	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	120766	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.143	65	96648	72.090	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	144.180%
35) Dibromofluoromethane	7.716	113	79422	54.129	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	108.260%
50) Toluene-d8	10.179	98	327123	65.706	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	131.420%
62) 4-Bromofluorobenzene	12.483	95	105490	51.000	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	102.000%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY012723\
Data File : VY012377.D
Acq On : 27 Jan 2023 12:41
Operator : KP/MD
Sample : VY0127SBL07
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VY0127SBL07

Quant Time: Jan 30 02:36:37 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y011623S.M
Quant Title : SW846 8260
QLast Update : Tue Jan 17 04:31:47 2023
Response via : Initial Calibration




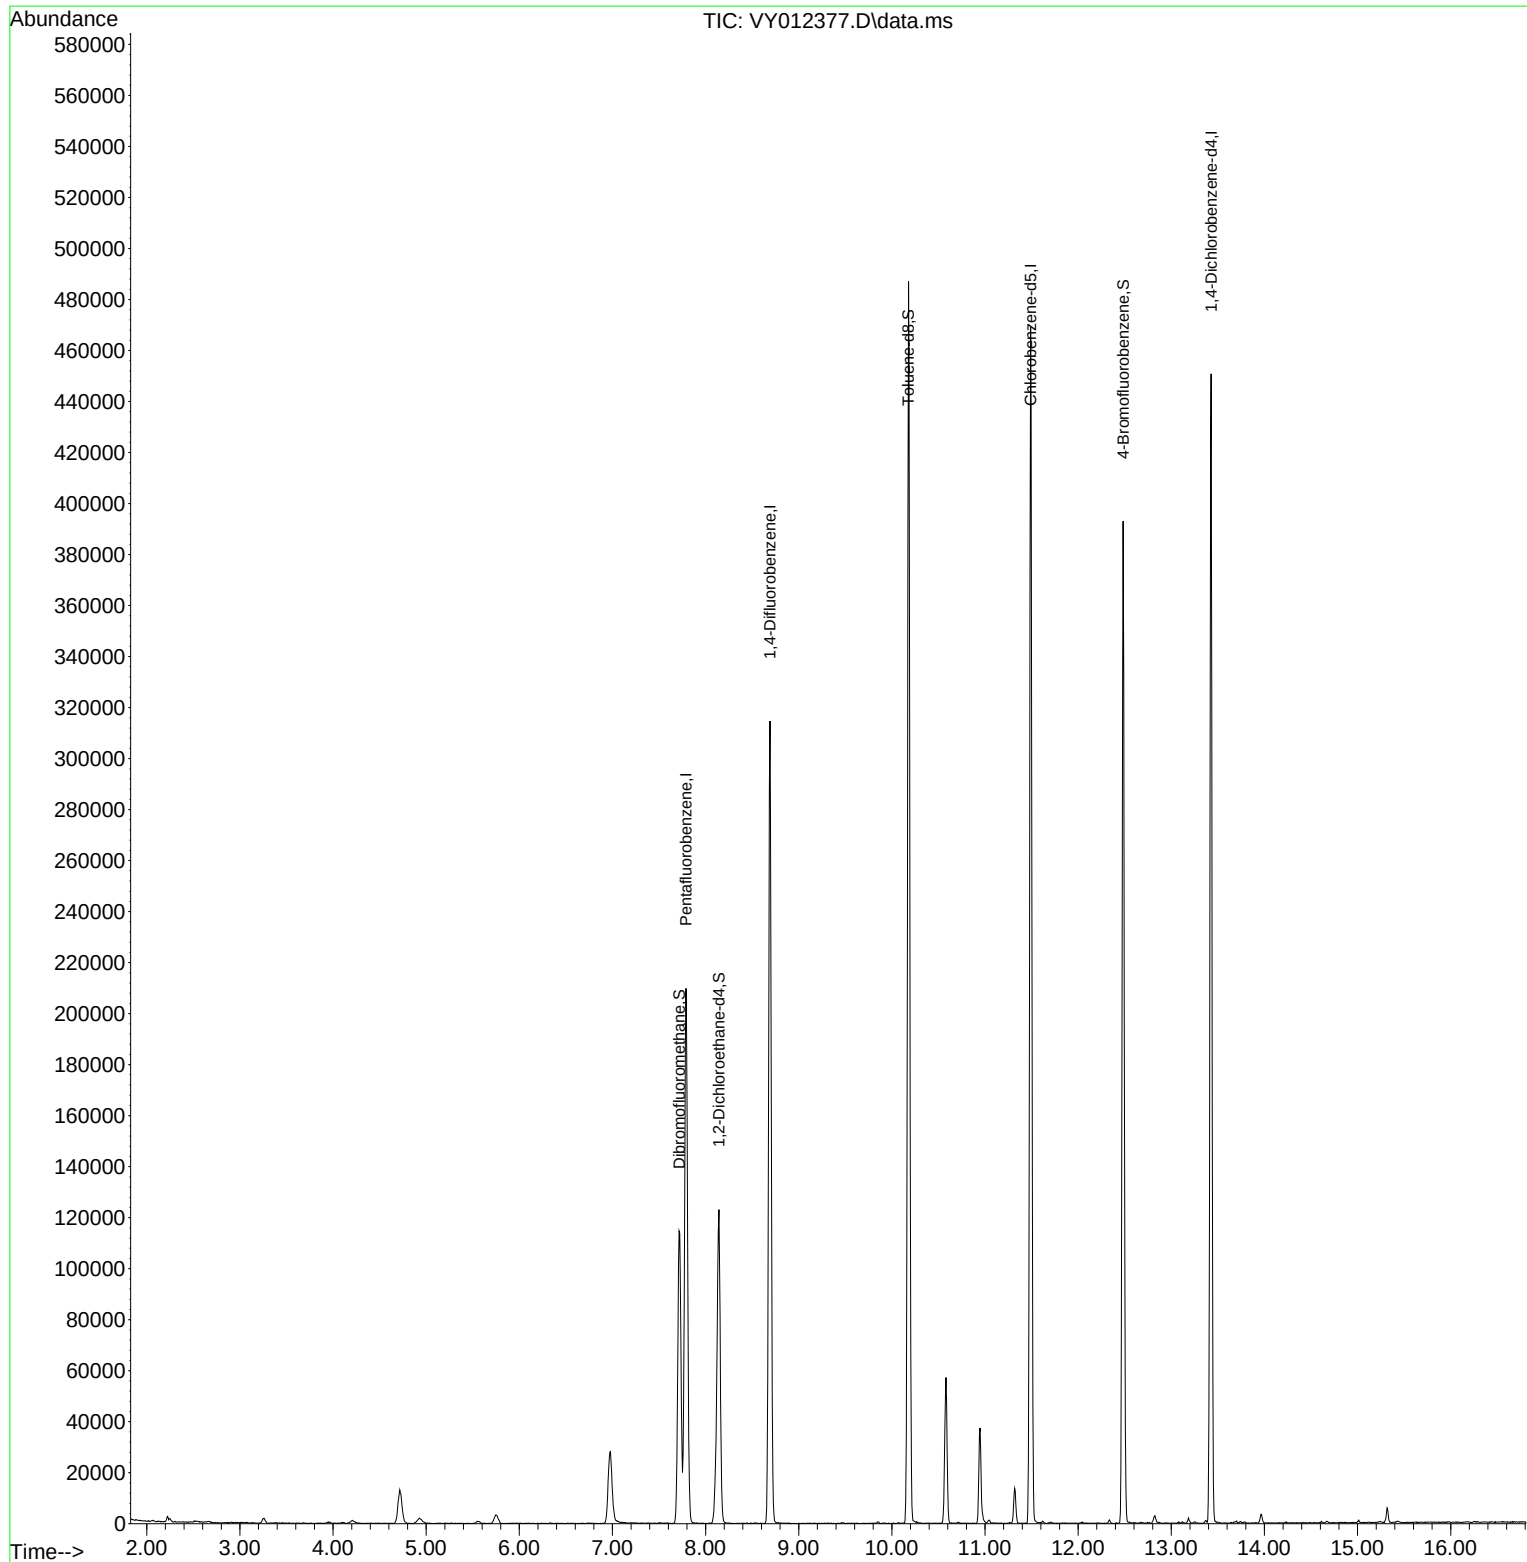


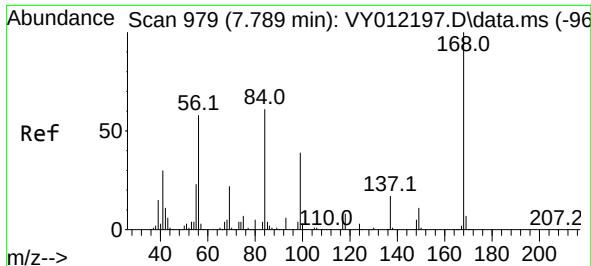

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. 0.000 min
Lab File: VY012377.D
Acq: 27 Jan 2023 12:41




Instrument :
MSVOA_Y
ClientSampleId :
VY0127SBL07


Tgt Ion:168 Resp: 165736
Ion Ratio Lower Upper
168 100
99 56.7 44.0 66.0

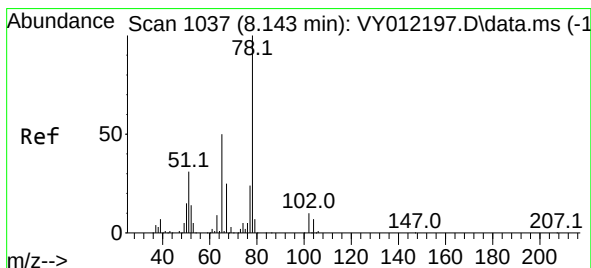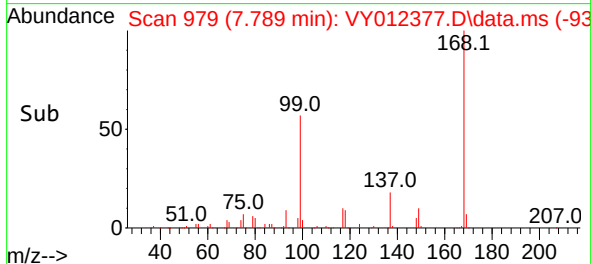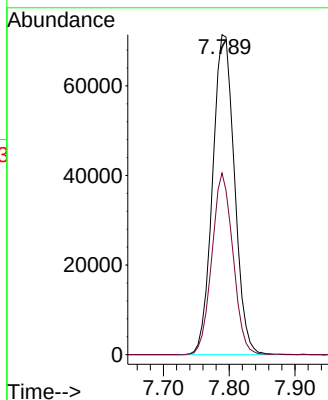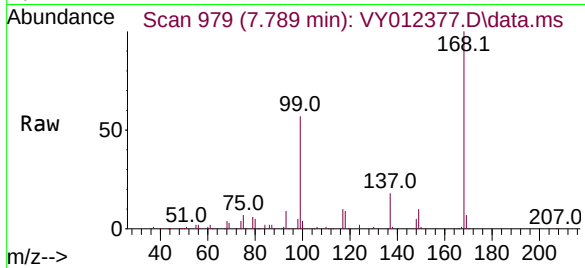

#33
1,2-Dichloroethane-d4
Concen: 72.090 ug/l
RT: 8.143 min Scan# 1037
Delta R.T. -0.000 min
Lab File: VY012377.D
Acq: 27 Jan 2023 12:41

Tgt Ion: 65 Resp: 96648
Ion Ratio Lower Upper
65 100
67 48.3 0.0 103.2

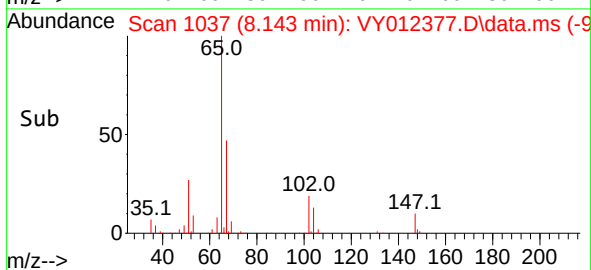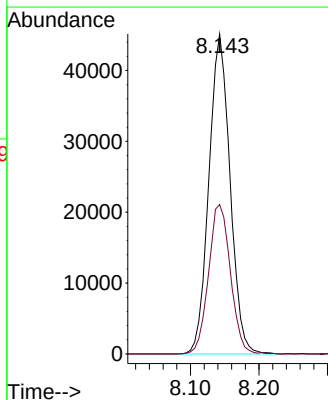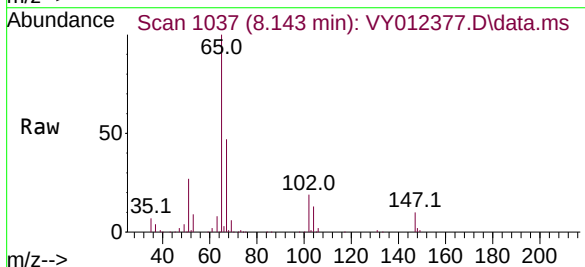

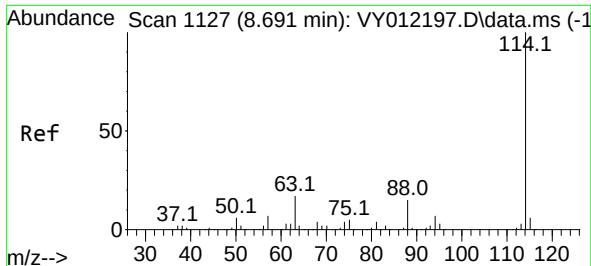

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.691 min Scan# 1127

Delta R.T. 0.000 min

Lab File: VY012377.D

Acq: 27 Jan 2023 12:41

Instrument :

MSVOA_Y

ClientSampleId :

VY0127SBL07





Tgt Ion:114 Resp: 277107

Ion Ratio Lower Upper

114 100

63 17.5 0.0 39.6

88 15.2 0.0 32.2

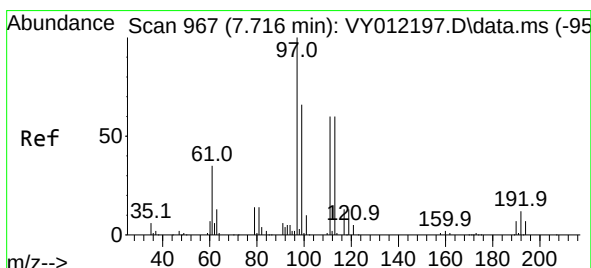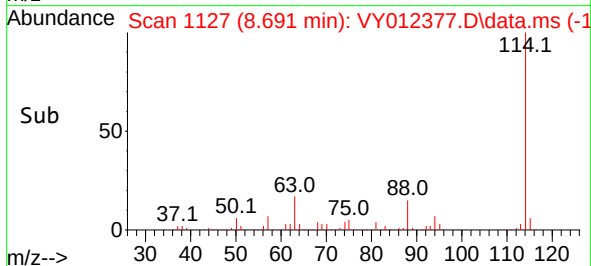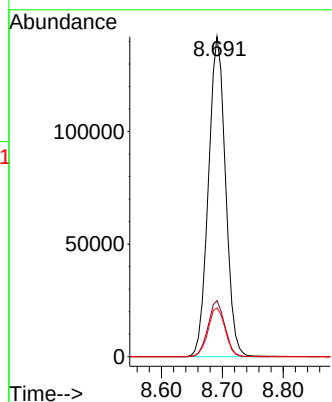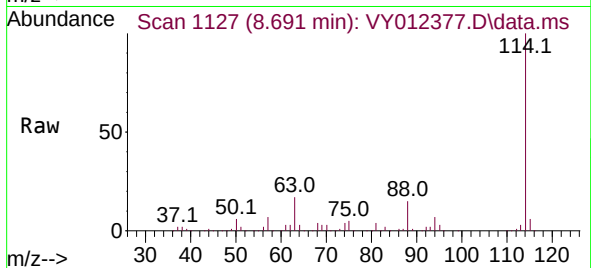

#35

Dibromofluoromethane

Concen: 54.129 ug/l

RT: 7.716 min Scan# 967

Delta R.T. -0.000 min

Lab File: VY012377.D

Acq: 27 Jan 2023 12:41




Tgt Ion:113 Resp: 79422


Ion Ratio Lower Upper

113 100

111 102.0 83.0 124.4

192 22.1 16.0 24.0

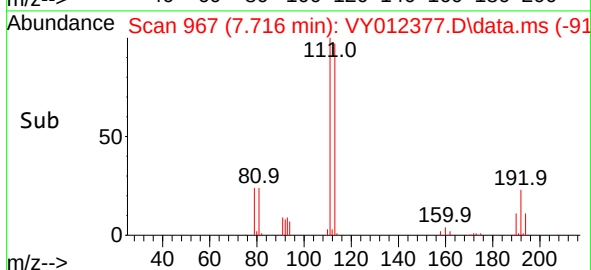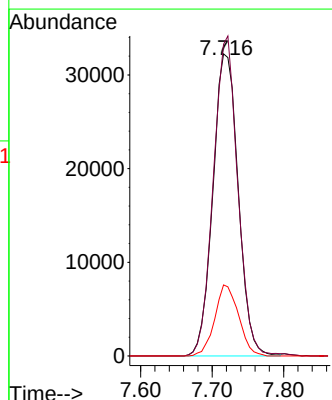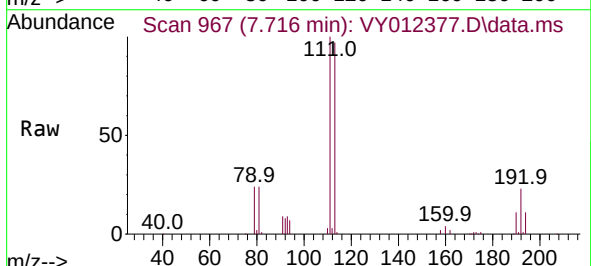

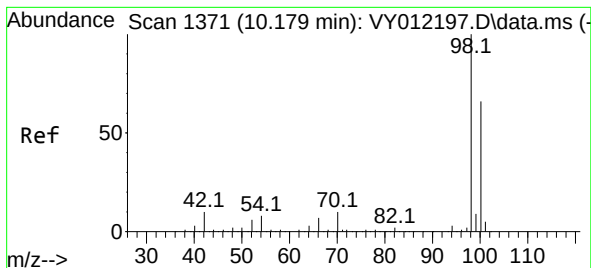

#50

Toluene-d8

Concen: 65.706 ug/l

RT: 10.179 min Scan# 1371

Delta R.T. -0.000 min

Lab File: VY012377.D

Acq: 27 Jan 2023 12:41

Instrument :

MSVOA_Y

ClientSampleId :





VY0127SBL07

Tgt Ion: 98 Resp: 327123

Ion Ratio Lower Upper

98 100

100 65.0 51.9 77.9

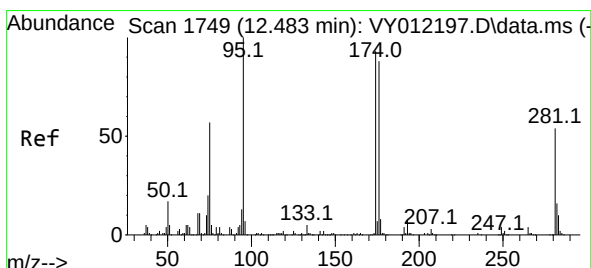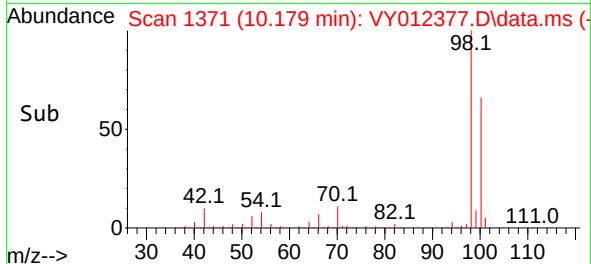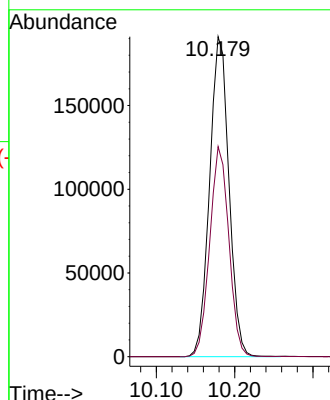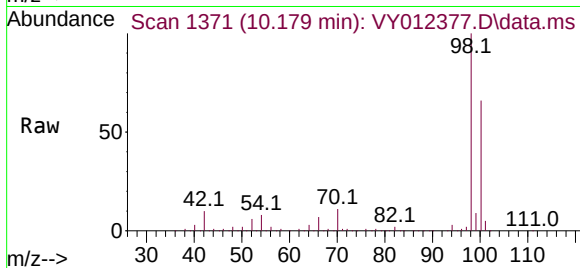

#62

4-Bromofluorobenzene

Concen: 51.000 ug/l

RT: 12.483 min Scan# 1749

Delta R.T. 0.000 min

Lab File: VY012377.D

Acq: 27 Jan 2023 12:41




Tgt Ion: 95 Resp: 105490


Ion Ratio Lower Upper

95 100

174 93.9 0.0 172.0

176 92.1 0.0 167.6

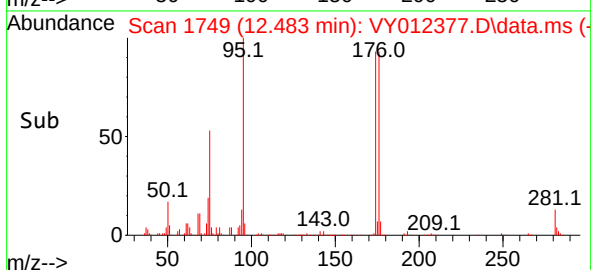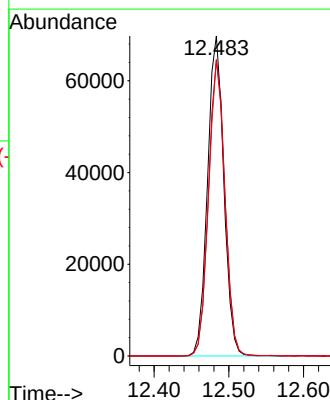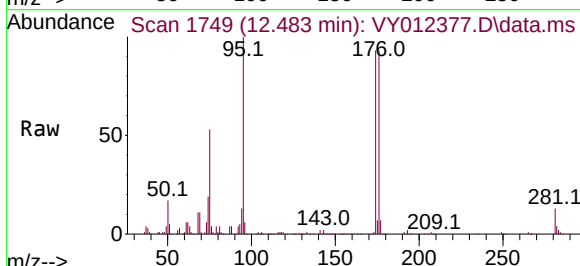

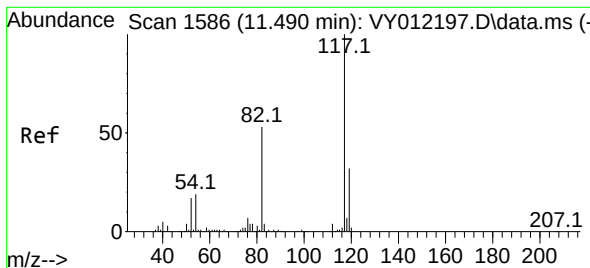

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.490 min Scan# 11

Delta R.T. -0.000 min

Lab File: VY012377.D

Acq: 27 Jan 2023 12:41

Instrument :

MSVOA_Y

ClientSampleId :

VY0127SBL07





Tgt Ion:117 Resp: 266120

Ion Ratio Lower Upper

117 100

82 52.3 44.8 67.2

119 32.4 25.4 38.2

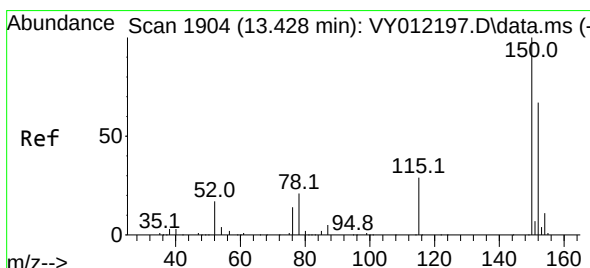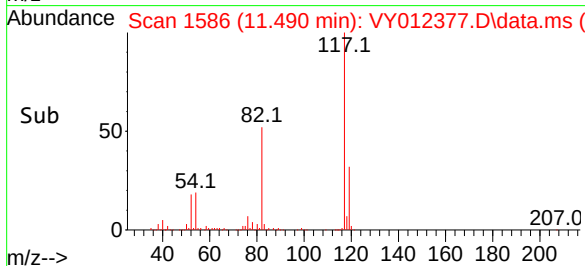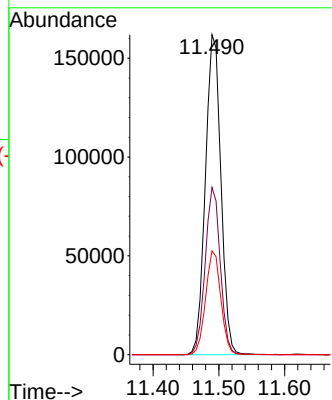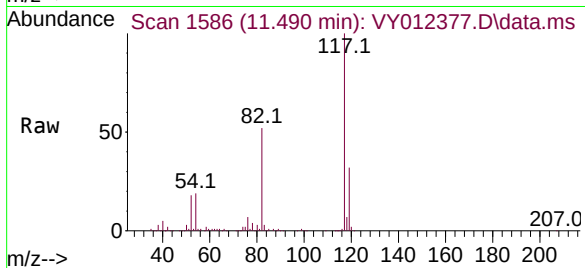

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.428 min Scan# 1904

Delta R.T. 0.006 min

Lab File: VY012377.D

Acq: 27 Jan 2023 12:41

Tgt Ion:152 Resp: 120766

Ion Ratio Lower Upper

152 100

115 56.9 29.1 87.3

150 156.4 0.0 342.6

