
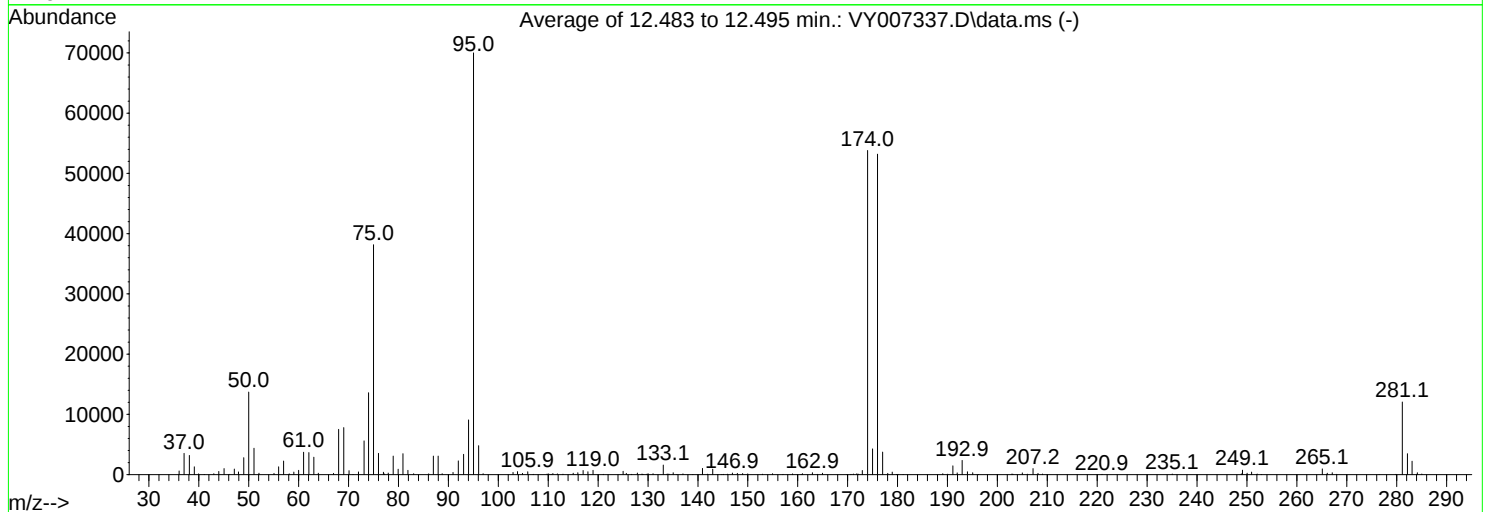


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY013122\
Data File : VY007337.D
Acq On : 31 Jan 2022 12:41
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y011322S.M
Title : SW846 8260
Last Update : Fri Jan 14 05:48:29 2022

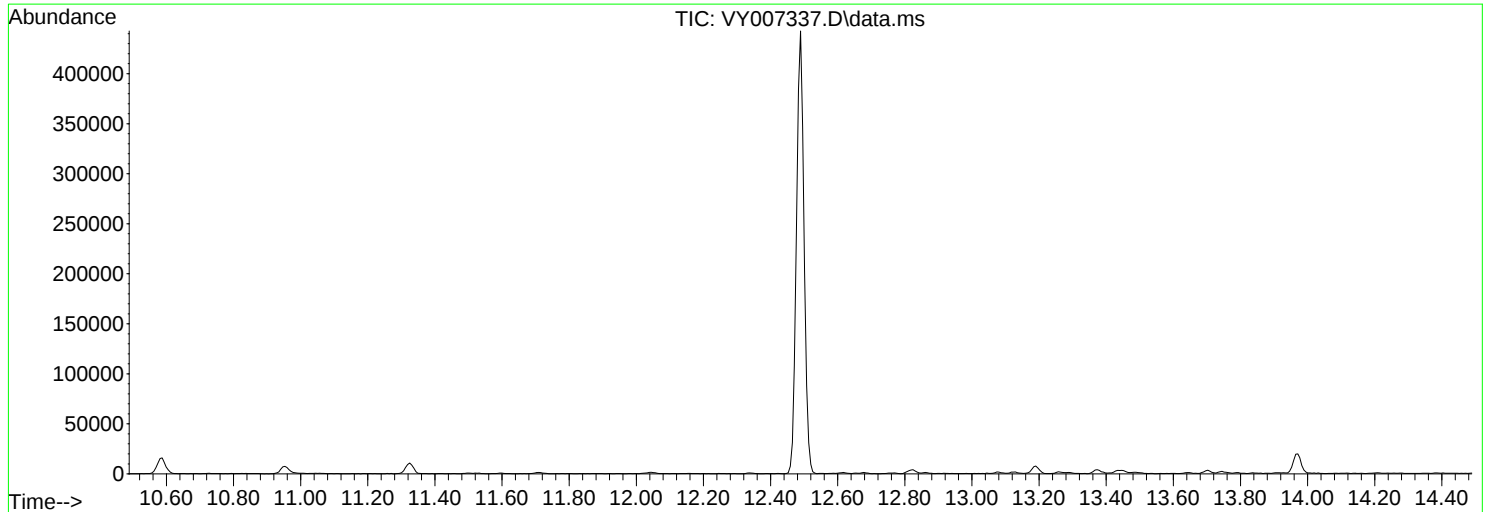

AutoFind: Scans 1749, 1750, 1751; Background Corrected with Scan 1741

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.6	13694	PASS
75	95	30	60	54.5	38176	PASS
95	95	100	100	100.0	70013	PASS
96	95	5	9	6.9	4817	PASS
173	174	0.00	2	1.3	698	PASS
174	95	50	100	76.9	53808	PASS
175	174	5	9	8.0	4285	PASS
176	174	95	101	98.9	53211	PASS
177	176	5	9	7.1	3757	PASS