

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY020823\
 Data File : VY012535.D
 Acq On : 08 Feb 2023 12:18
 Operator : KP/MD
 Sample : 01464-09
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 TRIP-BLANK

Quant Time: Feb 09 07:13:16 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y020723S.M
 Quant Title : SW846 8260
 QLast Update : Wed Feb 08 01:09:03 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.789	168	144146	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.691	114	241928	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.489	117	233968	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	110154	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.143	65	86917	47.418	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	94.840%
35) Dibromofluoromethane	7.716	113	71973	40.851	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	81.700%
50) Toluene-d8	10.179	98	283665	38.681	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	77.360%
62) 4-Bromofluorobenzene	12.483	95	94423	36.914	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	73.820%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY020823\
Data File : VY012535.D
Acq On : 08 Feb 2023 12:18
Operator : KP/MD
Sample : 01464-09
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
TRIP-BLANK

Quant Time: Feb 09 07:13:16 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y020723S.M
Quant Title : SW846 8260
QLast Update : Wed Feb 08 01:09:03 2023
Response via : Initial Calibration




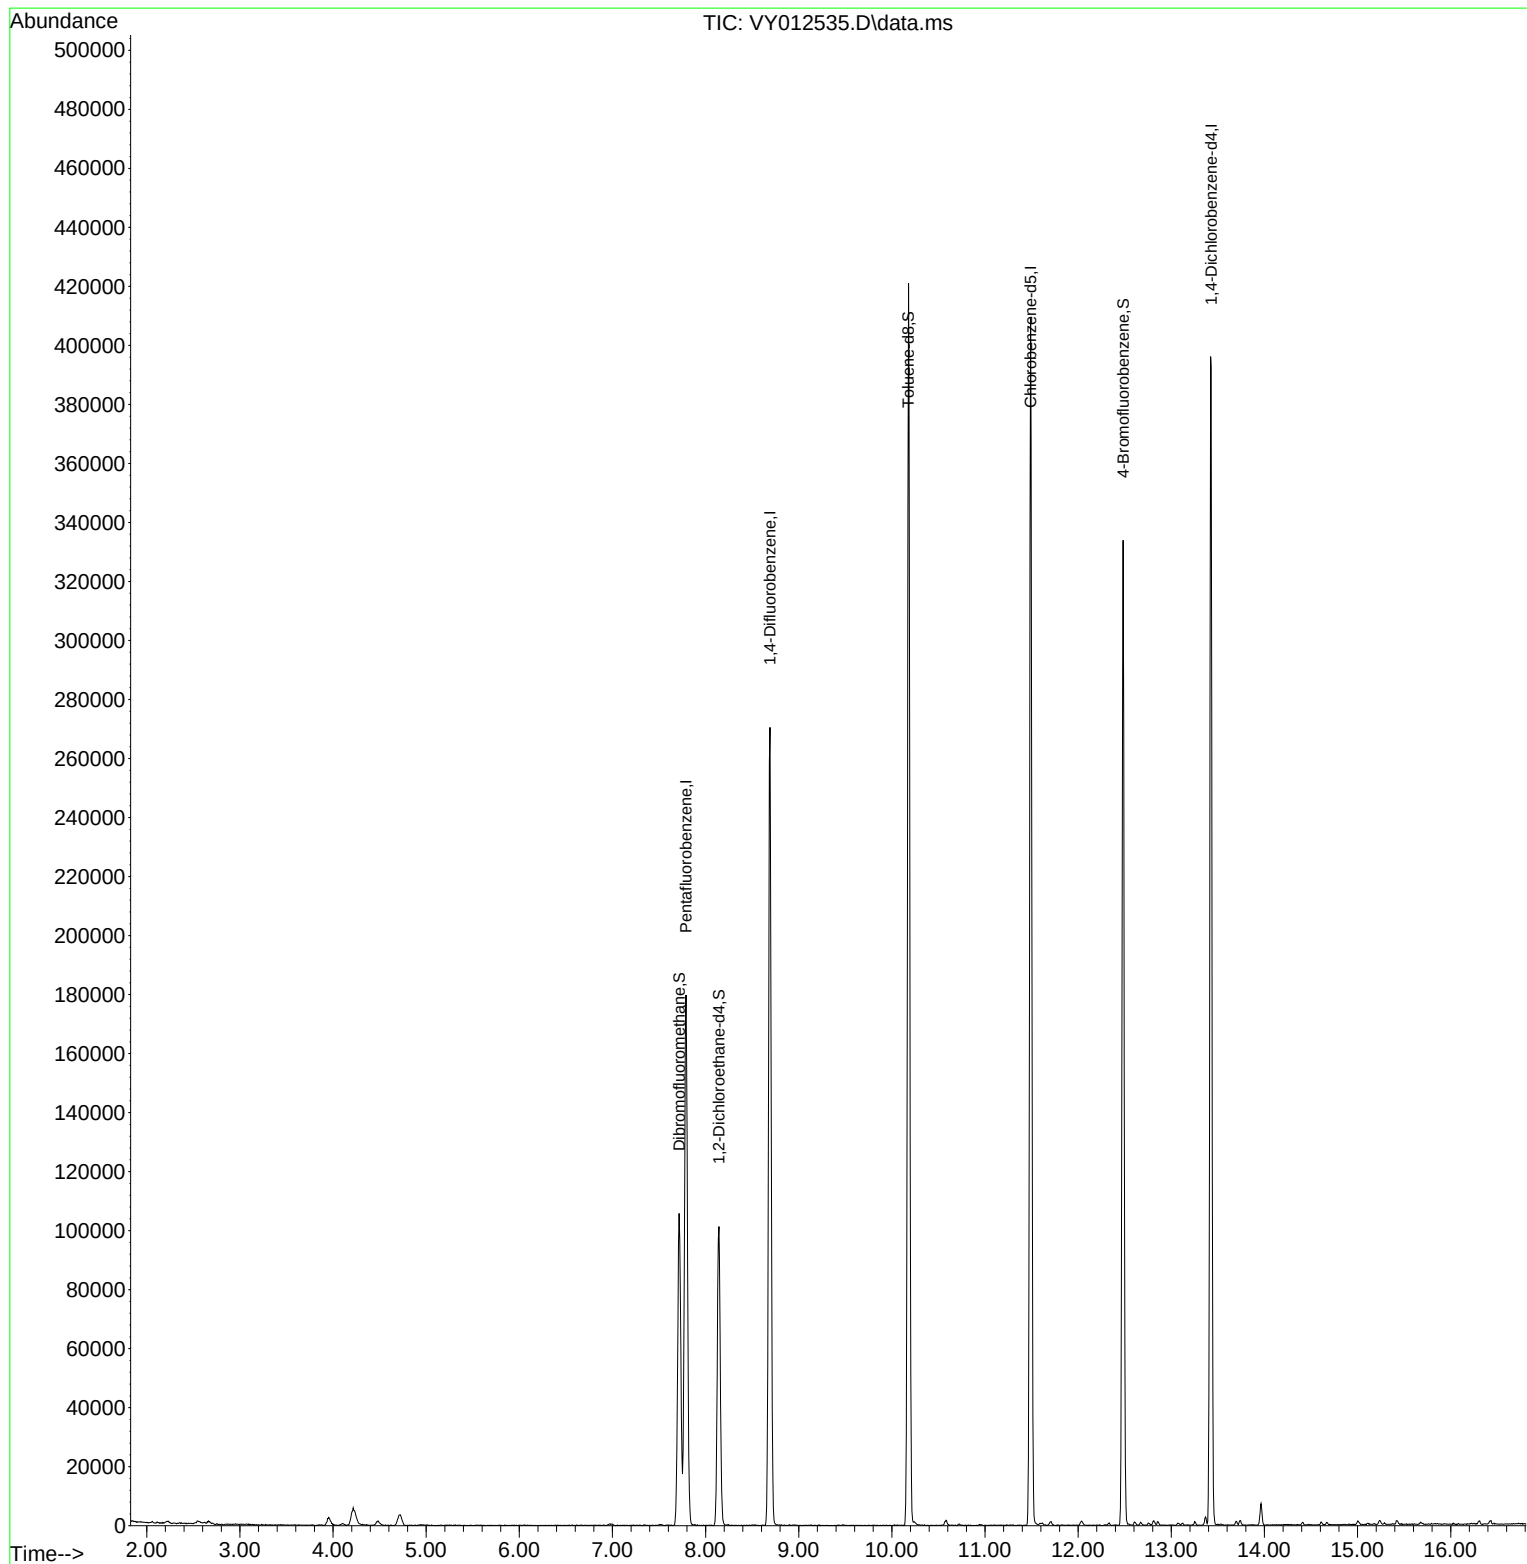


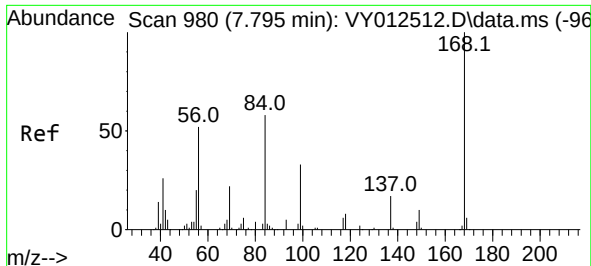

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. -0.006 min
Lab File: VY012535.D
Acq: 08 Feb 2023 12:18




Instrument :
MSVOA_Y
ClientSampleId :
TRIP-BLANK


Tgt Ion:168 Resp: 144146
Ion Ratio Lower Upper
168 100
99 54.4 40.8 61.2

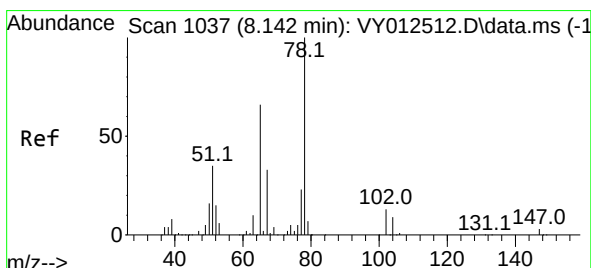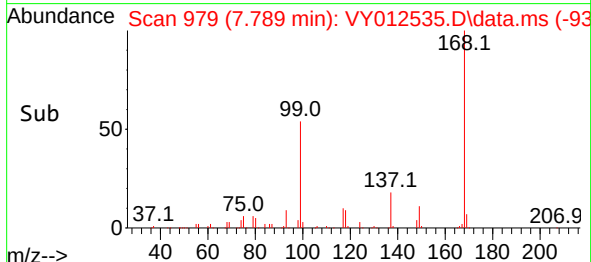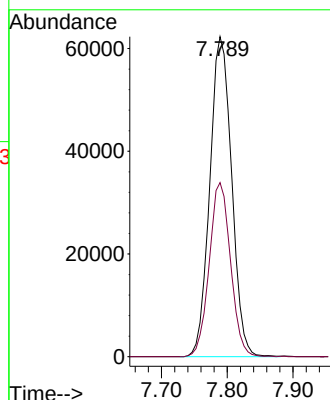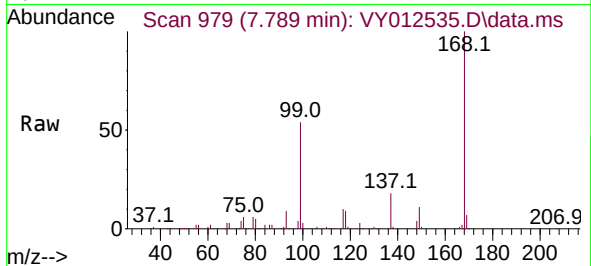

#33
1,2-Dichloroethane-d4
Concen: 47.418 ug/l
RT: 8.143 min Scan# 1037
Delta R.T. 0.000 min
Lab File: VY012535.D
Acq: 08 Feb 2023 12:18

Tgt Ion: 65 Resp: 86917
Ion Ratio Lower Upper
65 100
67 48.7 0.0 98.6

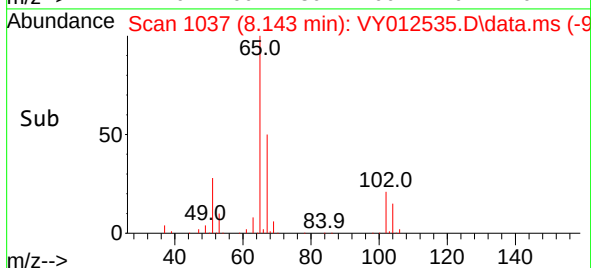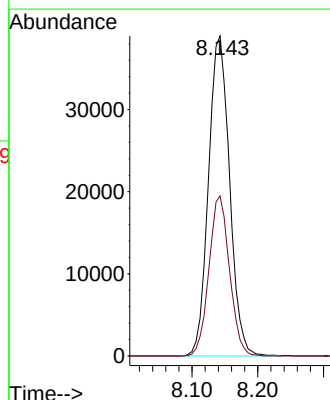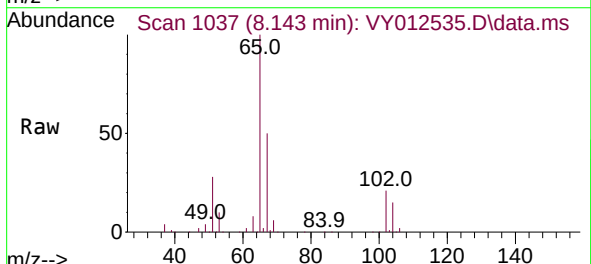

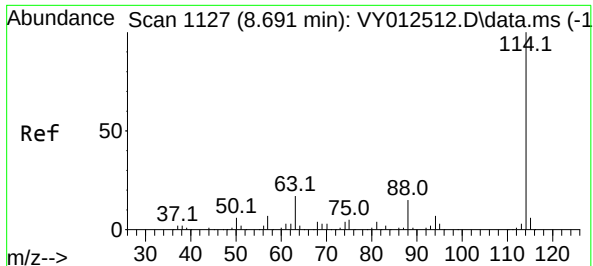

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.691 min Scan# 1127

Delta R.T. 0.000 min

Lab File: VY012535.D

Acq: 08 Feb 2023 12:18

Instrument :

MSVOA_Y

ClientSampleId :

TRIP-BLANK





Tgt Ion:114 Resp: 241928

Ion Ratio Lower Upper

114 100

63 17.2 0.0 33.6

88 14.9 0.0 29.8

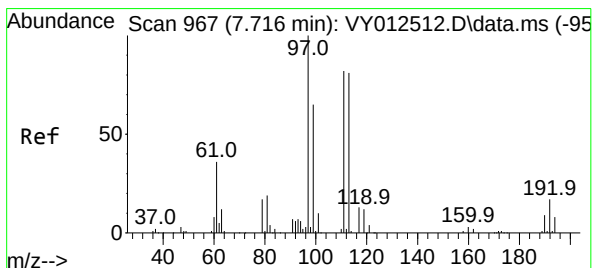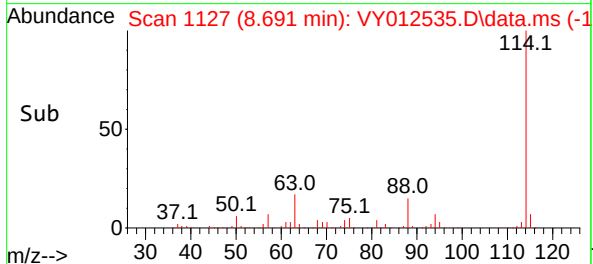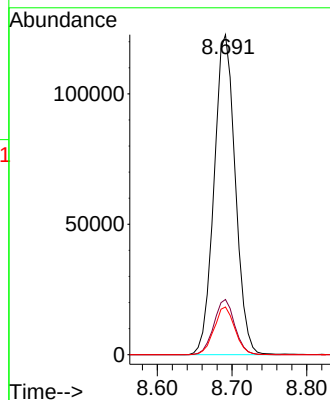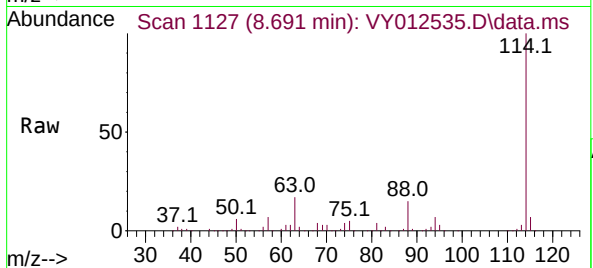

#35

Dibromofluoromethane

Concen: 40.851 ug/l

RT: 7.716 min Scan# 967

Delta R.T. 0.000 min

Lab File: VY012535.D

Acq: 08 Feb 2023 12:18




Tgt Ion:113 Resp: 71973


Ion Ratio Lower Upper

113 100

111 101.4 81.9 122.9

192 22.3 17.5 26.3


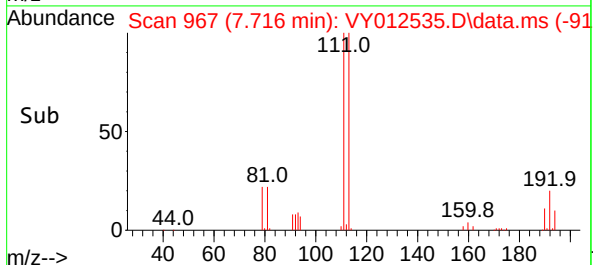
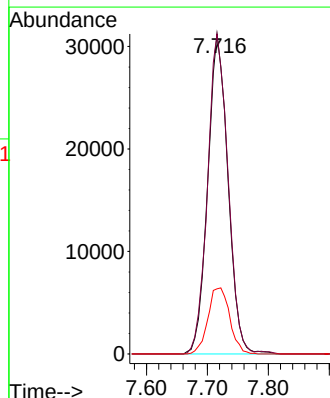
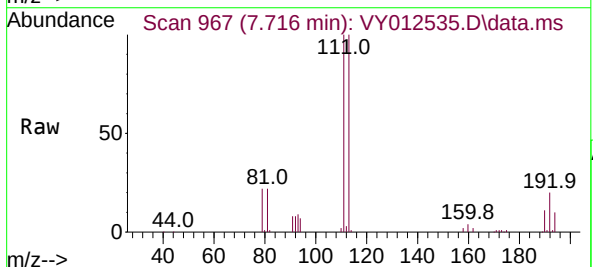


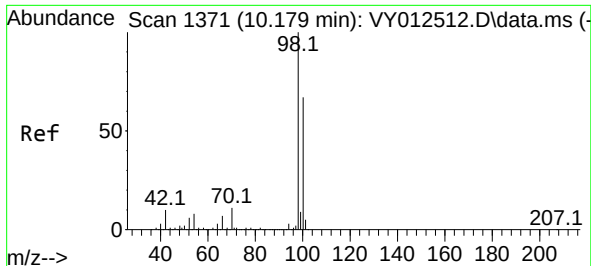

#50
Toluene-d8
Concen: 38.681 ug/l
RT: 10.179 min Scan# 1371
Delta R.T. 0.000 min
Lab File: VY012535.D
Acq: 08 Feb 2023 12:18




Instrument :
MSVOA_Y
ClientSampleId :
TRIP-BLANK


Tgt Ion: 98 Resp: 283665
Ion Ratio Lower Upper
98 100
100 64.3 52.2 78.2

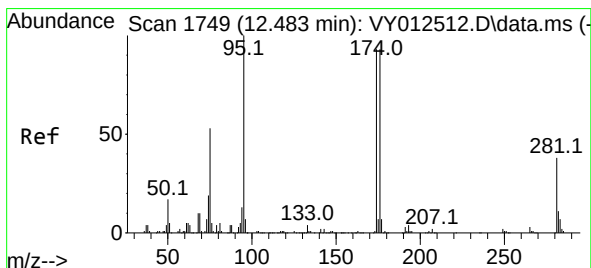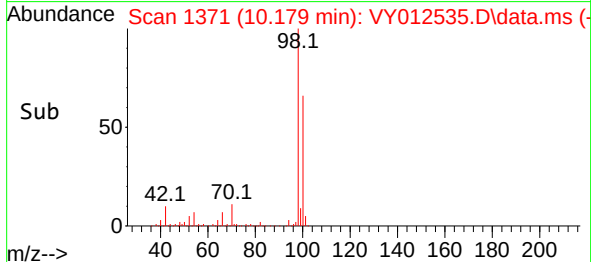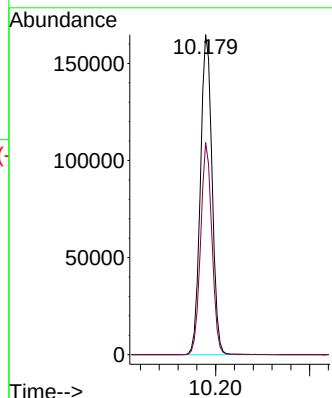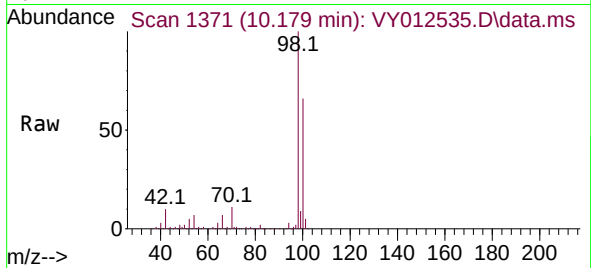

#62
4-Bromofluorobenzene
Concen: 36.914 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.000 min
Lab File: VY012535.D
Acq: 08 Feb 2023 12:18

Tgt Ion: 95 Resp: 94423
Ion Ratio Lower Upper
95 100
174 97.2 0.0 188.0
176 92.4 0.0 183.6

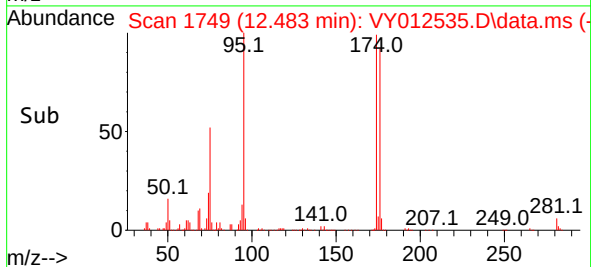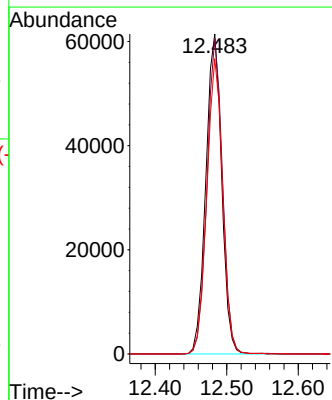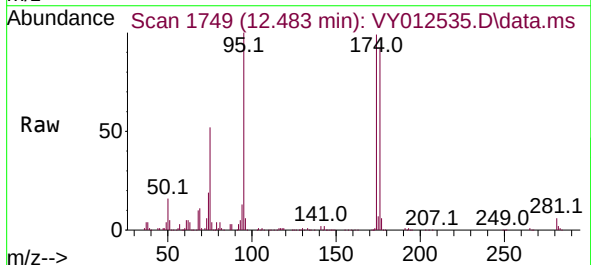

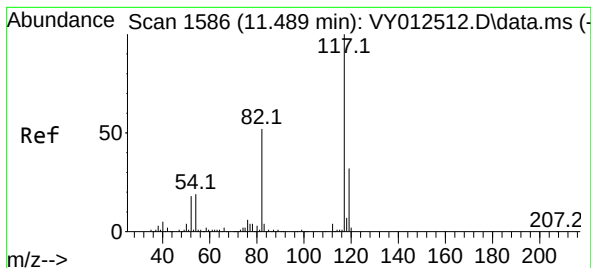

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.489 min Scan# 1

Delta R.T. 0.000 min

Lab File: VY012535.D

Acq: 08 Feb 2023 12:18

Instrument :

MSVOA_Y

ClientSampleId :

TRIP-BLANK





Tgt Ion:117 Resp: 233968

Ion Ratio Lower Upper

117 100

82 51.3 41.7 62.5

119 30.8 25.8 38.8

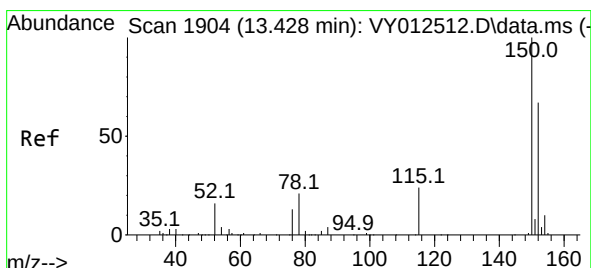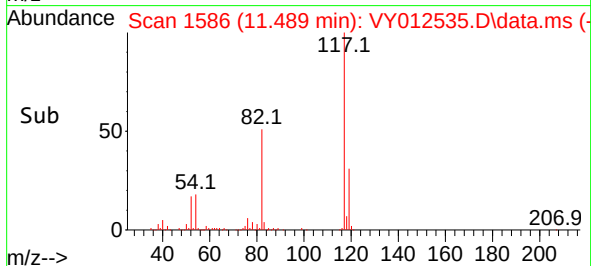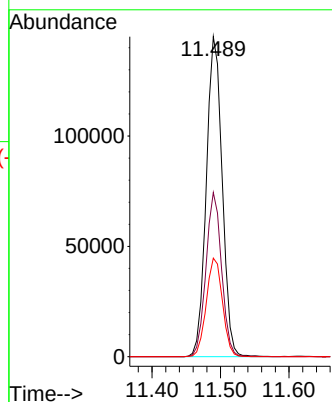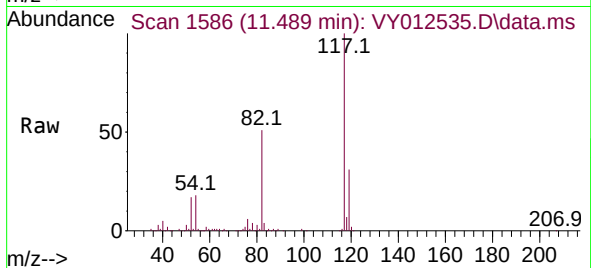

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.428 min Scan# 1904

Delta R.T. 0.000 min

Lab File: VY012535.D

Acq: 08 Feb 2023 12:18

Tgt Ion:152 Resp: 110154

Ion Ratio Lower Upper

152 100

115 55.5 28.1 84.3

150 158.5 0.0 351.0

