

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY020823\
 Data File : VY012550.D
 Acq On : 08 Feb 2023 18:09
 Operator : KP/MD
 Sample : 01481-09
 Misc : 7.04g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 JPP-46-020723

Quant Time: Feb 09 07:15:46 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y020723S.M
 Quant Title : SW846 8260
 QLast Update : Wed Feb 08 01:09:03 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.789	168	146763	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.685	114	244408	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.490	117	233614	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.422	152	102425	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.137	65	88358	47.345	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	94.680%
35) Dibromofluoromethane	7.716	113	72195	40.561	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	81.120%
50) Toluene-d8	10.179	98	288678	38.965	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	77.940%
62) 4-Bromofluorobenzene	12.483	95	91887	35.558	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	71.120%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY020823\
Data File : VY012550.D
Acq On : 08 Feb 2023 18:09
Operator : KP/MD
Sample : 01481-09
Misc : 7.04g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
JPP-46-020723

Quant Time: Feb 09 07:15:46 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y020723S.M
Quant Title : SW846 8260
QLast Update : Wed Feb 08 01:09:03 2023
Response via : Initial Calibration




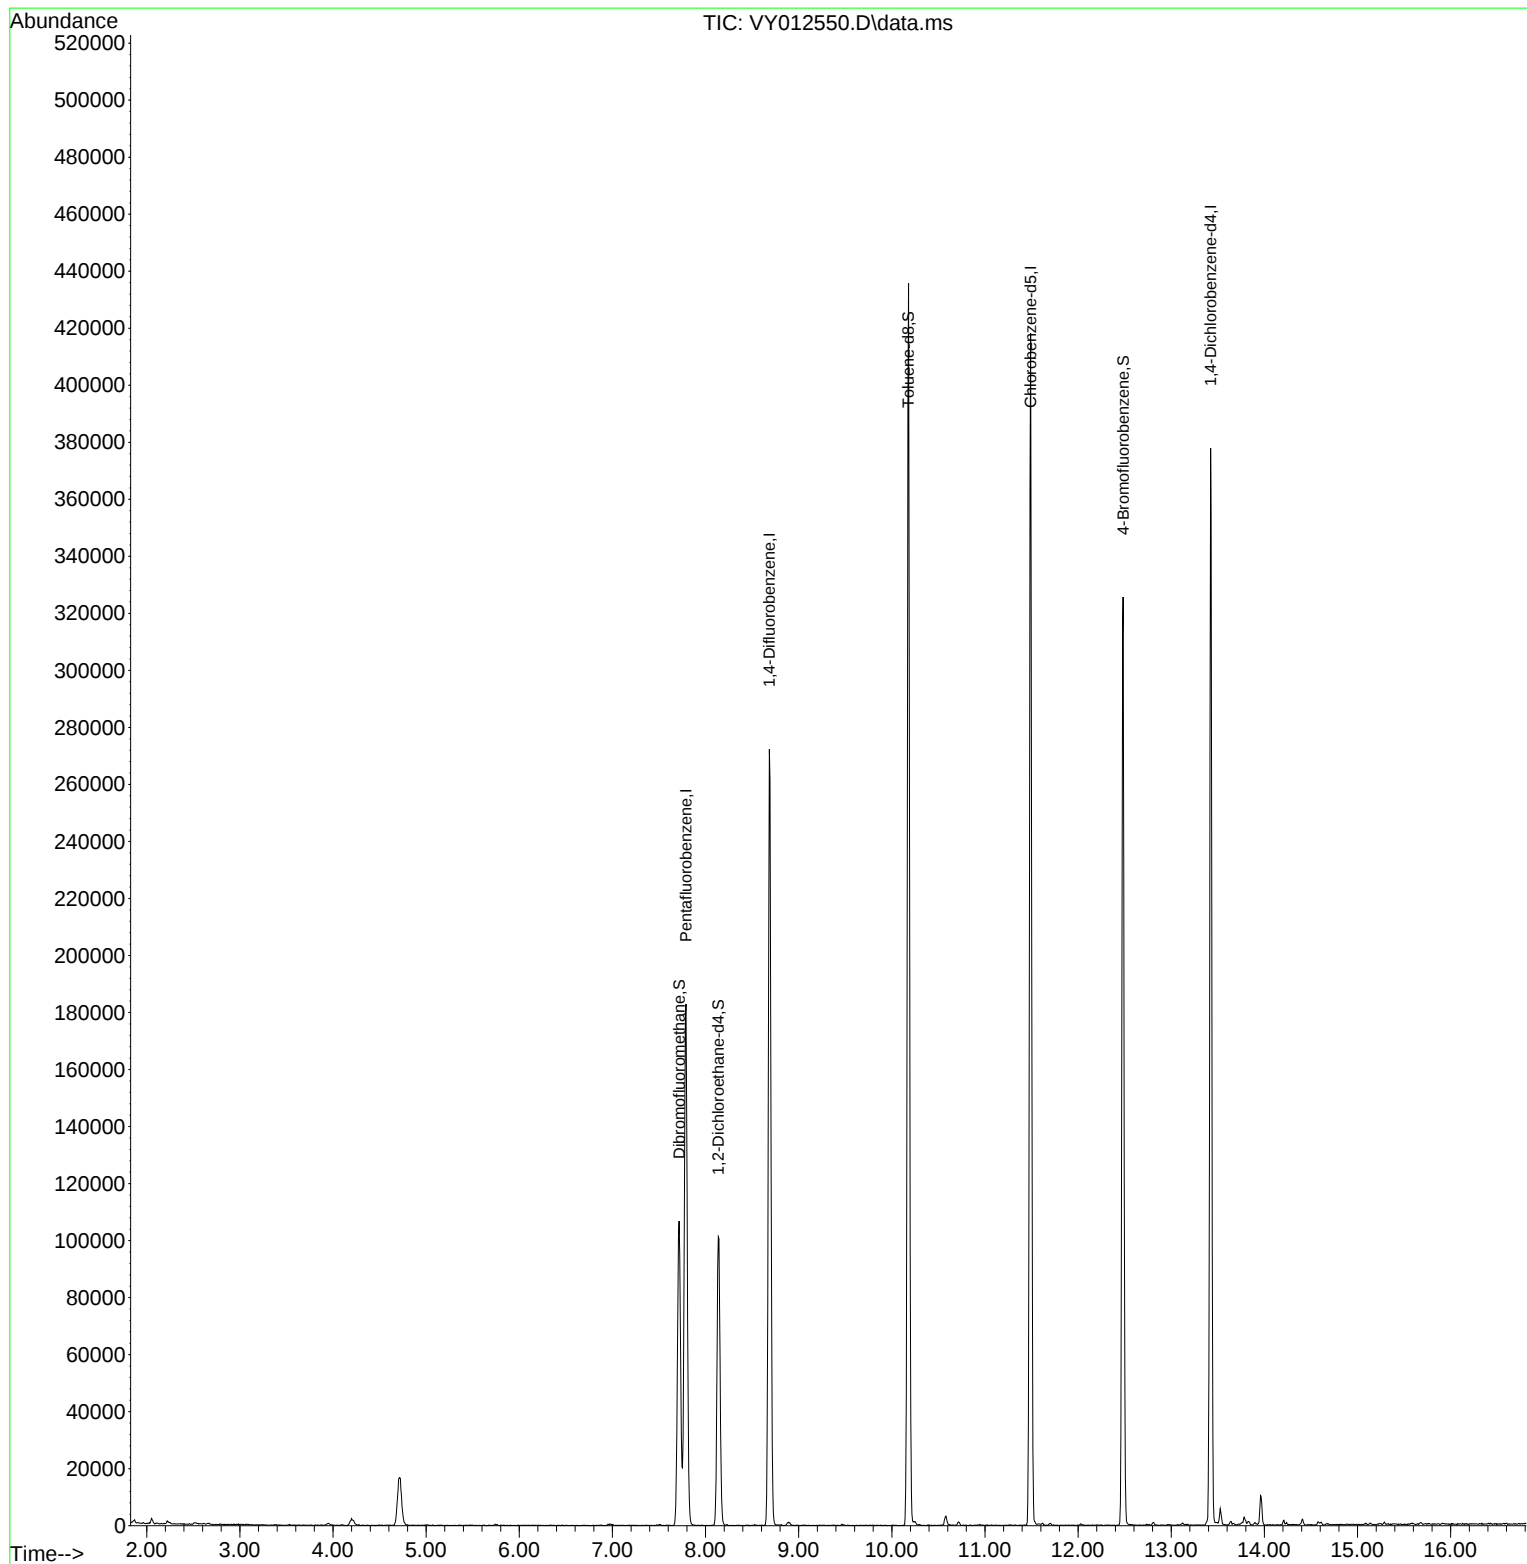


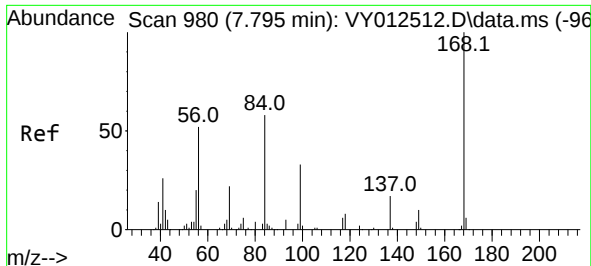

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. -0.006 min
Lab File: VY012550.D
Acq: 08 Feb 2023 18:09




Instrument :
MSVOA_Y
ClientSampleId :
JPP-46-020723


Tgt Ion:168 Resp: 146763
Ion Ratio Lower Upper
168 100
99 53.9 40.8 61.2

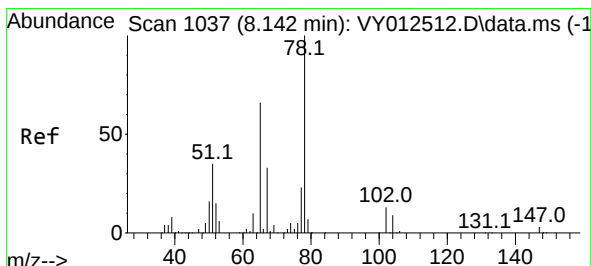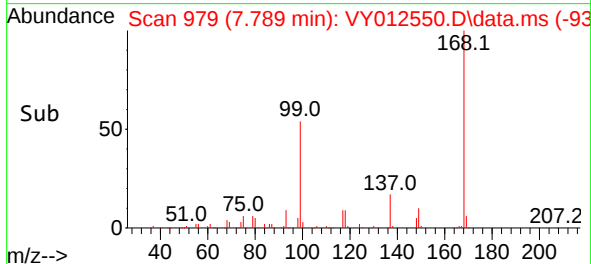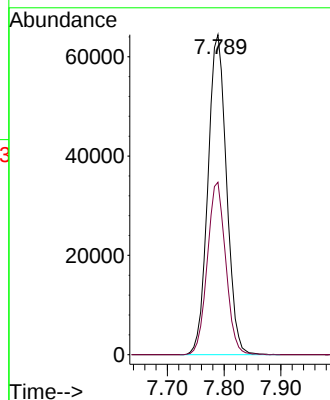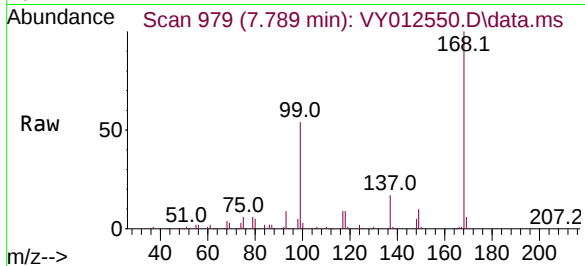

#33
1,2-Dichloroethane-d4
Concen: 47.345 ug/l
RT: 8.137 min Scan# 1036
Delta R.T. -0.006 min
Lab File: VY012550.D
Acq: 08 Feb 2023 18:09

Tgt Ion: 65 Resp: 88358
Ion Ratio Lower Upper
65 100
67 49.2 0.0 98.6

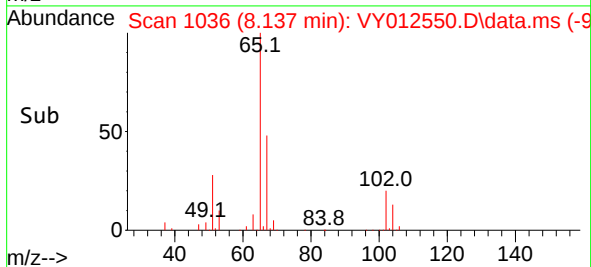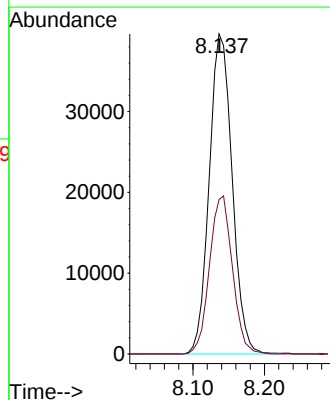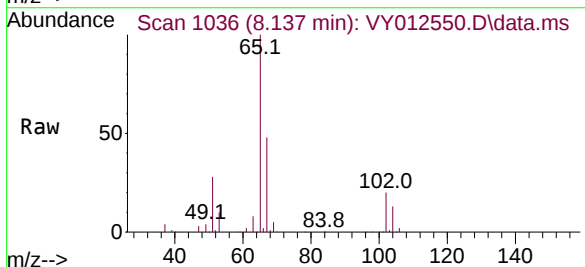

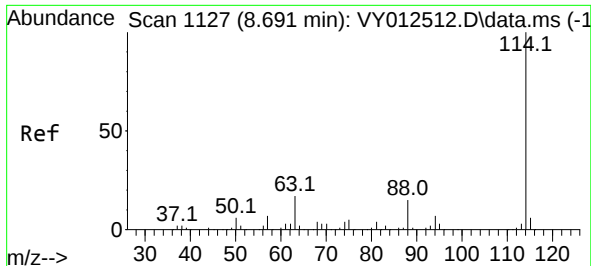

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.685 min Scan# 1126

Delta R.T. -0.006 min

Lab File: VY012550.D

Acq: 08 Feb 2023 18:09

Instrument :

MSVOA_Y

ClientSampleId :

JPP-46-020723





Tgt Ion:114 Resp: 244408

Ion Ratio Lower Upper

114 100

63 17.9 0.0 33.6

88 14.2 0.0 29.8

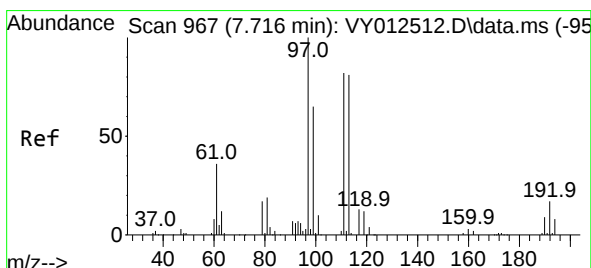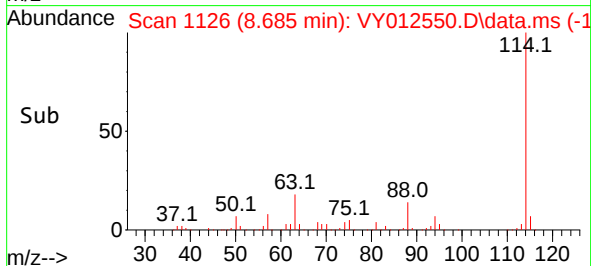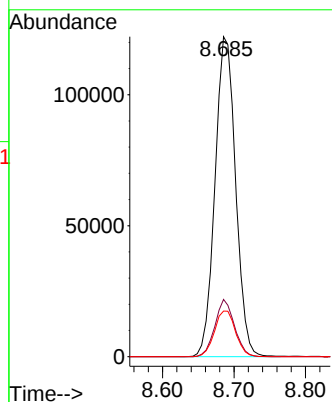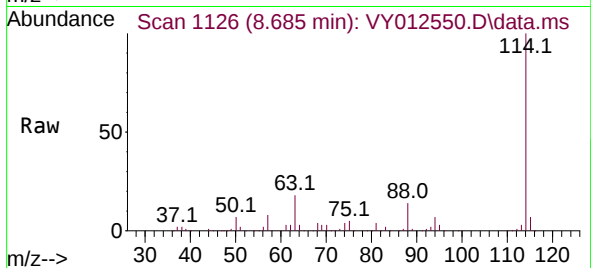

#35

Dibromofluoromethane

Concen: 40.561 ug/l

RT: 7.716 min Scan# 967

Delta R.T. 0.000 min

Lab File: VY012550.D

Acq: 08 Feb 2023 18:09




Tgt Ion:113 Resp: 72195


Ion Ratio Lower Upper

113 100

111 103.4 81.9 122.9

192 21.9 17.5 26.3


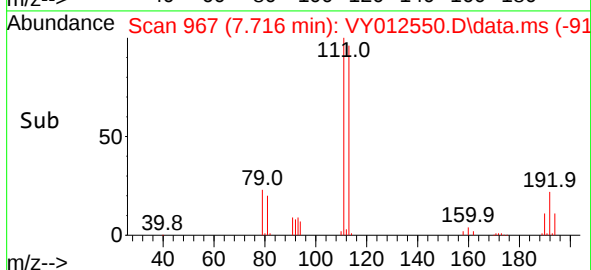
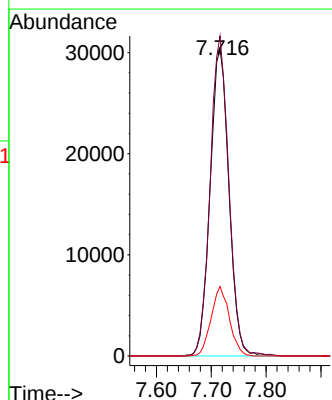
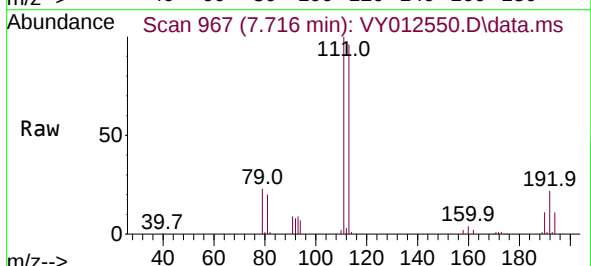


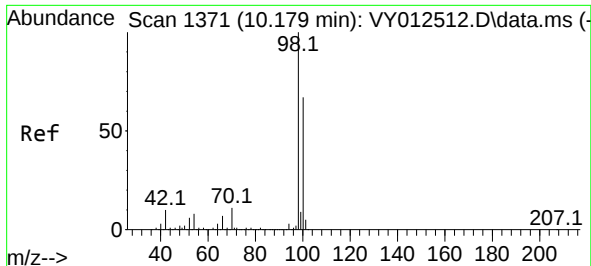

#50
Toluene-d8
Concen: 38.965 ug/l
RT: 10.179 min Scan# 1371
Delta R.T. 0.000 min
Lab File: VY012550.D
Acq: 08 Feb 2023 18:09




Instrument :
MSVOA_Y
ClientSampleId :
JPP-46-020723


Tgt Ion: 98 Resp: 288678
Ion Ratio Lower Upper
98 100
100 65.1 52.2 78.2

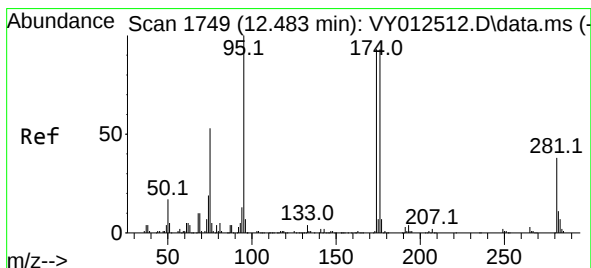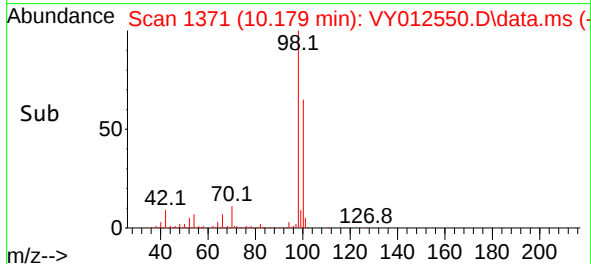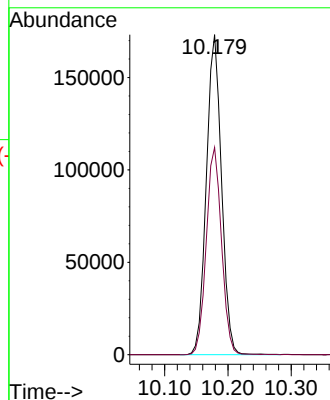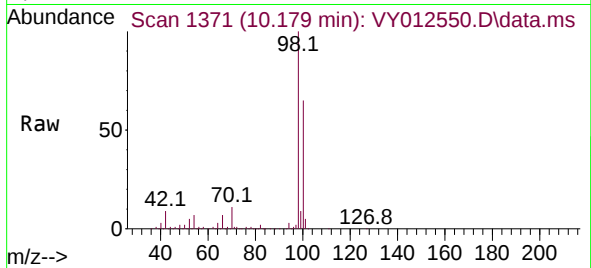

#62
4-Bromofluorobenzene
Concen: 35.558 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.000 min
Lab File: VY012550.D
Acq: 08 Feb 2023 18:09

Tgt Ion: 95 Resp: 91887
Ion Ratio Lower Upper
95 100
174 96.2 0.0 188.0
176 94.2 0.0 183.6


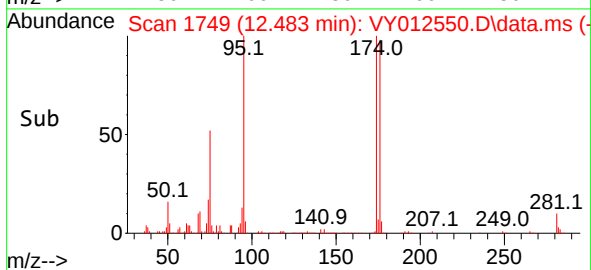
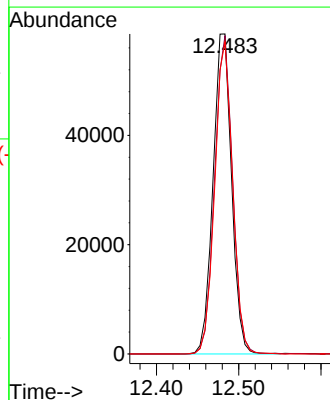
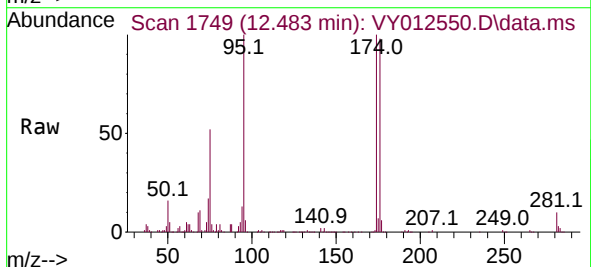


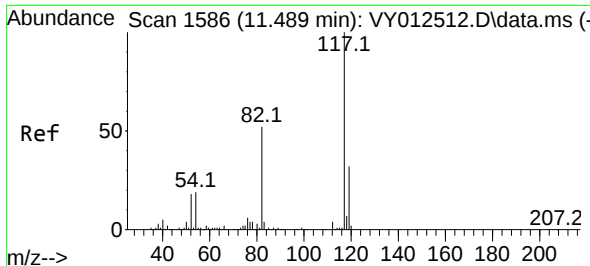

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.490 min Scan# 11
Delta R.T. 0.000 min
Lab File: VY012550.D
Acq: 08 Feb 2023 18:09

Instrument :
MSVOA_Y
ClientSampleId :
JPP-46-020723

Tgt Ion:117 Resp: 233614
Ion Ratio Lower Upper
117 100
82 52.2 41.7 62.5
119 33.3 25.8 38.8

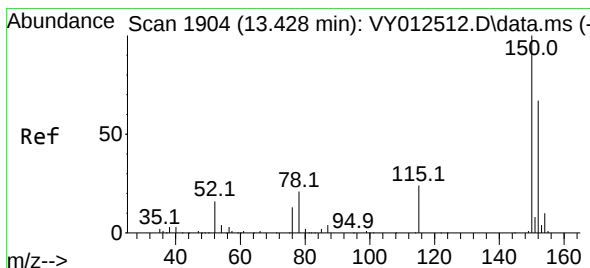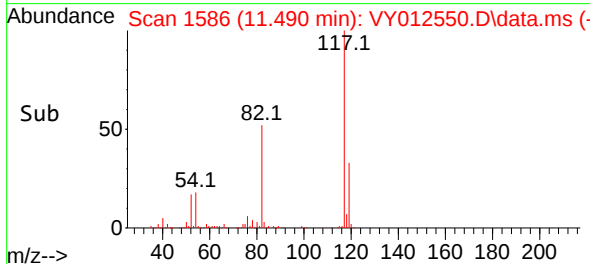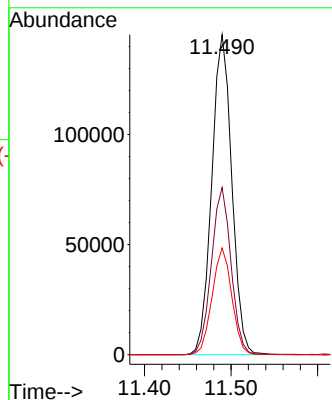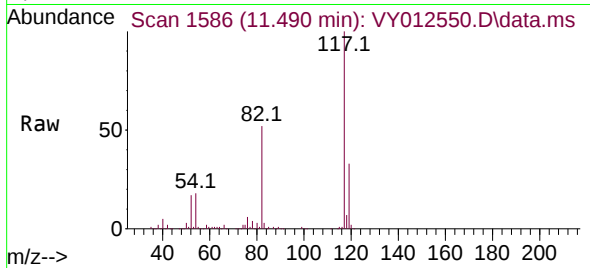

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.422 min Scan# 1903
Delta R.T. -0.006 min
Lab File: VY012550.D
Acq: 08 Feb 2023 18:09

Tgt Ion:152 Resp: 102425
Ion Ratio Lower Upper
152 100
115 55.7 28.1 84.3
150 156.1 0.0 351.0

