

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY020923\
 Data File : VY012565.D
 Acq On : 09 Feb 2023 14:45
 Operator : KP/MD
 Sample : 01513-01
 Misc : 5.06g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VNJ-208

Quant Time: Feb 10 05:59:05 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y020723S.M
 Quant Title : SW846 8260
 QLast Update : Wed Feb 08 01:09:03 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.789	168	141728	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.691	114	239775	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.490	117	239307	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	112579	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.143	65	83758	46.474	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	92.940%
35) Dibromofluoromethane	7.716	113	71896	41.173	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	82.340%
50) Toluene-d8	10.179	98	285829	39.326	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	78.660%
62) 4-Bromofluorobenzene	12.483	95	94805	37.396	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	74.800%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY020923\
Data File : VY012565.D
Acq On : 09 Feb 2023 14:45
Operator : KP/MD
Sample : 01513-01
Misc : 5.06g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VNJ-208

Quant Time: Feb 10 05:59:05 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y020723S.M
Quant Title : SW846 8260
QLast Update : Wed Feb 08 01:09:03 2023
Response via : Initial Calibration




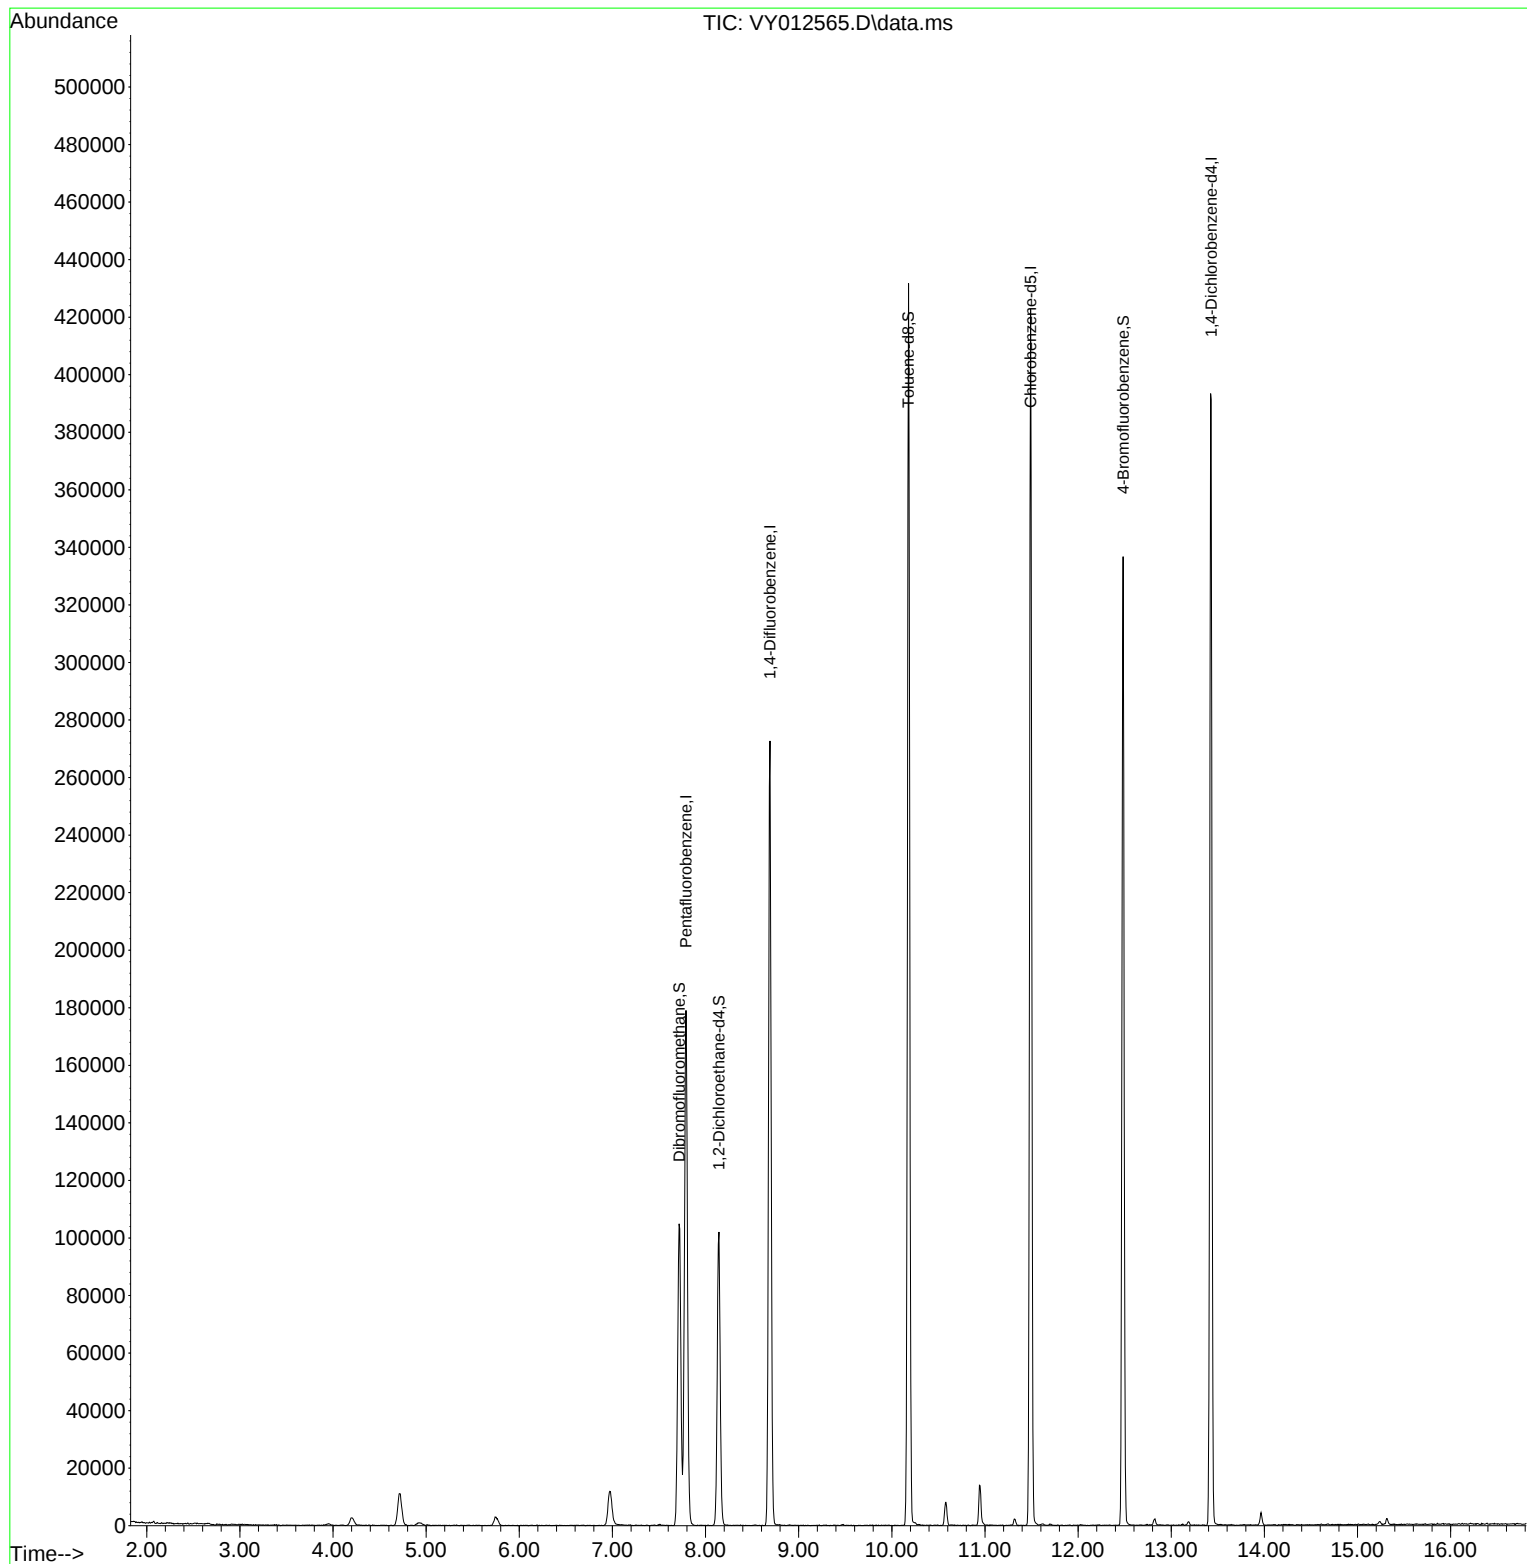


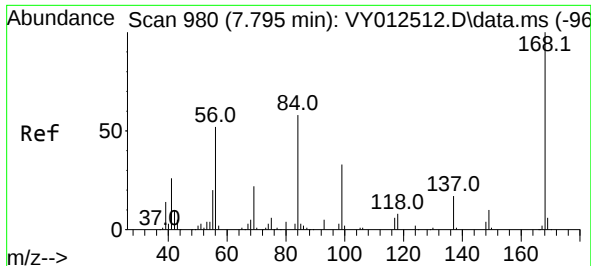

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. -0.006 min
Lab File: VY012565.D
Acq: 09 Feb 2023 14:45




Instrument :
MSVOA_Y
ClientSampleId :
VNJ-208


Tgt Ion:168 Resp: 141728
Ion Ratio Lower Upper
168 100
99 53.3 40.8 61.2

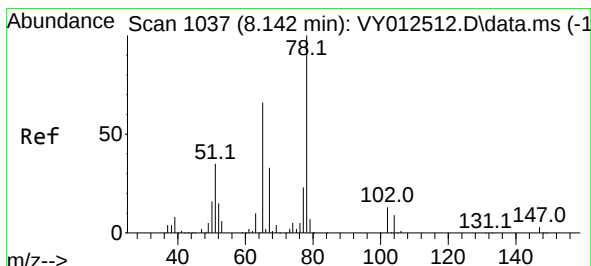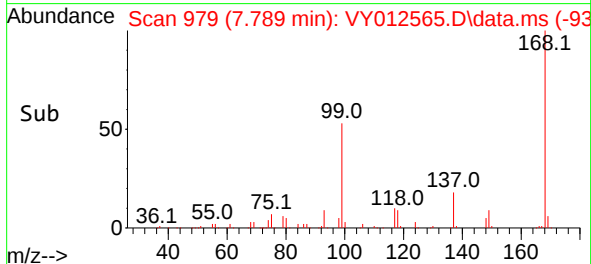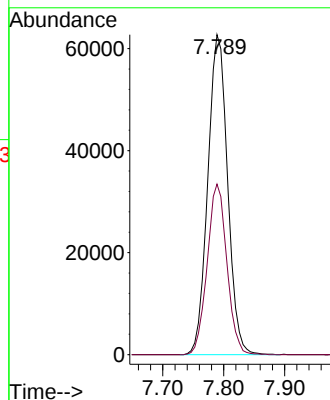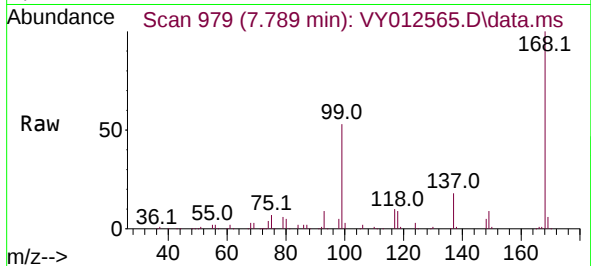

#33
1,2-Dichloroethane-d4
Concen: 46.474 ug/l
RT: 8.143 min Scan# 1037
Delta R.T. 0.000 min
Lab File: VY012565.D
Acq: 09 Feb 2023 14:45

Tgt Ion: 65 Resp: 83758
Ion Ratio Lower Upper
65 100
67 49.4 0.0 98.6

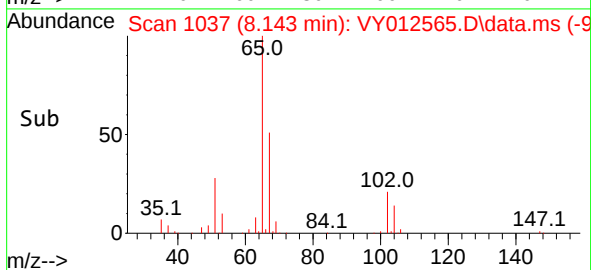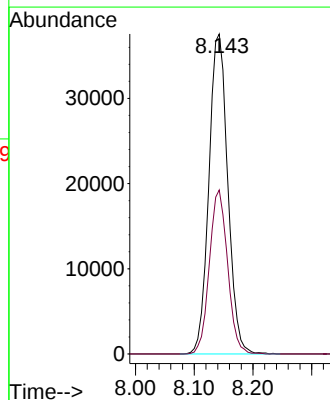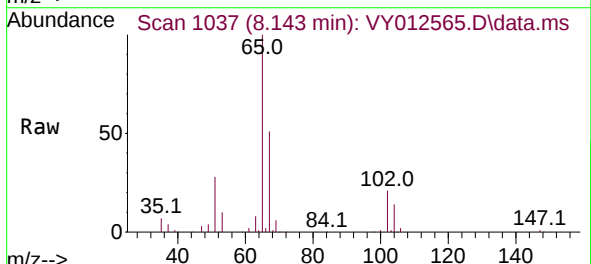

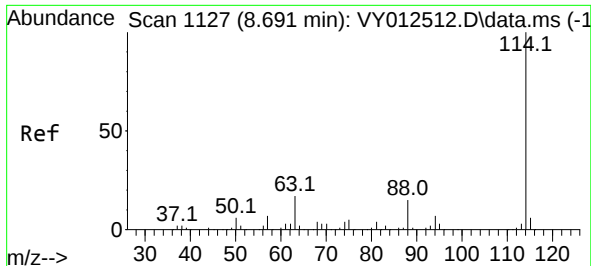

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.691 min Scan# 1127

Delta R.T. 0.000 min

Lab File: VY012565.D

Acq: 09 Feb 2023 14:45

Instrument :

MSVOA_Y

ClientSampleId :

VNJ-208





Tgt Ion:114 Resp: 239775

Ion Ratio Lower Upper

114 100

63 16.9 0.0 33.6

88 14.1 0.0 29.8

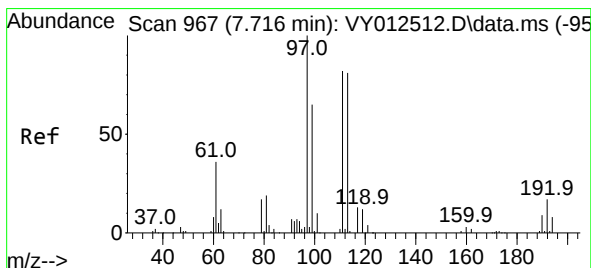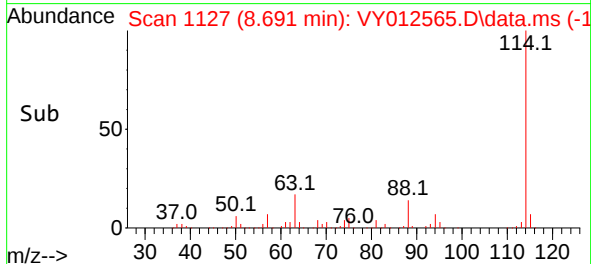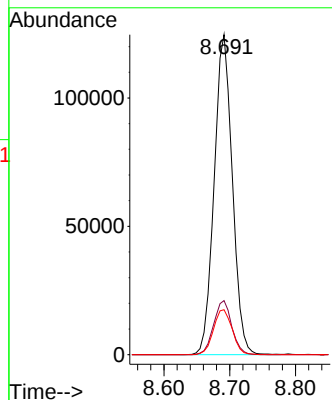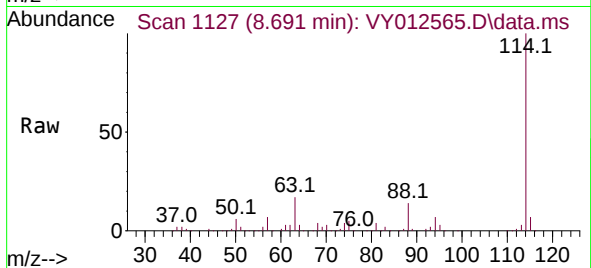

#35

Dibromofluoromethane

Concen: 41.173 ug/l

RT: 7.716 min Scan# 967

Delta R.T. 0.000 min

Lab File: VY012565.D

Acq: 09 Feb 2023 14:45




Tgt Ion:113 Resp: 71896


Ion Ratio Lower Upper

113 100

111 101.8 81.9 122.9

192 22.4 17.5 26.3


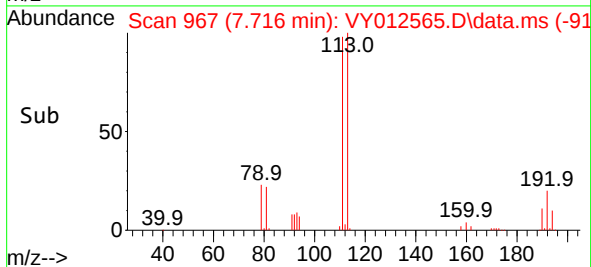
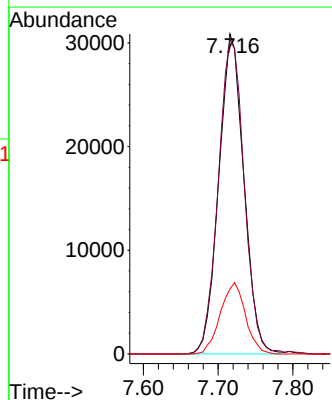
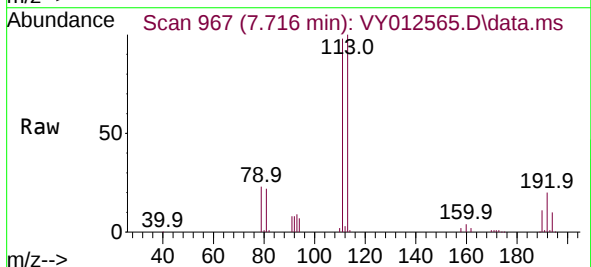


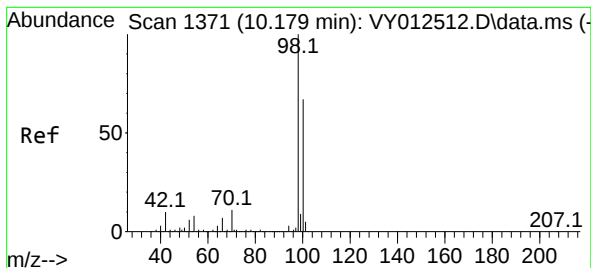

#50
Toluene-d8
Concen: 39.326 ug/l
RT: 10.179 min Scan# 1371
Delta R.T. 0.000 min
Lab File: VY012565.D
Acq: 09 Feb 2023 14:45




Instrument :
MSVOA_Y
ClientSampleId :
VNJ-208


Tgt Ion: 98 Resp: 285829
Ion Ratio Lower Upper
98 100
100 64.9 52.2 78.2

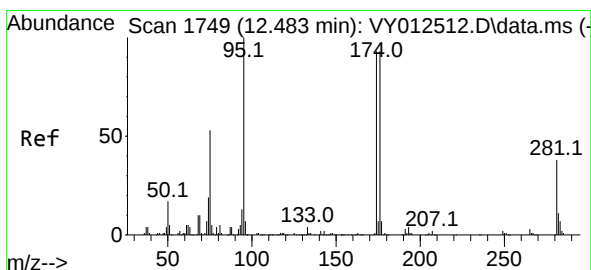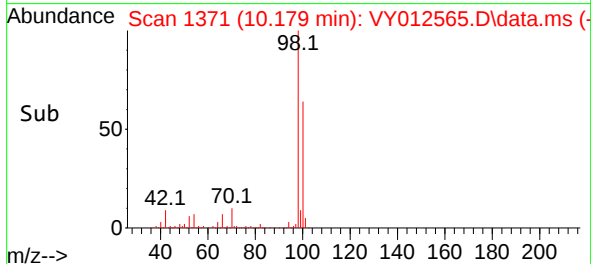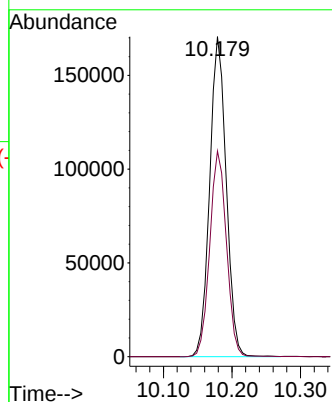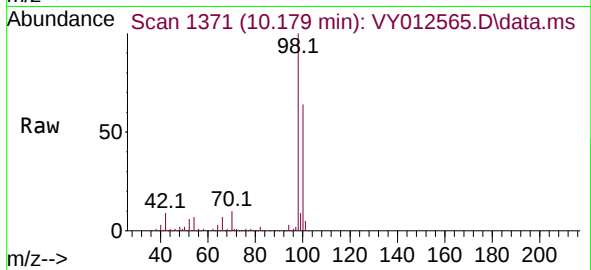

#62
4-Bromofluorobenzene
Concen: 37.396 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.000 min
Lab File: VY012565.D
Acq: 09 Feb 2023 14:45

Tgt Ion: 95 Resp: 94805
Ion Ratio Lower Upper
95 100
174 98.1 0.0 188.0
176 94.7 0.0 183.6

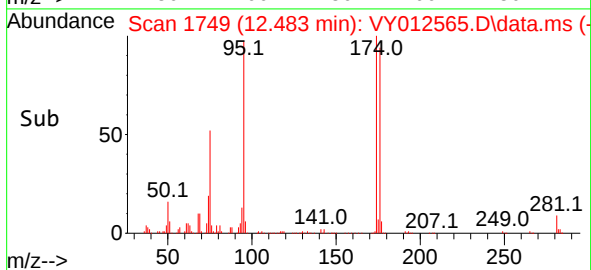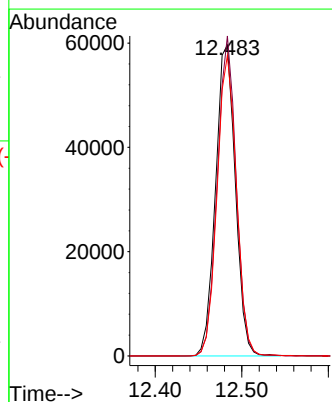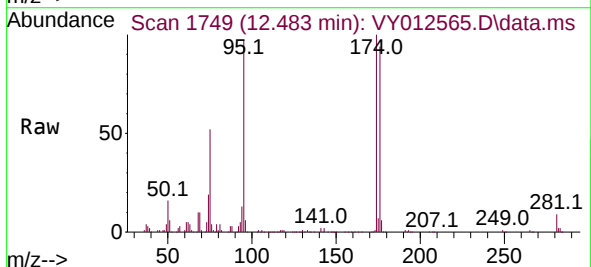

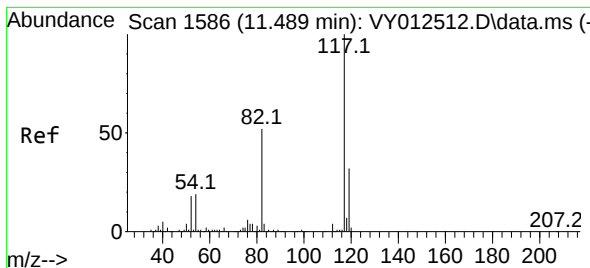

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.490 min Scan# 11

Delta R.T. 0.000 min

Lab File: VY012565.D

Acq: 09 Feb 2023 14:45

Instrument :

MSVOA_Y

ClientSampleId :

VNJ-208





Tgt Ion:117 Resp: 239307

Ion Ratio Lower Upper

117 100

82 50.4 41.7 62.5

119 32.6 25.8 38.8

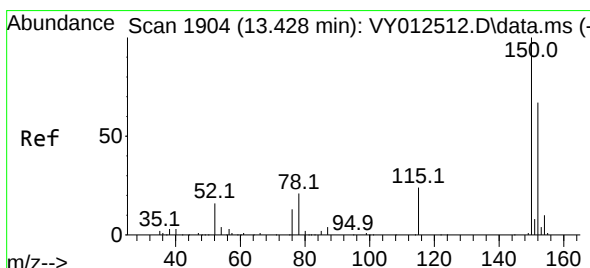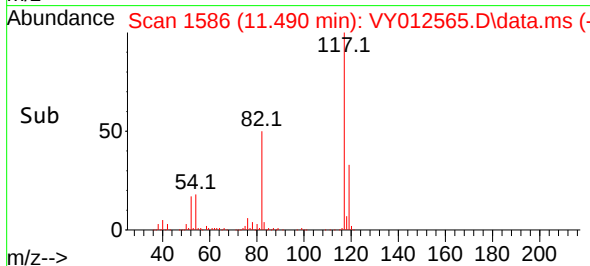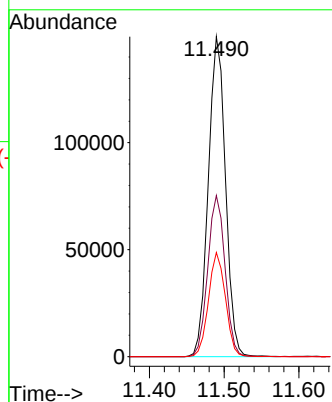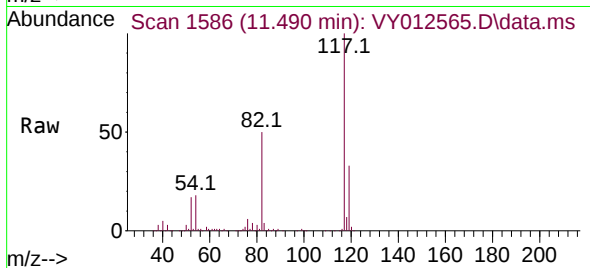

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.428 min Scan# 1904

Delta R.T. 0.000 min

Lab File: VY012565.D

Acq: 09 Feb 2023 14:45

Tgt Ion:152 Resp: 112579

Ion Ratio Lower Upper

152 100

115 55.8 28.1 84.3

150 156.3 0.0 351.0

