


Data Path : Z:\VOASRV\HPCHEM1\MSVOA Y\DATA\VY021120\
 Data File : VY001591.D
 Acq On : 11 Feb 2020 09:52
 Operator : SY/MD
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y020420S.M
 Title : SW846 8260
 Last Update : Tue Feb 04 15:10:08 2020

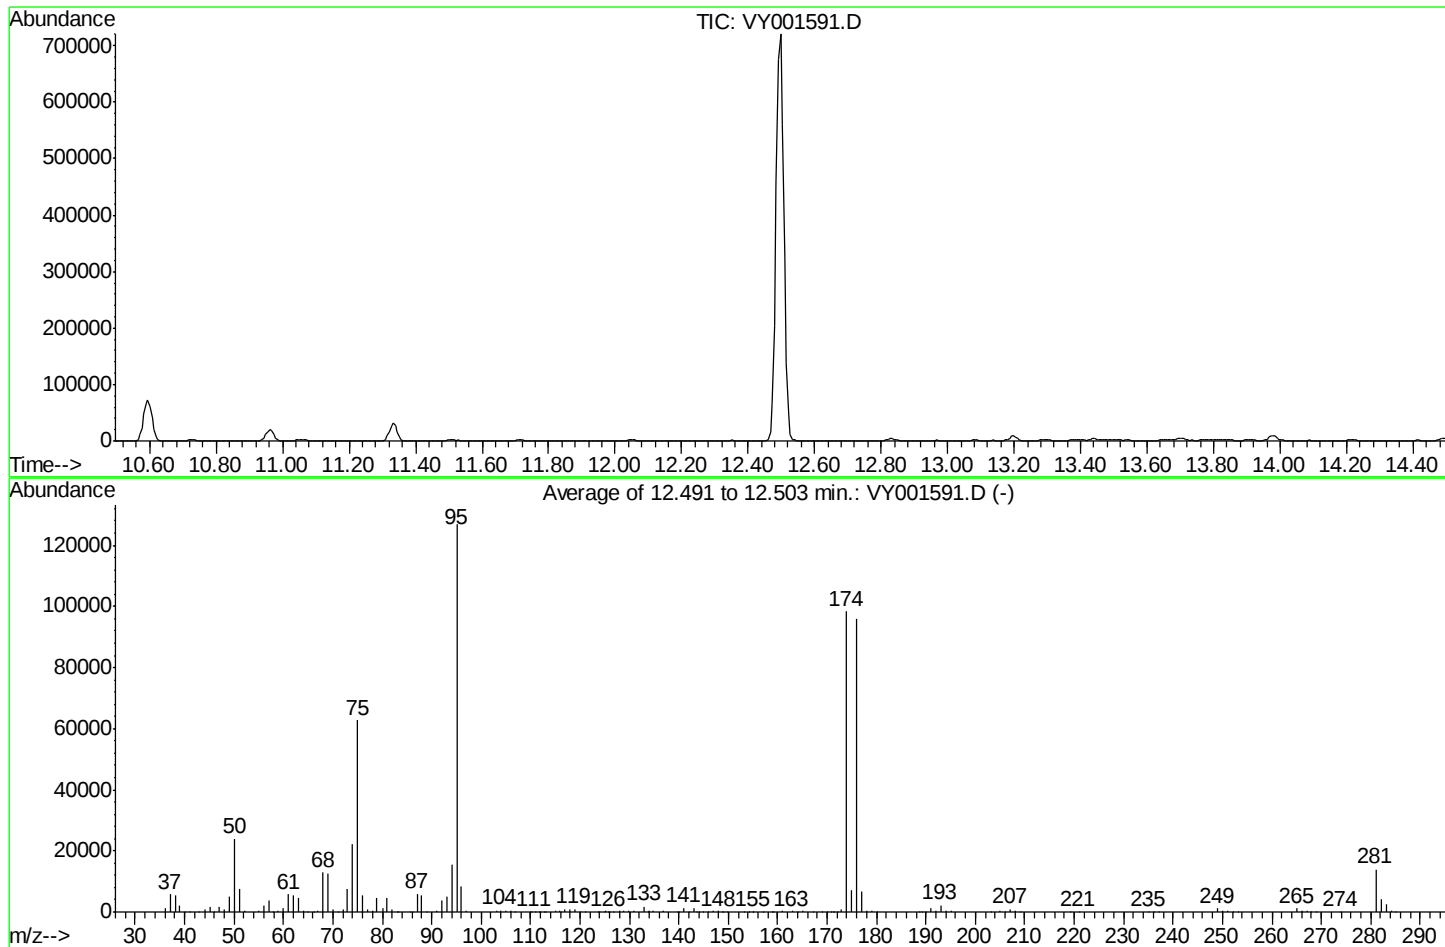

AutoFind: Scans 1764, 1765, 1766; Background Corrected with Scan 1755

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.0	24080	PASS
75	95	30	60	49.4	62717	PASS
95	95	100	100	100.0	126874	PASS
96	95	5	9	6.7	8516	PASS
173	174	0.00	2	0.7	714	PASS
174	95	50	100	77.5	98378	PASS
175	174	5	9	7.2	7085	PASS
176	174	95	101	97.7	96146	PASS
177	176	5	9	6.9	6622	PASS