
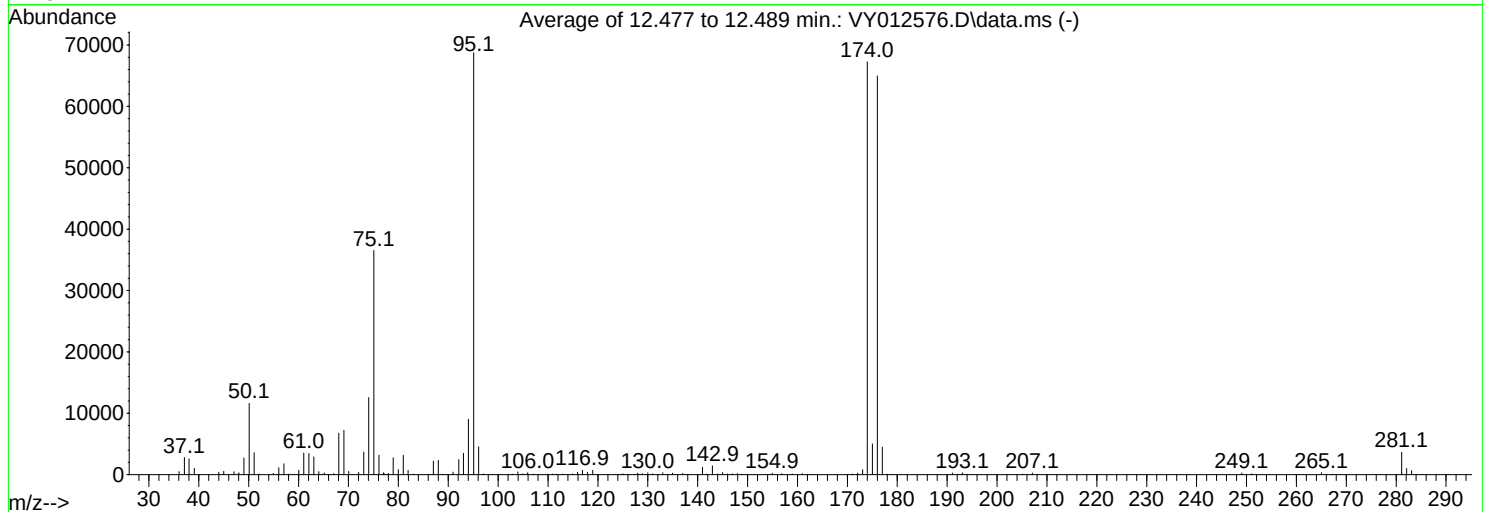


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY021423\
 Data File : VY012576.D
 Acq On : 14 Feb 2023 09:19
 Operator : KP/MD
 Sample : BFB
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y020723S.M
 Title : SW846 8260
 Last Update : Wed Feb 08 01:09:03 2023

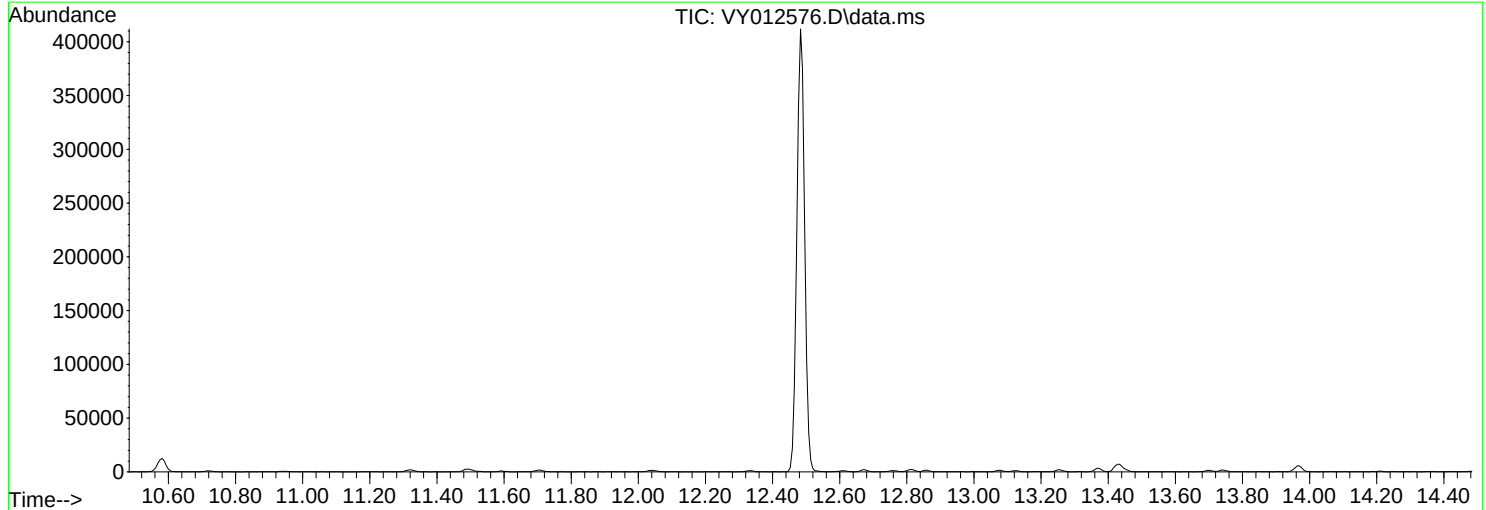

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.9	11634	PASS
75	95	30	60	53.1	36523	PASS
95	95	100	100	100.0	68725	PASS
96	95	5	9	6.6	4524	PASS
173	174	0.00	2	1.2	822	PASS
174	95	50	100	97.9	67251	PASS
175	174	5	9	7.4	5001	PASS
176	174	95	101	96.6	64963	PASS
177	176	5	9	6.9	4485	PASS