

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY021523\
 Data File : VY012619.D
 Acq On : 15 Feb 2023 17:11
 Operator : KP/MD
 Sample : 01559-02
 Misc : 5.05g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BP-VPB-RW10-GW-783-785

Quant Time: Feb 16 01:00:10 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y020723S.M
 Quant Title : SW846 8260
 QLast Update : Wed Feb 08 01:09:03 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.783	168	184668	50.000	ug/l	-0.01
34) 1,4-Difluorobenzene	8.685	114	308811	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.490	117	312187	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.422	152	152519	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.136	65	99885	42.535	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	85.080%
35) Dibromofluoromethane	7.710	113	91804	40.821	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	81.640%
50) Toluene-d8	10.179	98	365042	38.997	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	78.000%
62) 4-Bromofluorobenzene	12.477	95	132964	40.723	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	81.440%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY021523\
Data File : VY012619.D
Acq On : 15 Feb 2023 17:11
Operator : KP/MD
Sample : 01559-02
Misc : 5.05g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BP-VPB-RW10-GW-783-785

Quant Time: Feb 16 01:00:10 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y020723S.M
Quant Title : SW846 8260
QLast Update : Wed Feb 08 01:09:03 2023
Response via : Initial Calibration




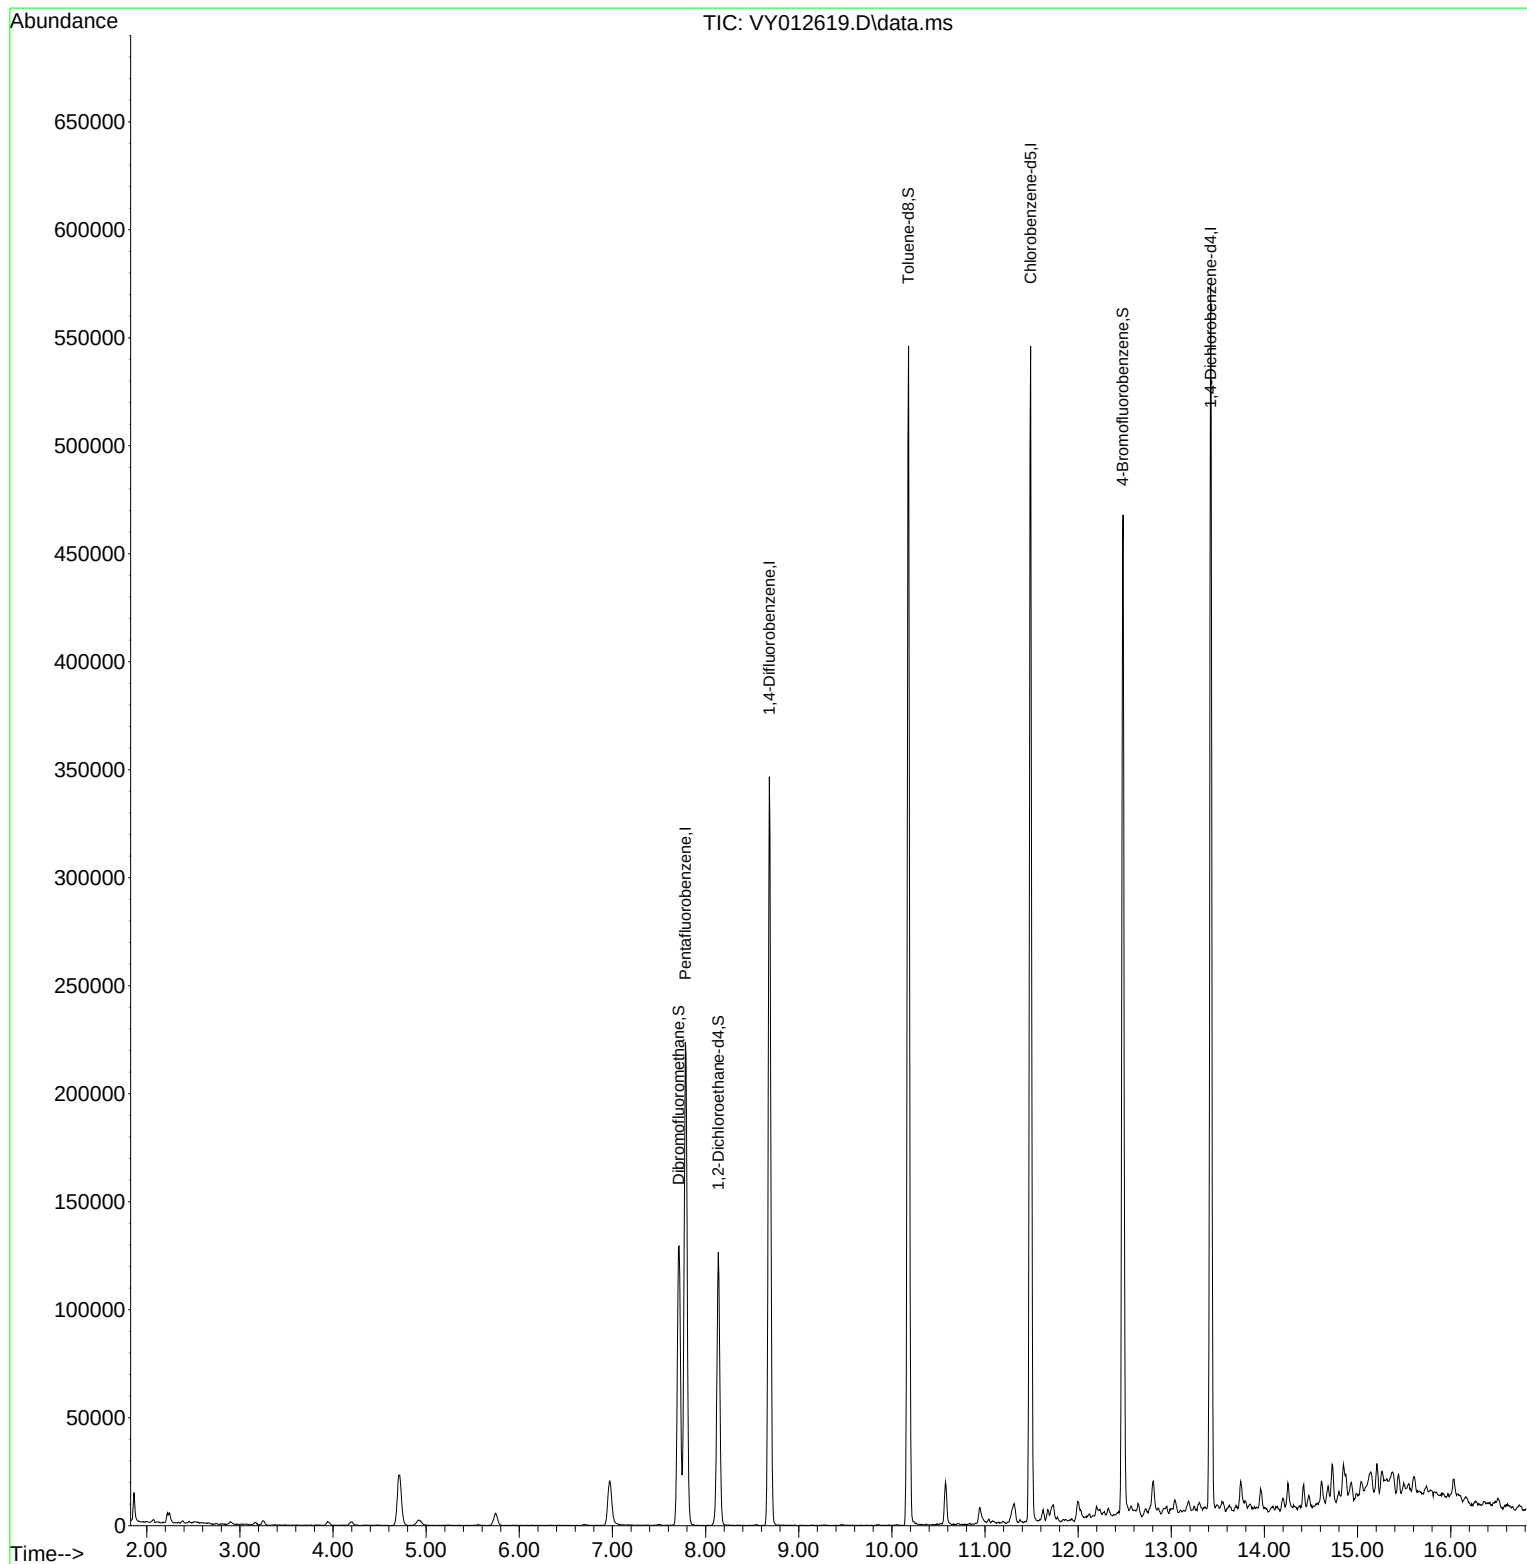


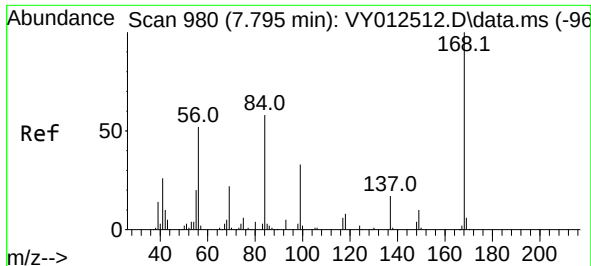

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.783 min Scan# 91
Delta R.T. -0.012 min
Lab File: VY012619.D
Acq: 15 Feb 2023 17:11




Instrument :
MSVOA_Y
ClientSampleId :
BP-VPB-RW10-GW-783-785


Tgt Ion:168 Resp: 184668
Ion Ratio Lower Upper
168 100
99 51.8 40.8 61.2

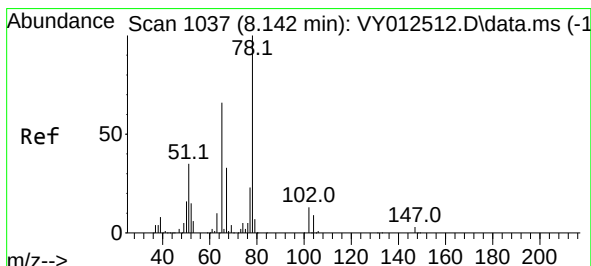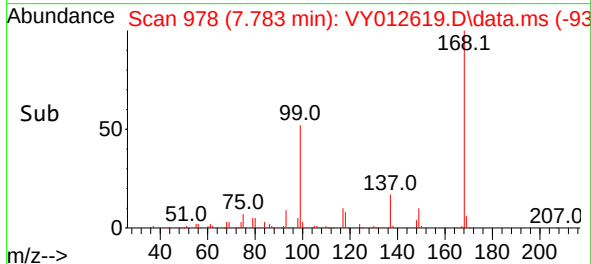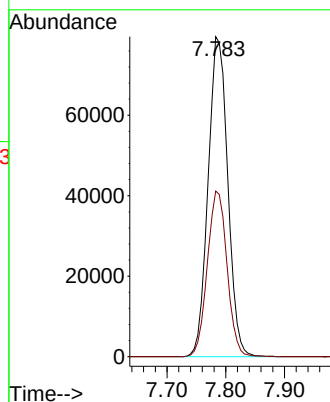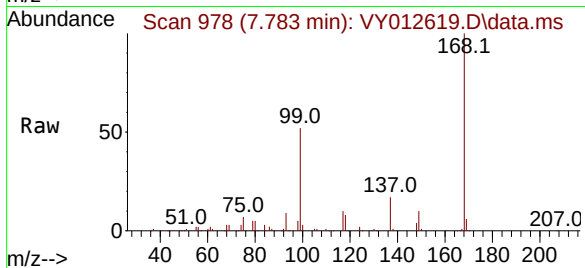

#33
1,2-Dichloroethane-d4
Concen: 42.535 ug/l
RT: 8.136 min Scan# 1036
Delta R.T. -0.006 min
Lab File: VY012619.D
Acq: 15 Feb 2023 17:11

Tgt Ion: 65 Resp: 99885
Ion Ratio Lower Upper
65 100
67 50.8 0.0 98.6

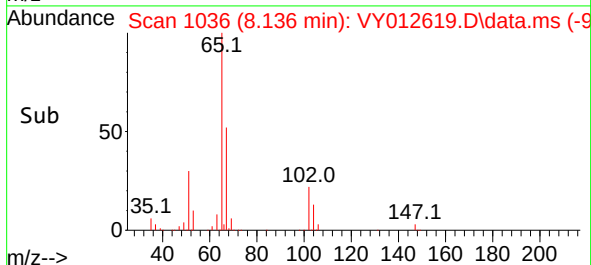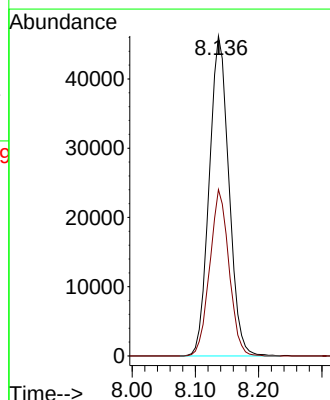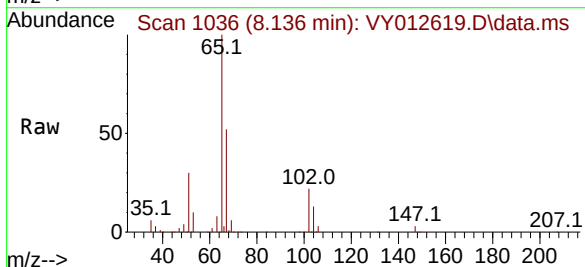

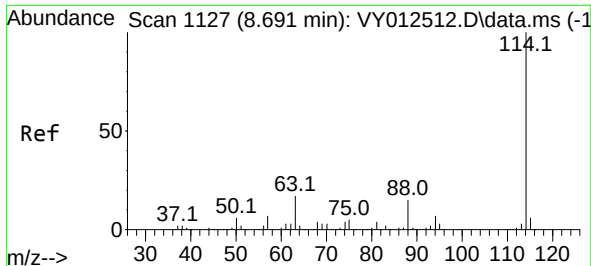

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.685 min Scan# 1126

Delta R.T. -0.006 min

Lab File: VY012619.D

Acq: 15 Feb 2023 17:11

Instrument :

MSVOA_Y

ClientSampleId :

BP-VPB-RW10-GW-783-785





Tgt Ion:114 Resp: 308811

Ion Ratio Lower Upper

114 100

63 16.9 0.0 33.6

88 15.3 0.0 29.8

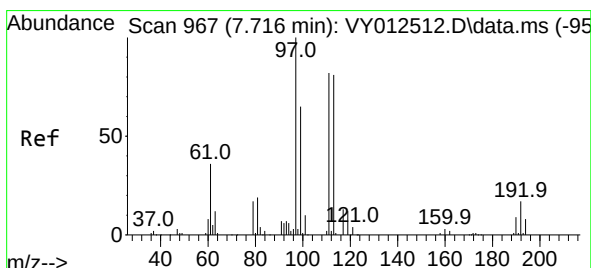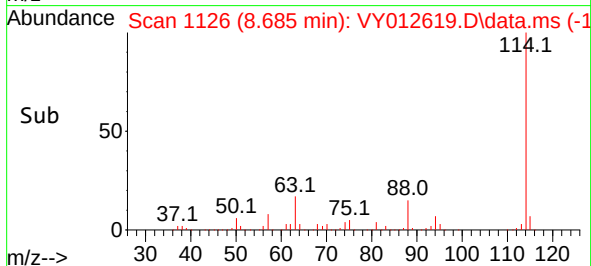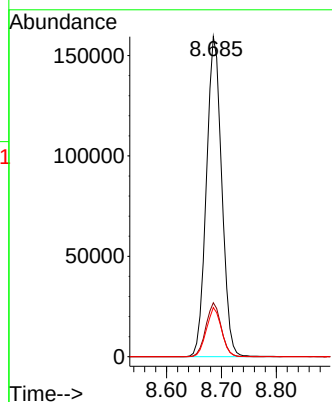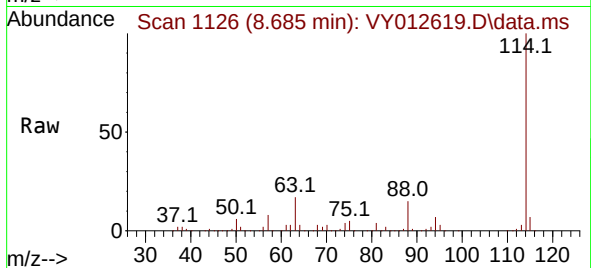

#35

Dibromofluoromethane

Concen: 40.821 ug/l

RT: 7.710 min Scan# 966

Delta R.T. -0.006 min

Lab File: VY012619.D

Acq: 15 Feb 2023 17:11




Tgt Ion:113 Resp: 91804


Ion Ratio Lower Upper

113 100

111 103.1 81.9 122.9

192 22.8 17.5 26.3


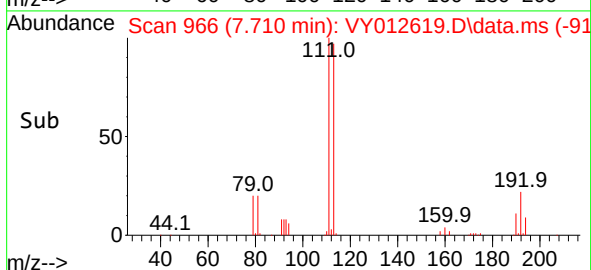
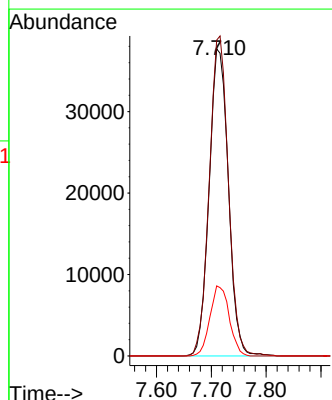
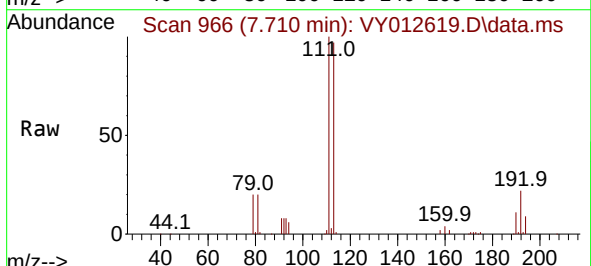


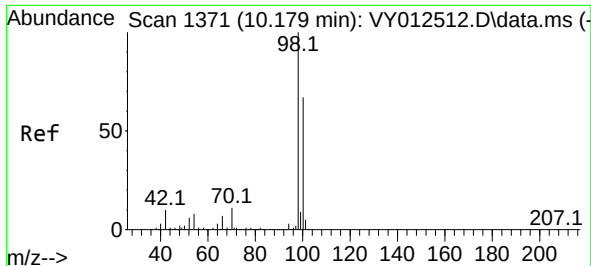

#50
Toluene-d8
Concen: 38.997 ug/l
RT: 10.179 min Scan# 1371
Delta R.T. 0.000 min
Lab File: VY012619.D
Acq: 15 Feb 2023 17:11




Instrument :
MSVOA_Y
ClientSampleId :
BP-VPB-RW10-GW-783-785


Tgt Ion: 98 Resp: 365042
Ion Ratio Lower Upper
98 100
100 64.9 52.2 78.2

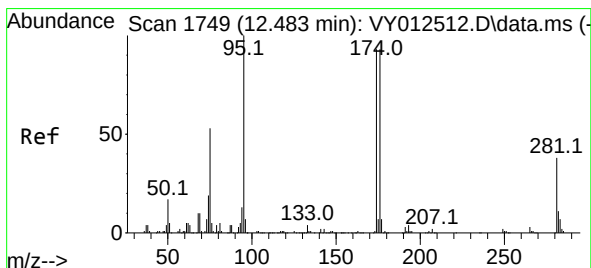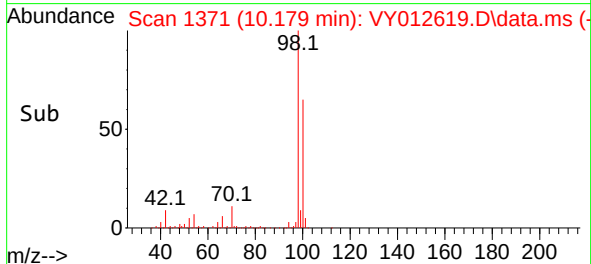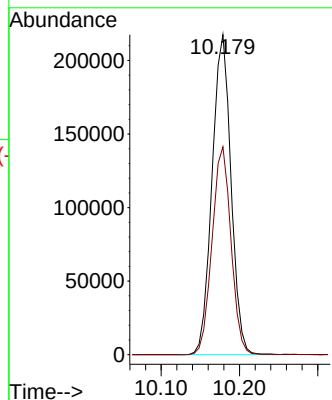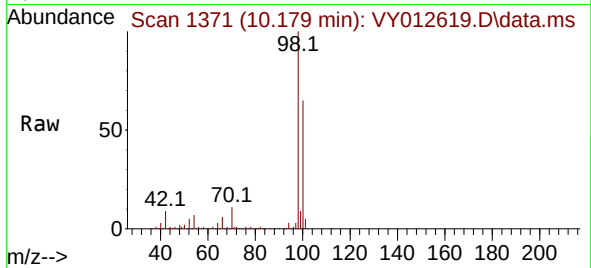

#62
4-Bromofluorobenzene
Concen: 40.723 ug/l
RT: 12.477 min Scan# 1748
Delta R.T. -0.006 min
Lab File: VY012619.D
Acq: 15 Feb 2023 17:11

Tgt Ion: 95 Resp: 132964
Ion Ratio Lower Upper
95 100
174 94.4 0.0 188.0
176 91.4 0.0 183.6


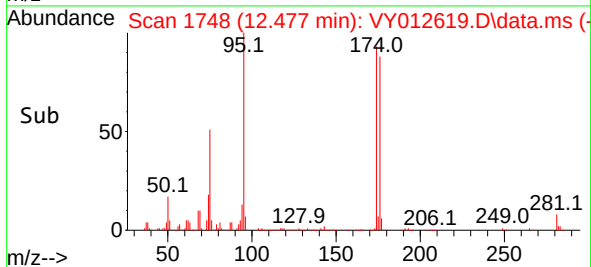
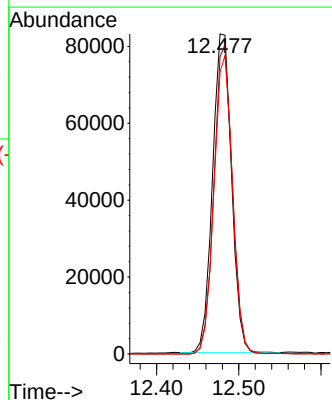
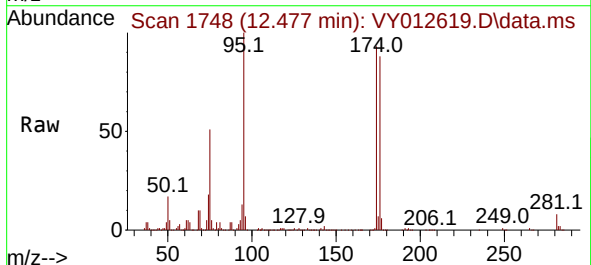


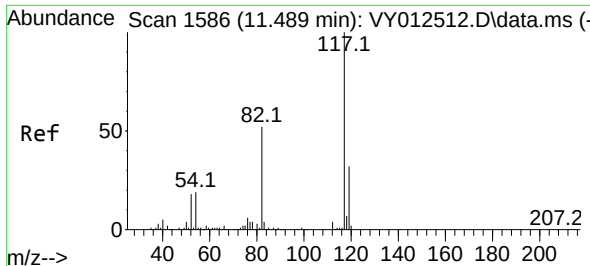

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.490 min Scan# 11
Delta R.T. 0.000 min
Lab File: VY012619.D
Acq: 15 Feb 2023 17:11

Instrument :
MSVOA_Y
ClientSampleId :
BP-VPB-RW10-GW-783-785

Tgt Ion:117 Resp: 312187
Ion Ratio Lower Upper
117 100
82 50.2 41.7 62.5
119 33.0 25.8 38.8

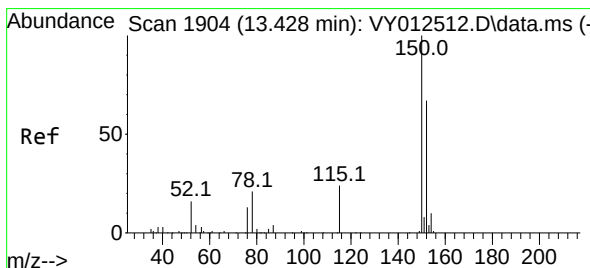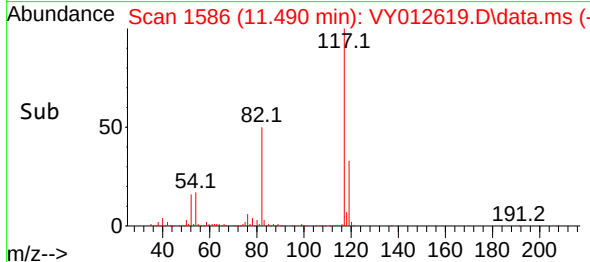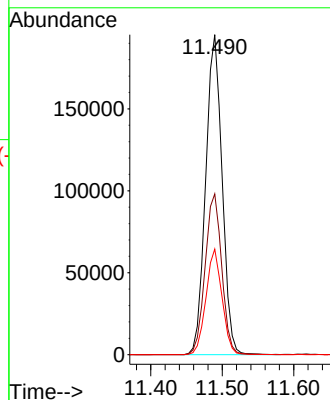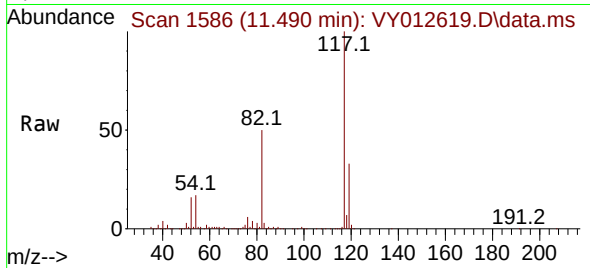

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.422 min Scan# 1903
Delta R.T. -0.006 min
Lab File: VY012619.D
Acq: 15 Feb 2023 17:11

Tgt Ion:152 Resp: 152519
Ion Ratio Lower Upper
152 100
115 57.6 28.1 84.3
150 157.2 0.0 351.0

