
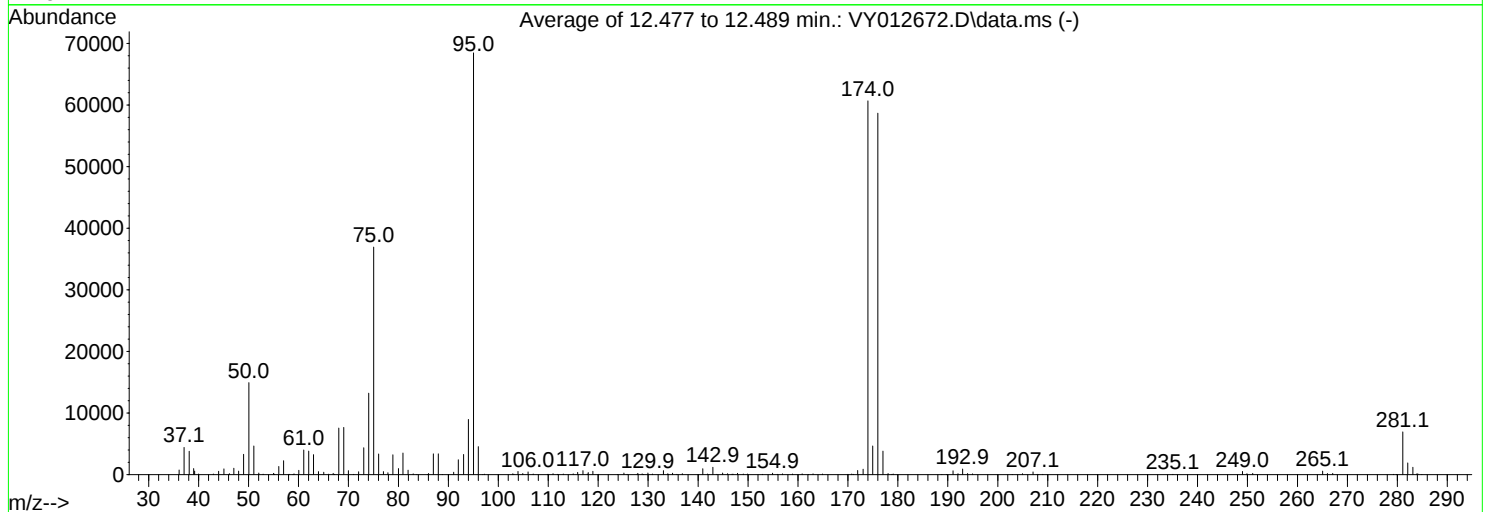


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY022123\
Data File : VY012672.D
Acq On : 21 Feb 2023 13:15
Operator : KP/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y022123S.M
Title : SW846 8260
Last Update : Wed Feb 22 01:21:05 2023

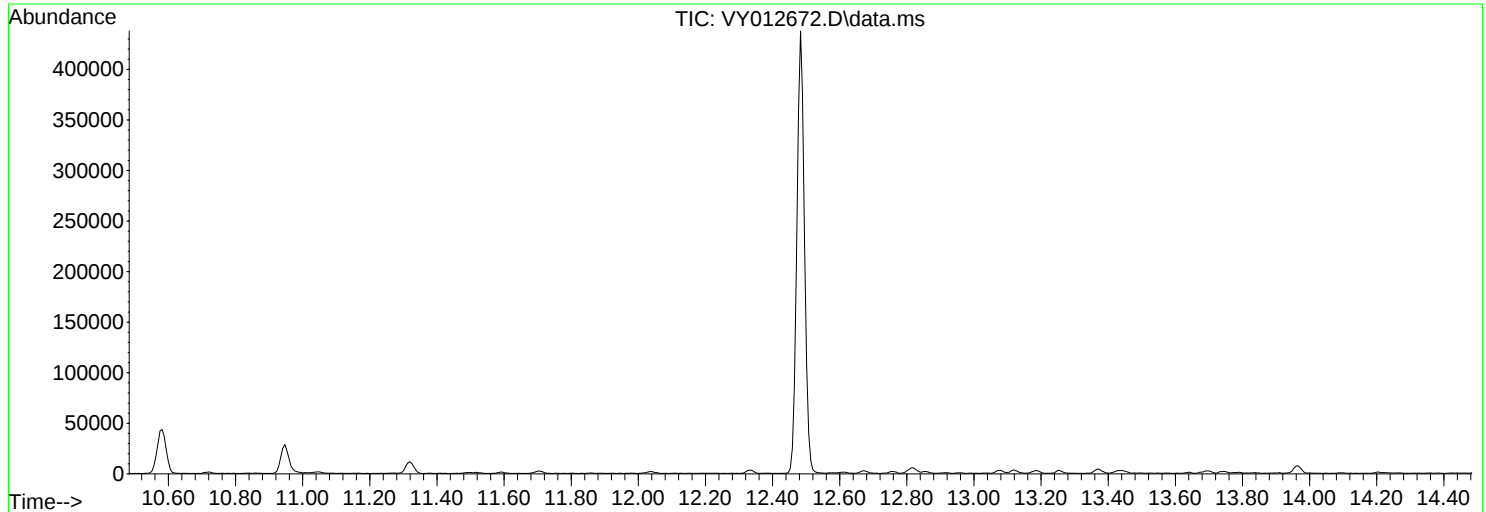

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	21.8	14940	PASS
75	95	30	60	53.9	36947	PASS
95	95	100	100	100.0	68485	PASS
96	95	5	9	6.7	4563	PASS
173	174	0.00	2	1.5	899	PASS
174	95	50	100	88.6	60688	PASS
175	174	5	9	7.7	4644	PASS
176	174	95	101	96.7	58685	PASS
177	176	5	9	6.5	3808	PASS